

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
 Data File : BM003892.D
 Acq On : 30 Dec 2015 22:29
 Operator : SJ/UM
 Sample : G4868-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43N2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	5	8	11	rBV	3570	3644	0.33%	0.032%
2	3.169	11	14	21	rVB	11346	13211	1.20%	0.117%
3	5.187	354	357	360	rBB	1244	1327	0.12%	0.012%
4	5.257	366	369	371	rBB	1187	1379	0.12%	0.012%
5	6.851	634	640	648	rBB	65350	97062	8.79%	0.863%
6	7.004	661	666	677	rBB	164548	254534	23.04%	2.262%
7	7.204	694	700	708	rBV	196749	299533	27.12%	2.662%
8	7.263	708	710	714	rVB	2179	2809	0.25%	0.025%
9	7.669	773	779	787	rBB	181122	275911	24.98%	2.452%
10	7.734	787	790	794	rBB	3098	3493	0.32%	0.031%
11	8.039	839	842	846	rBB	2099	2775	0.25%	0.025%
12	8.386	895	901	911	rBB	178398	279674	25.32%	2.485%
13	8.828	970	976	986	rBB	197432	314451	28.47%	2.794%
14	9.545	1093	1098	1106	rBB	165493	268169	24.28%	2.383%
15	10.086	1184	1190	1201	rBB	269674	434934	39.37%	3.865%
16	10.457	1246	1253	1259	rBV	259519	422212	38.22%	3.752%
17	10.510	1259	1262	1268	rVB	15707	21857	1.98%	0.194%
18	10.604	1273	1278	1285	rBB	11216	17328	1.57%	0.154%
19	11.369	1404	1408	1415	rBB	9313	17960	1.63%	0.160%
20	12.057	1521	1525	1529	rBB	2952	4187	0.38%	0.037%
21	12.133	1534	1538	1541	rBB	2996	4221	0.38%	0.038%
22	12.351	1572	1575	1579	rBB	2171	2640	0.24%	0.023%
23	12.745	1640	1642	1647	rBB	1314	1334	0.12%	0.012%
24	13.739	1804	1811	1819	rBB	488900	675230	61.13%	6.000%
25	14.015	1852	1858	1865	rBV	565777	816546	73.92%	7.256%
26	14.168	1876	1884	1895	rBB	7169	14280	1.29%	0.127%
27	14.327	1905	1911	1918	rBB2	363712	539209	48.81%	4.792%
28	14.392	1919	1922	1924	rBB	1610	1569	0.14%	0.014%
29	14.551	1944	1949	1960	rBV	41373	66426	6.01%	0.590%
30	15.321	2074	2080	2087	rBV	723921	1018645	92.22%	9.052%
31	15.380	2087	2090	2092	rVB	1160	1460	0.13%	0.013%
32	15.451	2097	2102	2110	rBB	206223	262174	23.73%	2.330%
33	15.557	2117	2120	2124	rBB	4575	5916	0.54%	0.053%
34	16.862	2339	2342	2345	rBB	868	1157	0.10%	0.010%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003892.D
Acq On : 30 Dec 2015 22:29
Operator : SJ/UM
Sample : G4868-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43N2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION

35	17.074	2372	2378	2384	rBV2	410046	573532	51.92%	5.097%
36	17.115	2384	2385	2388	rVV	3319	2805	0.25%	0.025%
37	17.174	2388	2395	2412	rVB	745762	1037677	93.94%	9.221%
38	19.109	2721	2724	2728	rBV	6492	7109	0.64%	0.063%
39	19.368	2764	2768	2772	rVB	4736	5834	0.53%	0.052%
40	19.480	2780	2787	2794	rBV	809755	1104625	100.00%	9.816%
41	19.633	2809	2813	2815	rBV2	978	1145	0.10%	0.010%
42	20.127	2894	2897	2900	rBV3	716	1349	0.12%	0.012%
43	20.409	2941	2945	2950	rBV2	2726	2966	0.27%	0.026%
44	20.462	2950	2954	2955	rBV	1030	1175	0.11%	0.010%
45	20.633	2978	2983	2987	rBV2	5101	6231	0.56%	0.055%
46	20.703	2992	2995	2997	rBV3	1166	1300	0.12%	0.012%
47	20.762	3002	3005	3009	rVB2	2066	2896	0.26%	0.026%
48	20.844	3016	3019	3021	rBV3	1485	1579	0.14%	0.014%
49	20.986	3040	3043	3044	rBV2	1627	1763	0.16%	0.016%
50	21.003	3044	3046	3048	rVB3	1875	1422	0.13%	0.013%
51	21.056	3051	3055	3059	rVB2	4248	5904	0.53%	0.052%
52	21.274	3087	3092	3099	rBV	464687	589667	53.38%	5.240%
53	21.421	3115	3117	3120	rVB3	2698	2637	0.24%	0.023%
54	21.856	3188	3191	3195	rVB3	3818	4787	0.43%	0.043%
55	22.315	3266	3269	3274	rVB2	8574	10226	0.93%	0.091%
56	22.821	3351	3355	3360	rVB2	9863	14137	1.28%	0.126%
57	23.374	3441	3449	3459	rBV	588355	1071353	96.99%	9.520%
58	23.515	3465	3473	3484	rVB	303772	564330	51.09%	5.015%
59	24.021	3555	3559	3569	rVB2	13908	26295	2.38%	0.234%
60	24.756	3678	3684	3693	rVB2	15491	35811	3.24%	0.318%
61	25.621	3826	3831	3839	rVB4	10785	27419	2.48%	0.244%


Sum of corrected areas: 11253231

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003892.D
Acq On : 30 Dec 2015 22:29
Operator : SJ/UM
Sample : G4868-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43N2

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

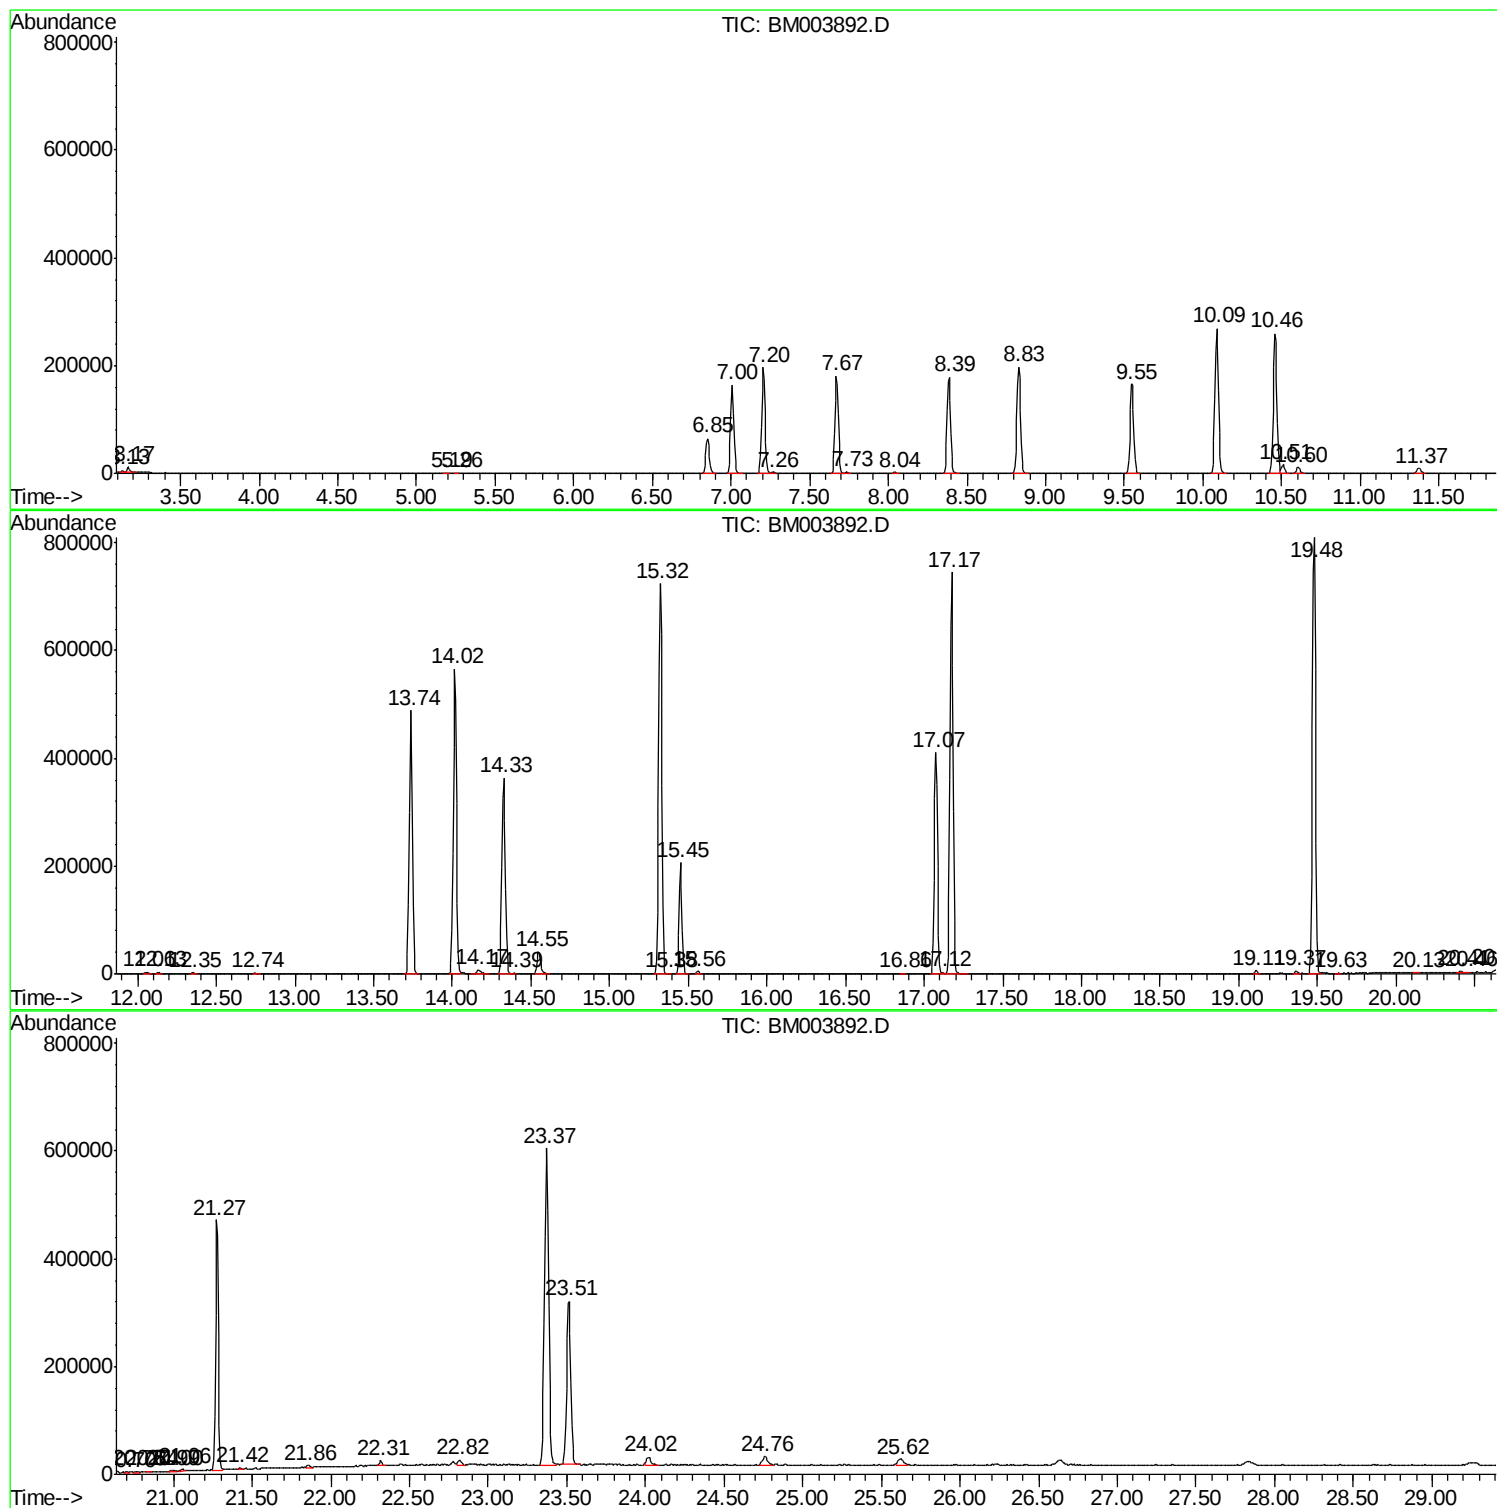

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003892.D
Acq On : 30 Dec 2015 22:29
Operator : SJ/UM
Sample : G4868-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43N2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003892.D
Acq On : 30 Dec 2015 22:29
Operator : SJ/UM
Sample : G4868-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43N2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc