

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
 Data File : BM003901.D
 Acq On : 31 Dec 2015 04:27
 Operator : SJ/UM
 Sample : G4868-17
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43P0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	5	8	13	rVB	3920	4168	0.30%	0.031%
2	4.798	287	291	294	rBB	2149	2746	0.20%	0.020%
3	6.851	634	640	649	rBB	74346	110667	7.88%	0.815%
4	7.004	660	666	678	rBB	220598	341005	24.27%	2.511%
5	7.204	694	700	711	rBB	253071	383095	27.26%	2.821%
6	7.669	773	779	787	rBB	201085	310689	22.11%	2.288%
7	8.386	895	901	911	rBB	206644	332122	23.64%	2.445%
8	8.828	970	976	988	rBB	265150	419503	29.86%	3.089%
9	9.545	1092	1098	1106	rBB	218241	356038	25.34%	2.621%
10	10.086	1184	1190	1204	rBB	331574	546076	38.86%	4.021%
11	10.457	1246	1253	1264	rBB	291658	476774	33.93%	3.510%
12	10.604	1273	1278	1287	rBB	12542	20005	1.42%	0.147%
13	12.057	1521	1525	1530	rBB	3505	5364	0.38%	0.039%
14	13.739	1804	1811	1822	rBB	612006	853087	60.71%	6.281%
15	14.015	1852	1858	1876	rBV	720301	1044134	74.31%	7.688%
16	14.168	1880	1884	1889	rBB	2094	3776	0.27%	0.028%
17	14.327	1905	1911	1918	rBB2	412245	619436	44.08%	4.561%
18	14.545	1944	1948	1960	rBB	39556	65296	4.65%	0.481%
19	15.321	2074	2080	2091	rBB	907411	1292743	92.00%	9.518%
20	15.451	2097	2102	2109	rBV	253315	325727	23.18%	2.398%
21	15.562	2117	2121	2125	rBB	6972	8228	0.59%	0.061%
22	17.074	2372	2378	2388	rBB	484152	667848	47.53%	4.917%
23	17.174	2388	2395	2412	rBV	942221	1314010	93.52%	9.675%
24	19.109	2719	2724	2728	rBV	7849	8772	0.62%	0.065%
25	19.362	2764	2767	2772	rBV	5387	6661	0.47%	0.049%
26	19.480	2780	2787	2794	rBV	1019358	1405120	100.00%	10.346%
27	21.274	3087	3092	3099	rBV	547193	670064	47.69%	4.934%
28	22.315	3265	3269	3274	rBV3	4391	6567	0.47%	0.048%
29	22.774	3343	3347	3351	rBV2	6272	9663	0.69%	0.071%
30	22.815	3351	3354	3358	rVB2	5087	7095	0.50%	0.052%
31	23.368	3440	3448	3462	rBV	701774	1302669	92.71%	9.591%
32	23.509	3464	3472	3484	rVV2	339286	631155	44.92%	4.647%
33	24.015	3555	3558	3566	rVB3	8465	13701	0.98%	0.101%
34	24.756	3678	3684	3689	rBV	8470	17550	1.25%	0.129%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003901.D
Acq On : 31 Dec 2015 04:27
Operator : SJ/UM
Sample : G4868-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43P0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION


Sum of corrected areas: 13581554

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003901.D
Acq On : 31 Dec 2015 04:27
Operator : SJ/UM
Sample : G4868-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43P0

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

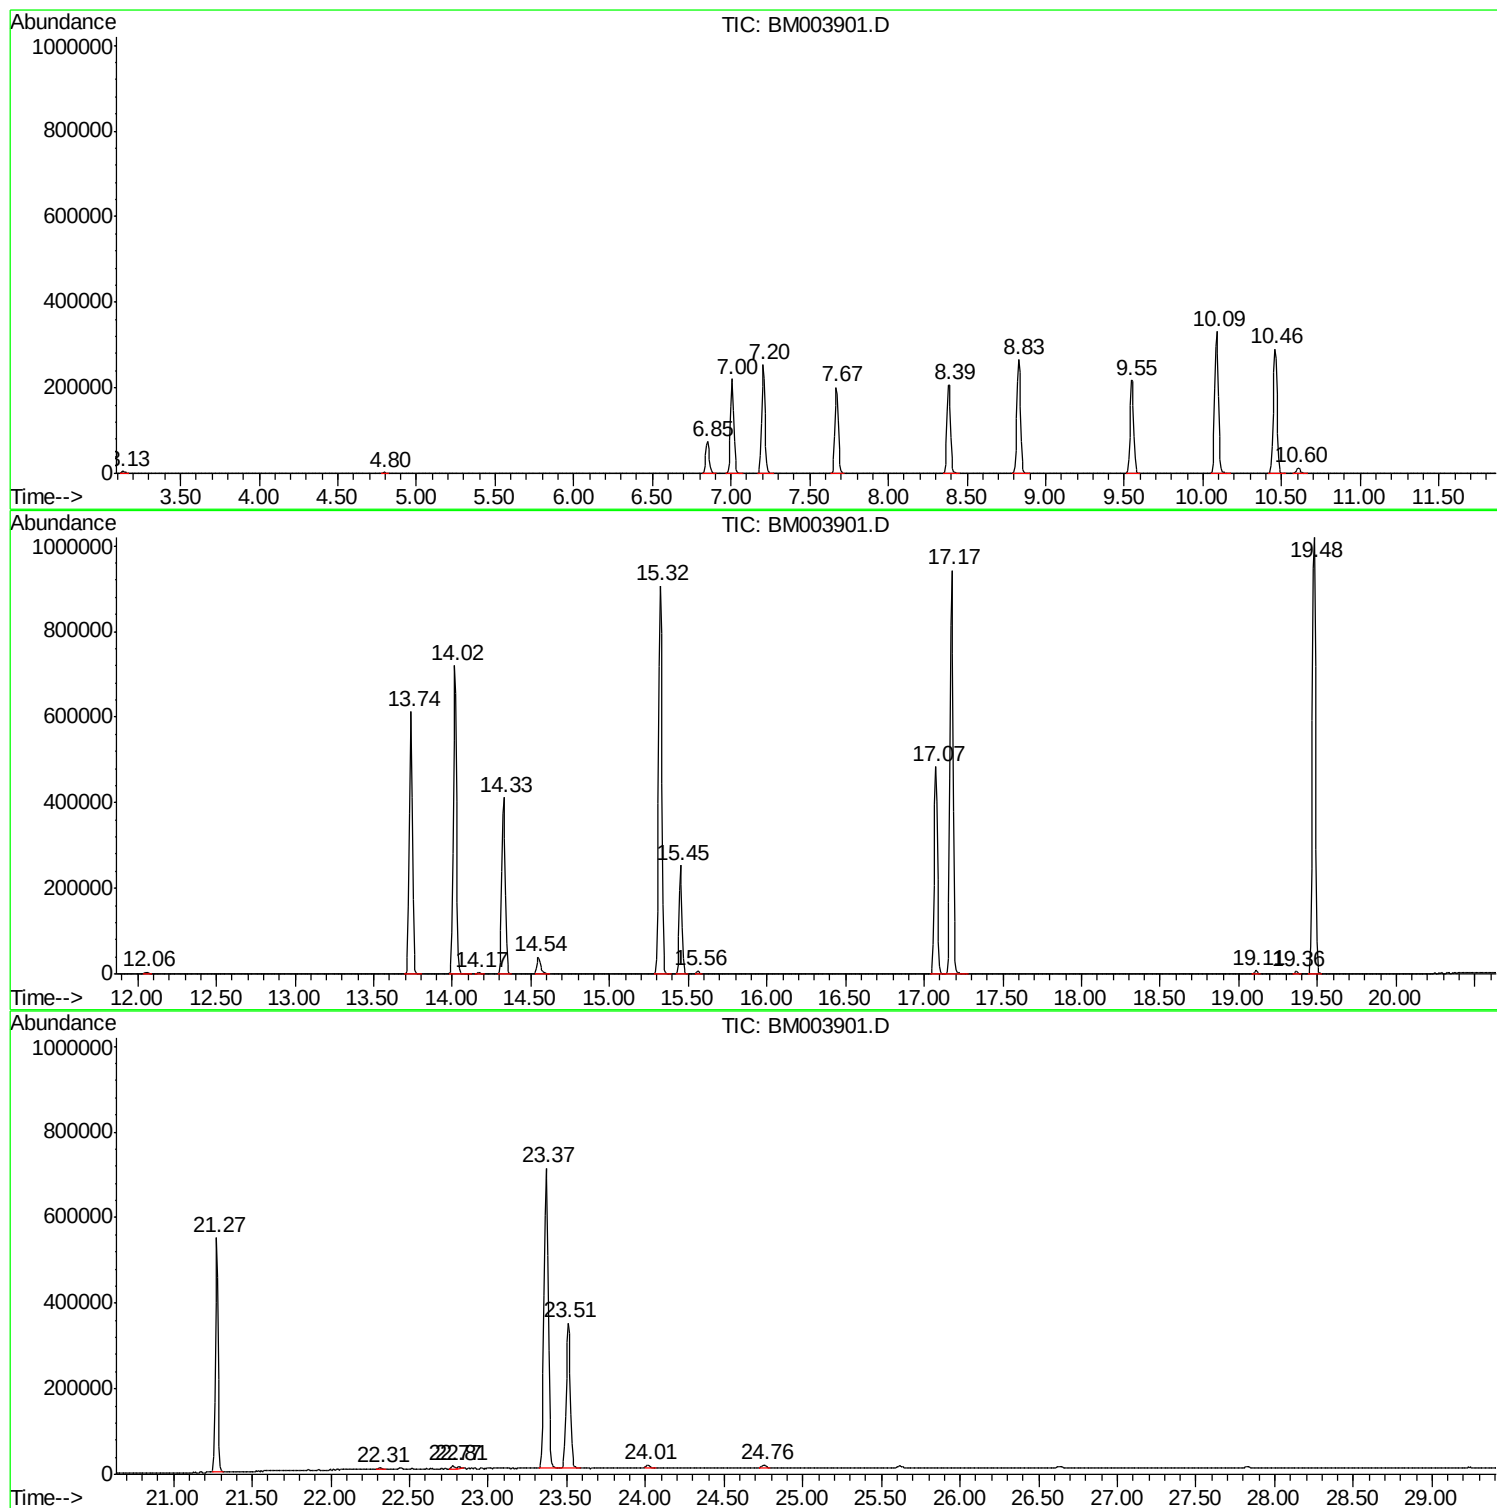

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003901.D
Acq On : 31 Dec 2015 04:27
Operator : SJ/UM
Sample : G4868-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43P0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003901.D
Acq On : 31 Dec 2015 04:27
Operator : SJ/UM
Sample : G4868-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43P0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc