

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
 Data File : BM003902.D
 Acq On : 31 Dec 2015 05:03
 Operator : SJ/UM
 Sample : G4868-24
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43P1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	5	8	11	rVB	2322	2472	0.19%	0.021%
2	6.851	635	640	649	rBB	44515	66038	5.07%	0.559%
3	7.004	661	666	678	rBB	177501	273997	21.04%	2.318%
4	7.204	694	700	711	rBB	185547	283506	21.77%	2.398%
5	7.669	773	779	787	rBB	193958	297132	22.81%	2.513%
6	8.386	895	901	910	rBB	140078	219780	16.87%	1.859%
7	8.828	970	976	988	rBB	214887	334744	25.70%	2.831%
8	9.545	1093	1098	1106	rBB	174472	280140	21.51%	2.370%
9	10.086	1184	1190	1203	rBB	256652	411984	31.63%	3.485%
10	10.457	1246	1253	1264	rBB	284996	463267	35.57%	3.919%
11	10.604	1274	1278	1285	rBB	7832	12616	0.97%	0.107%
12	12.057	1521	1525	1529	rBB	2719	4079	0.31%	0.035%
13	13.739	1804	1811	1821	rBB	504520	732124	56.21%	6.193%
14	14.015	1852	1858	1877	rBB	600258	863602	66.30%	7.305%
15	14.168	1880	1884	1888	rBV	1945	3054	0.23%	0.026%
16	14.327	1905	1911	1918	rBB2	424319	632194	48.54%	5.347%
17	14.545	1944	1948	1959	rBB	22685	38539	2.96%	0.326%
18	15.321	2074	2080	2089	rBB	795146	1119997	85.99%	9.473%
19	15.451	2097	2102	2109	rBV	214306	276315	21.21%	2.337%
20	15.562	2117	2121	2125	rBB	5447	6486	0.50%	0.055%
21	16.862	2339	2342	2345	rBB	1159	1371	0.11%	0.012%
22	17.074	2372	2378	2387	rBB	523707	727410	55.85%	6.153%
23	17.174	2388	2395	2411	rBV	877470	1205881	92.58%	10.200%
24	19.109	2720	2724	2728	rVB	6201	7476	0.57%	0.063%
25	19.362	2763	2767	2772	rBV	4700	5889	0.45%	0.050%
26	19.480	2780	2787	2799	rBV	960971	1302497	100.00%	11.017%
27	21.274	3087	3092	3103	rBV	565032	689698	52.95%	5.834%
28	22.315	3266	3269	3273	rBV2	4134	4471	0.34%	0.038%
29	22.774	3345	3347	3351	rVB2	4860	5856	0.45%	0.050%
30	22.815	3351	3354	3359	rBV	4636	5708	0.44%	0.048%
31	23.368	3441	3448	3463	rVB	548287	958169	73.56%	8.105%
32	23.509	3465	3472	3483	rVV	304023	562326	43.17%	4.756%
33	24.015	3554	3558	3562	rBV2	7350	10705	0.82%	0.091%
34	24.756	3680	3684	3690	rVB2	7222	12959	0.99%	0.110%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003902.D
Acq On : 31 Dec 2015 05:03
Operator : SJ/UM
Sample : G4868-24
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43P1

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION


Sum of corrected areas: 11822482

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010116\
Data File : BM003902.D
Acq On : 31 Dec 2015 05:03
Operator : SJ/UM
Sample : G4868-24
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43P1

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

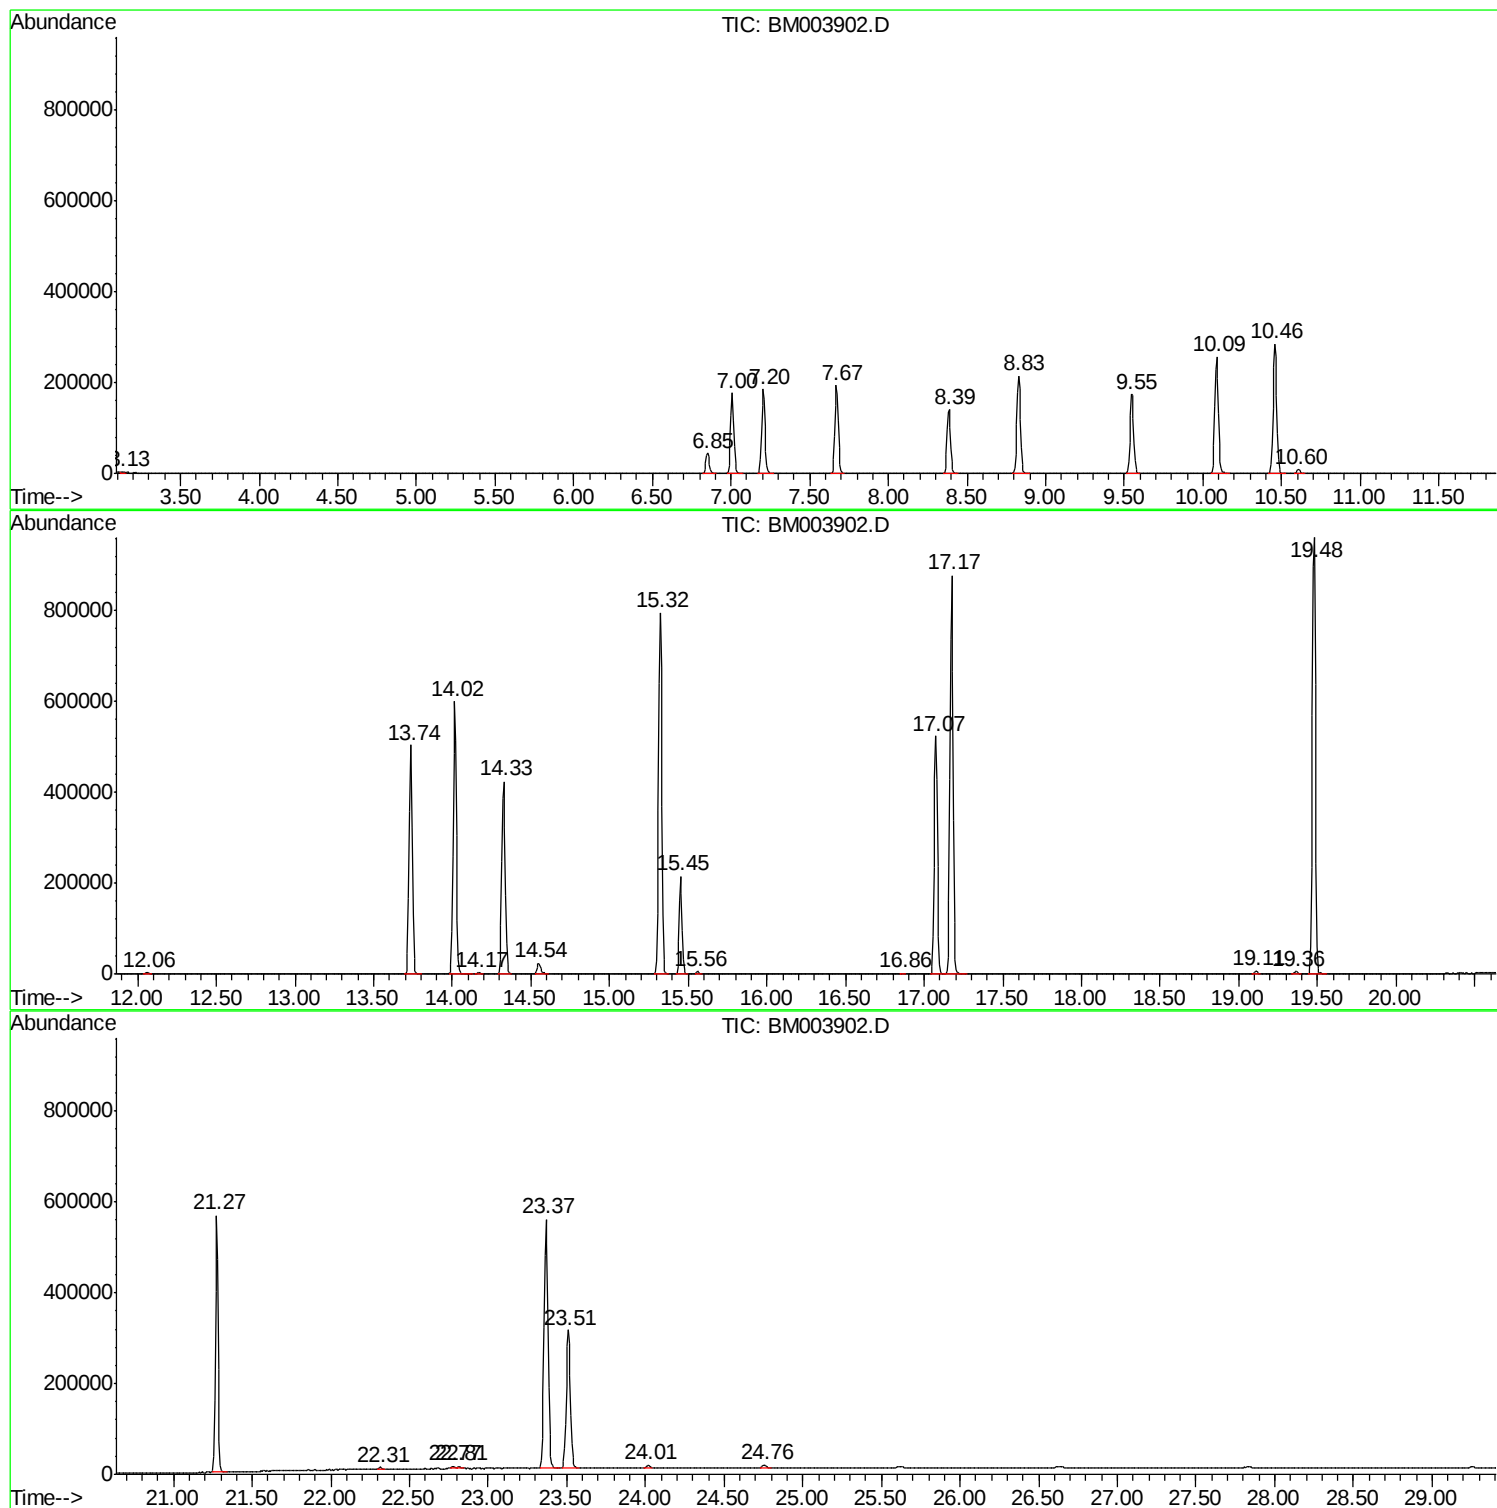

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003902.D
Acq On : 31 Dec 2015 05:03
Operator : SJ/UM
Sample : G4868-24
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43P1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010116\
Data File : BM003902.D
Acq On : 31 Dec 2015 05:03
Operator : SJ/UM
Sample : G4868-24
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43P1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc