


Data Path : Z:\HPCHEM1\BNA M\Data\BM010116\
 Data File : BM003870.D
 Acq On : 30 Dec 2015 08:20
 Operator : SJ/UM
 Sample : DFTPP66
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP66

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION
 Last Update : Thu Dec 31 04:08:11 2015

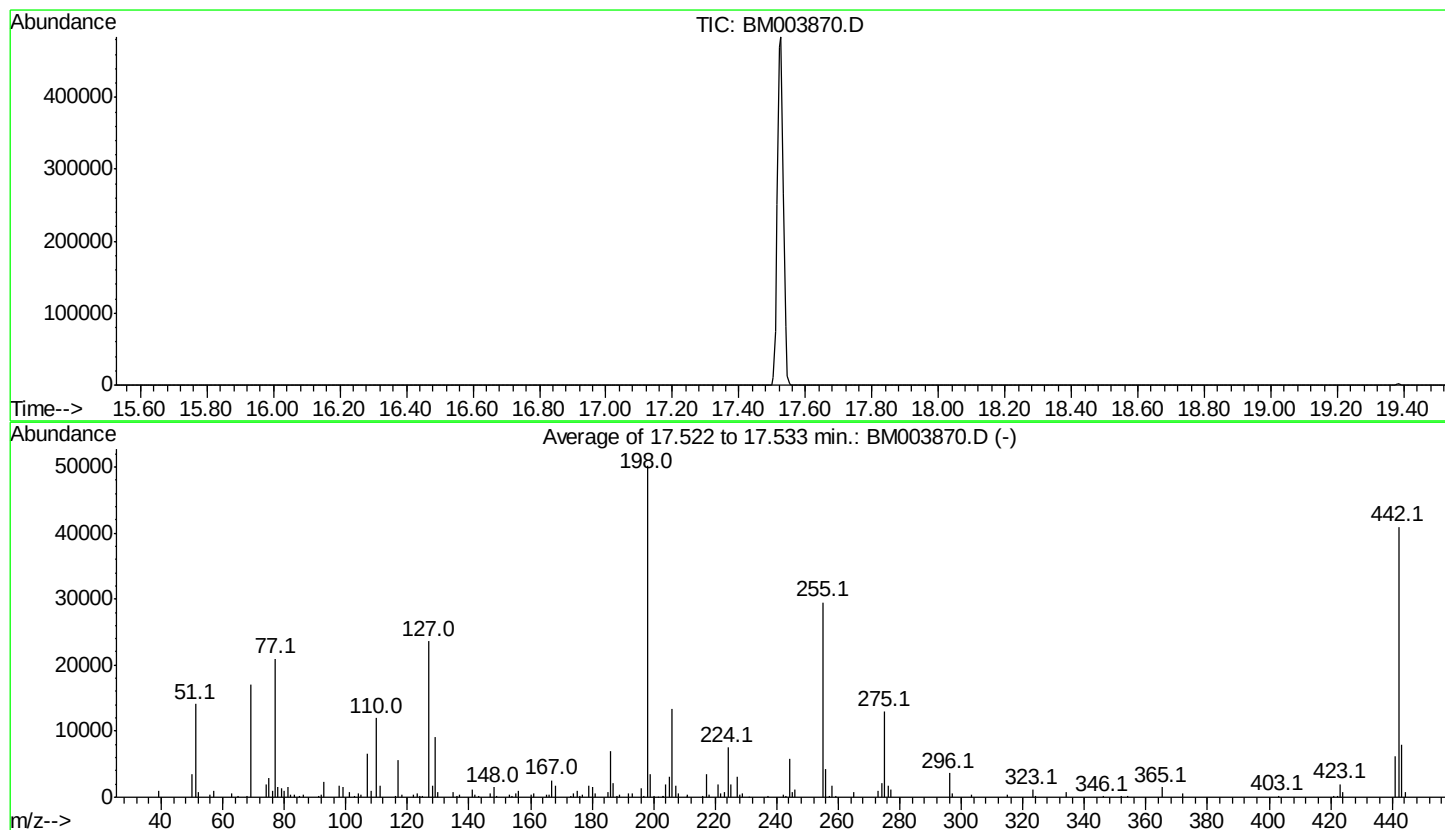

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	14130	PASS
68	69	0.00	2	0.8	137	PASS
69	198	0.00	100	33.9	17018	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	23592	PASS
197	198	0.00	2	0.2	105	PASS
198	198	100	100	100.0	50192	PASS
199	198	5	9	6.8	3433	PASS
275	198	10	60	25.7	12921	PASS
365	198	1	100	3.1	1532	PASS
441	443	0.01	100	78.7	6276	PASS
442	198	50	100	81.5	40901	PASS
443	442	15	24	19.5	7974	PASS

Scan 2449 (17.492 min): BM003870.D
DFTPP66

m/z	Abundance
207.00	354.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

m/z	Abundance
39.00	1397.0
50.10	4541.0
51.10	18408.0
52.00	966.0
56.00	540.0
57.00	1263.0
63.00	796.0
65.00	423.0
68.00	412.0
69.00	21848.0
74.00	2462.0
75.00	3782.0
76.10	1303.0
77.10	26976.0
78.00	1847.0
79.00	1725.0
80.00	1269.0
81.00	1891.0
82.00	494.0
83.10	460.0
85.00	384.0
86.00	521.0
91.00	451.0
92.00	504.0
93.00	2997.0
98.00	2244.0
99.00	2146.0
101.00	1030.0
103.00	303.0
104.00	681.0
105.00	575.0
107.00	8204.0
108.00	1269.0
110.00	14765.0
111.00	2306.0
116.00	408.0
117.00	6919.0
118.00	533.0
122.00	538.0
123.00	873.0
124.00	358.0
125.00	361.0
127.00	29048.0
128.00	2244.0
129.00	11040.0
130.00	953.0
135.00	940.0
135.90	393.0
137.00	569.0
141.00	1431.0
142.00	477.0
143.00	351.0
147.00	707.0
148.00	1775.0
149.00	371.0
153.00	497.0
154.00	356.0
155.00	834.0
156.10	1157.0
160.00	491.0
161.00	678.0
165.00	477.0
166.00	483.0
167.00	2929.0
168.00	2159.0
174.00	558.0
175.00	1108.0
177.00	491.0
179.00	2204.0
180.00	1799.0
181.00	633.0
185.00	1078.0
186.00	8286.0
187.00	2404.0
188.00	315.0
189.00	519.0
192.00	689.0
193.00	825.0
196.00	1635.0
198.00	57840.0
199.00	4187.0
200.10	312.0
202.90	396.0
204.00	2077.0
205.10	3298.0
206.10	15421.0
207.10	2248.0
208.00	587.0
210.90	647.0
216.00	311.0
217.00	3939.0
218.00	432.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

221.10	2158.0
221.80	571.0
223.00	904.0
224.10	8665.0
225.10	2203.0
227.00	3571.0
228.00	521.0
229.00	765.0
231.00	307.0
237.10	418.0
242.00	471.0
243.00	394.0
244.10	6553.0
245.10	865.0
246.10	1298.0
255.10	32824.0
256.00	4815.0
257.00	421.0
258.00	1878.0
265.00	781.0
273.00	970.0
274.10	2464.0
275.10	13940.0
276.10	2009.0
277.00	1215.0
296.00	3724.0
297.00	518.0
303.10	464.0
315.00	440.0
323.10	1146.0
334.10	771.0
354.10	328.0
365.10	1388.0
372.10	528.0
403.00	344.0
423.10	1855.0
424.10	728.0
441.10	5589.0
442.10	36920.0
443.10	7273.0
444.10	657.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

m/z	Abundance
39.00	1125.0
50.10	3985.0
51.10	15846.0
52.00	836.0
56.00	480.0
57.00	1155.0
63.00	718.0
65.00	396.0
69.00	19464.0
74.00	2056.0
75.00	3372.0
76.10	1154.0
77.10	23608.0
78.10	1697.0
79.00	1507.0
80.00	1174.0
81.00	1730.0
81.90	459.0
83.00	476.0
85.00	407.0
86.00	471.0
91.00	413.0
92.00	465.0
93.00	2672.0
98.00	2040.0
99.00	1834.0
101.00	1009.0
103.00	301.0
104.00	575.0
105.00	620.0
107.00	7622.0
108.00	1088.0
110.00	13854.0
111.00	2098.0
116.00	400.0
117.00	6633.0
118.00	497.0
122.00	463.0
123.00	774.0
124.00	340.0
125.00	337.0
127.00	27200.0
128.00	2024.0
129.00	10597.0
130.00	871.0
135.00	928.0
136.00	380.0
137.00	486.0
141.00	1454.0
141.90	445.0
143.00	317.0
147.00	753.0
148.00	1748.0
149.00	381.0
153.00	441.0
153.90	330.0
155.00	772.0
156.10	1163.0
160.00	423.0
161.00	683.0
165.00	580.0
166.00	420.0
167.00	3039.0
168.00	2027.0
173.00	341.0
174.00	648.0
175.00	1157.0
176.00	331.0
177.00	564.0
179.00	2082.0
180.00	1697.0
181.00	673.0
185.00	1010.0
186.00	8191.0
187.00	2420.0
189.00	544.0
192.00	749.0
193.10	837.0
196.00	1573.0
196.80	315.0
198.00	59816.0
199.00	3942.0
200.00	313.0
201.30	302.0
203.10	373.0
204.10	2231.0
205.10	3738.0
206.10	15742.0
207.10	2279.0
208.00	536.0
211.10	578.0
216.00	386.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

217.00	4367.0
218.00	590.0
221.00	2269.0
221.80	622.0
223.10	947.0
224.10	8921.0
225.10	2345.0
227.00	3768.0
228.00	516.0
229.00	779.0
237.00	457.0
242.00	440.0
243.10	459.0
244.10	6657.0
245.00	893.0
246.00	1371.0
255.10	35720.0
256.10	4920.0
257.10	452.0
258.00	2000.0
259.00	381.0
265.00	845.0
273.10	1138.0
274.10	2621.0
275.10	15461.0
276.10	2121.0
277.00	1378.0
296.10	4466.0
297.00	620.0
303.10	533.0
315.10	501.0
323.10	1310.0
324.10	325.0
334.10	927.0
346.10	346.0
352.00	426.0
354.10	452.0
365.00	1890.0
372.10	644.0
403.10	420.0
421.00	329.0
422.10	373.0
423.10	2450.0
424.10	798.0
441.10	7592.0
442.10	49664.0
443.10	9663.0
444.10	875.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

m/z	Abundance
39.00	586.0
50.00	1935.0
51.10	8136.0
52.00	405.0
57.00	549.0
63.00	324.0
69.00	9742.0
74.00	1065.0
75.00	1659.0
76.00	548.0
77.10	12322.0
78.00	847.0
79.00	743.0
79.90	627.0
81.00	834.0
93.00	1327.0
98.00	1088.0
99.00	936.0
100.90	503.0
104.00	330.0
107.00	3954.0
108.00	563.0
110.00	7217.0
111.00	1122.0
117.00	3389.0
123.00	399.0
127.00	14529.0
128.00	998.0
129.00	5450.0
130.00	426.0
134.90	426.0
141.00	694.0
147.00	438.0
148.00	934.0
155.00	391.0
156.00	639.0
161.00	374.0
164.90	312.0
167.00	1757.0
168.00	1100.0
174.00	339.0
175.00	644.0
179.00	1142.0
180.00	930.0
181.00	374.0
185.00	538.0
186.00	4549.0
187.00	1303.0
192.00	350.0
193.00	342.0
196.00	996.0
198.00	32920.0
199.00	2172.0
204.00	1313.0
205.00	2223.0
206.10	9117.0
207.00	1560.0
208.10	379.0
211.00	369.0
217.00	2430.0
221.00	1460.0
221.80	328.0
223.00	541.0
224.10	5037.0
225.00	1258.0
227.00	2041.0
228.00	305.0
229.00	406.0
244.10	4196.0
245.00	507.0
246.00	766.0
255.10	20096.0
256.10	3103.0
258.00	1310.0
265.00	576.0
273.00	687.0
274.10	1549.0
275.10	9364.0
276.10	1262.0
277.00	842.0
296.10	2617.0
297.10	396.0
315.00	321.0
323.10	899.0
334.00	511.0
365.00	1318.0
372.10	509.0
423.10	1774.0
424.10	586.0
441.10	5649.0
442.10	36120.0
443.10	6988.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

444.10

638.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66