


Data Path : Z:\HPCHEM1\BNA_M\Data\BM010215\
 Data File : BM000104.D
 Acq On : 02 Jan 2015 09:00
 Operator : TP/IZ
 Sample : DFTPP03
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-02-S-ML

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM122914.M
 Title : SVOA CALIBRATION
 Last Update : Wed Dec 31 02:57:11 2014

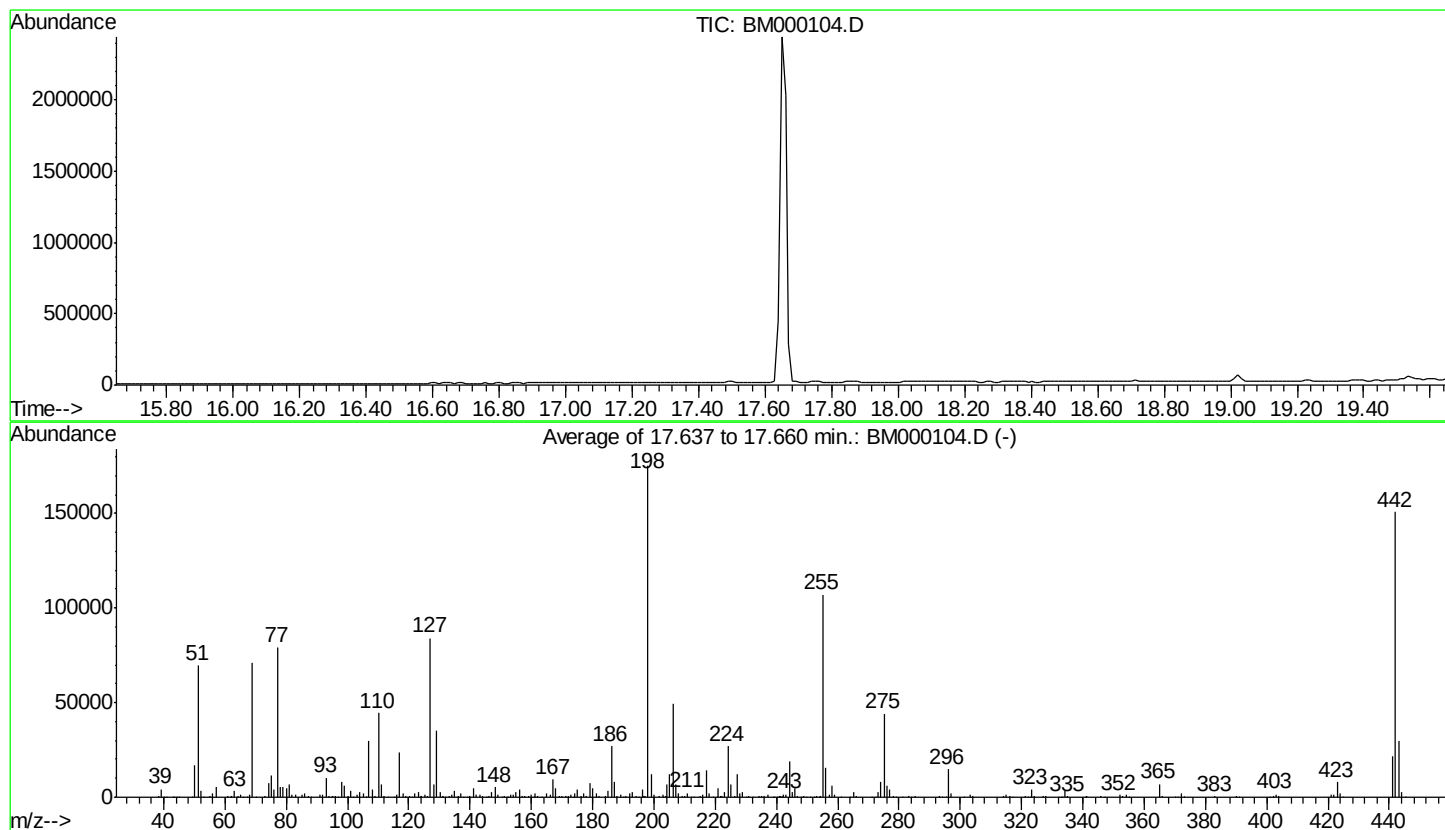

AutoFind: Scans 1308, 1309, 1310; Background Corrected with Scan 1305

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	69392	PASS
68	69	0.00	2	1.8	1266	PASS
69	198	0.00	100	40.6	71197	PASS
70	69	0.00	2	0.4	273	PASS
127	198	10	80	47.9	84010	PASS
197	198	0.00	2	0.4	772	PASS
198	198	100	100	100.0	175285	PASS
199	198	5	9	6.8	11911	PASS
275	198	10	60	25.2	44219	PASS
365	198	1	100	3.9	6783	PASS
441	443	0.01	100	74.0	21971	PASS
442	198	50	100	86.1	150872	PASS
443	442	15	24	19.7	29681	PASS