




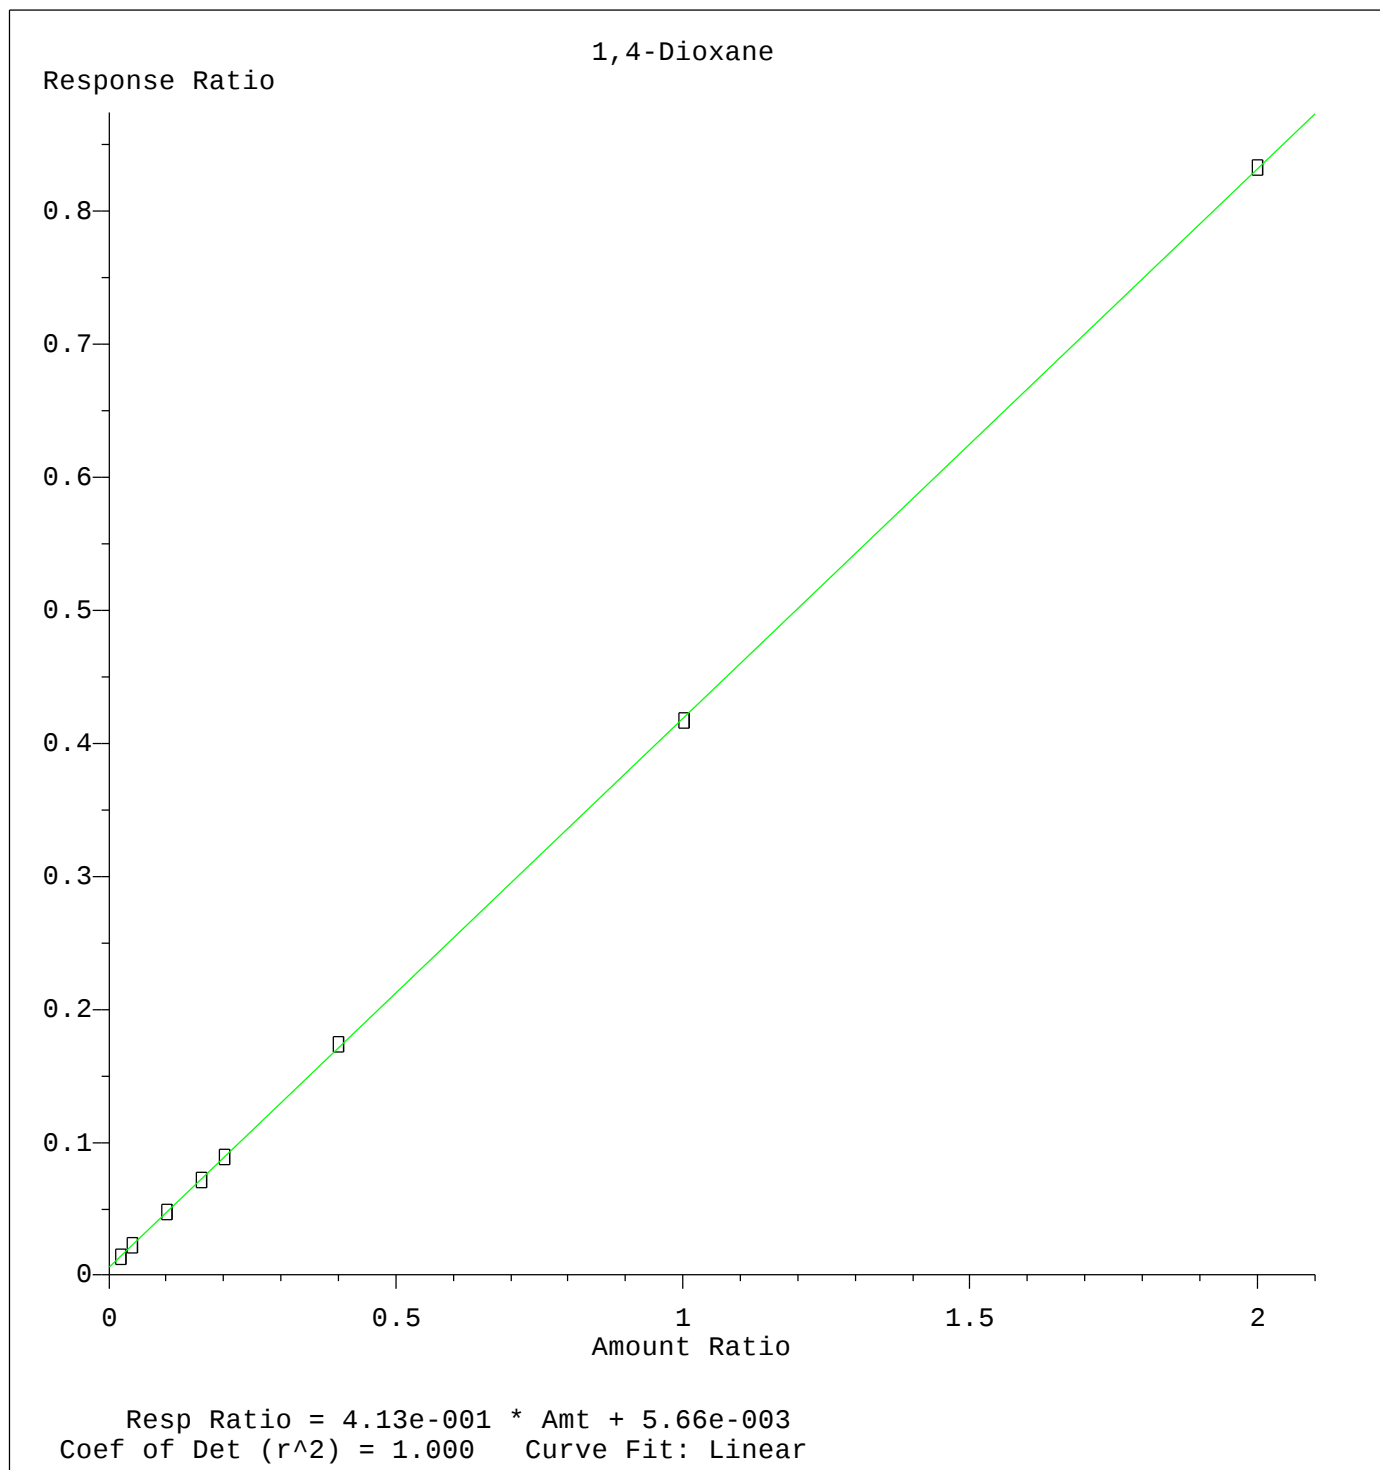


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM010216.M
Calibration Table Last Updated: Thu Dec 31 15:37:36 2015

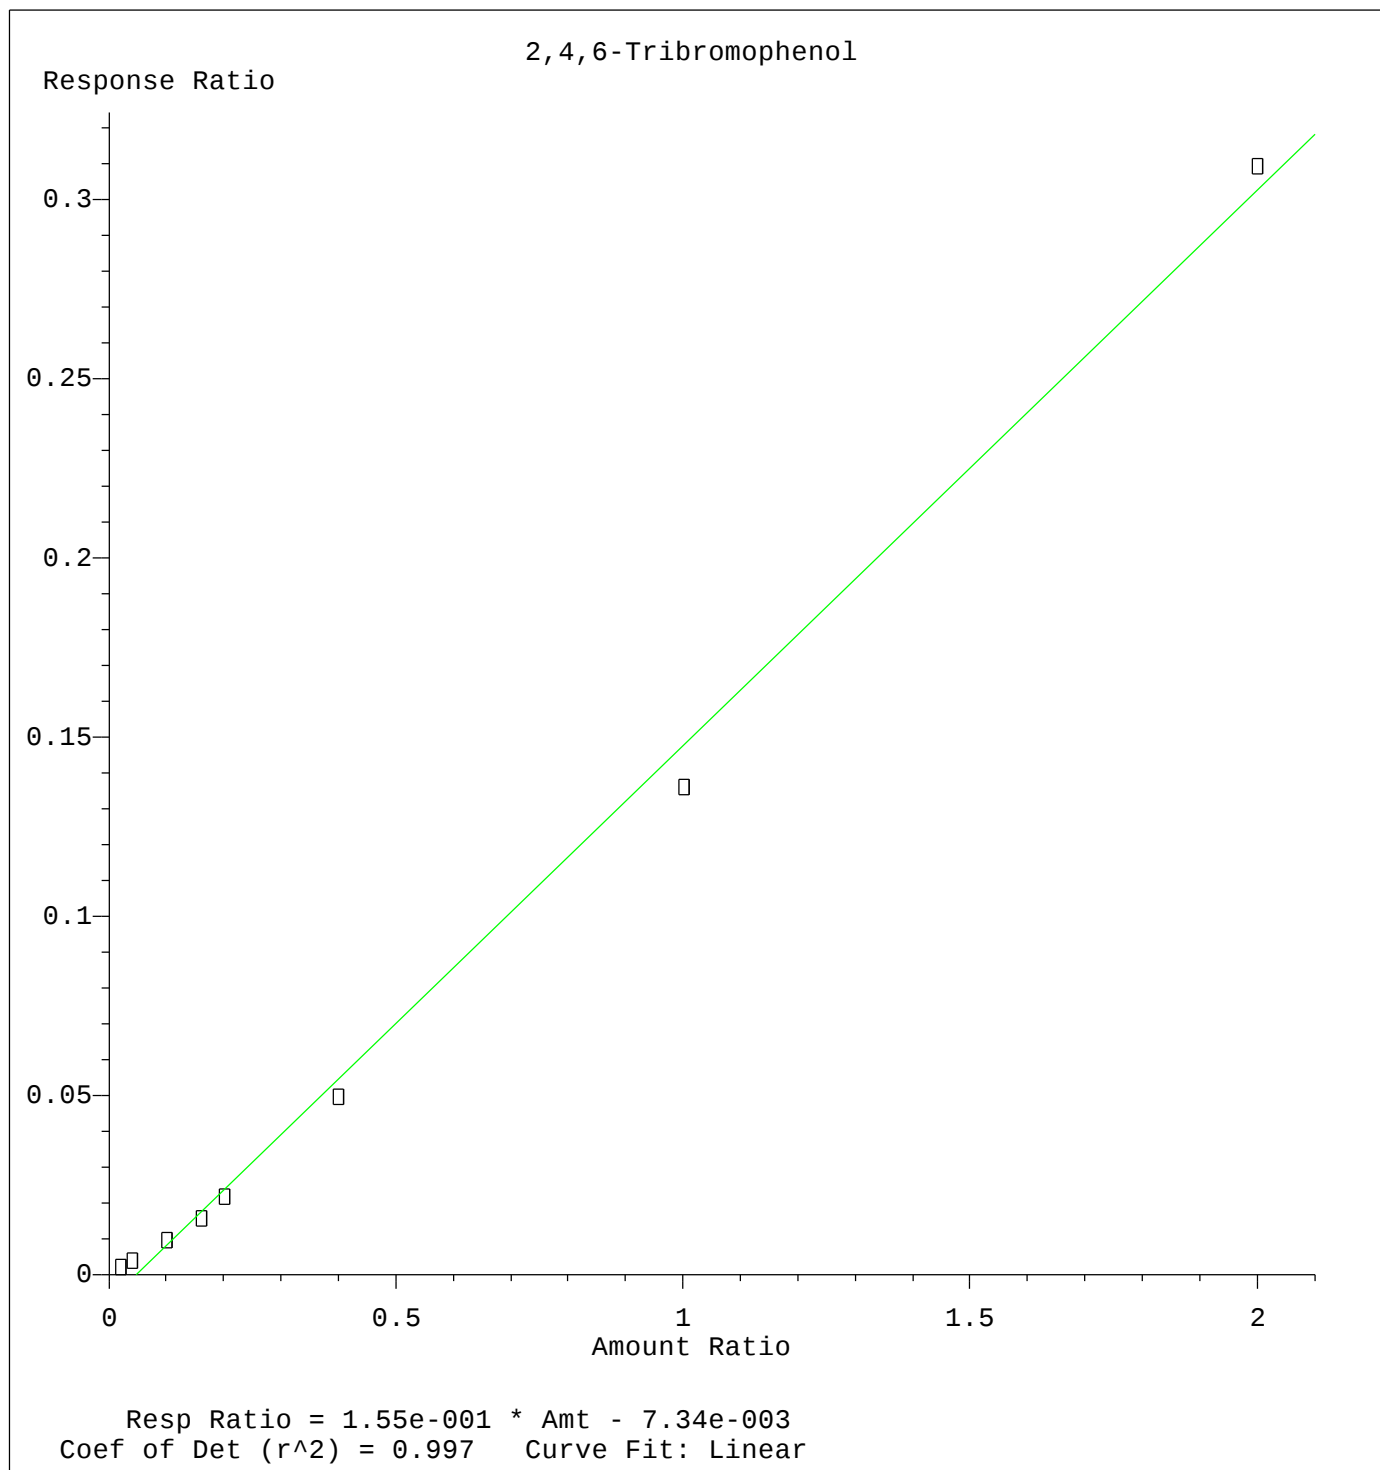


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM010216.M
Calibration Table Last Updated: Thu Dec 31 15:37:36 2015

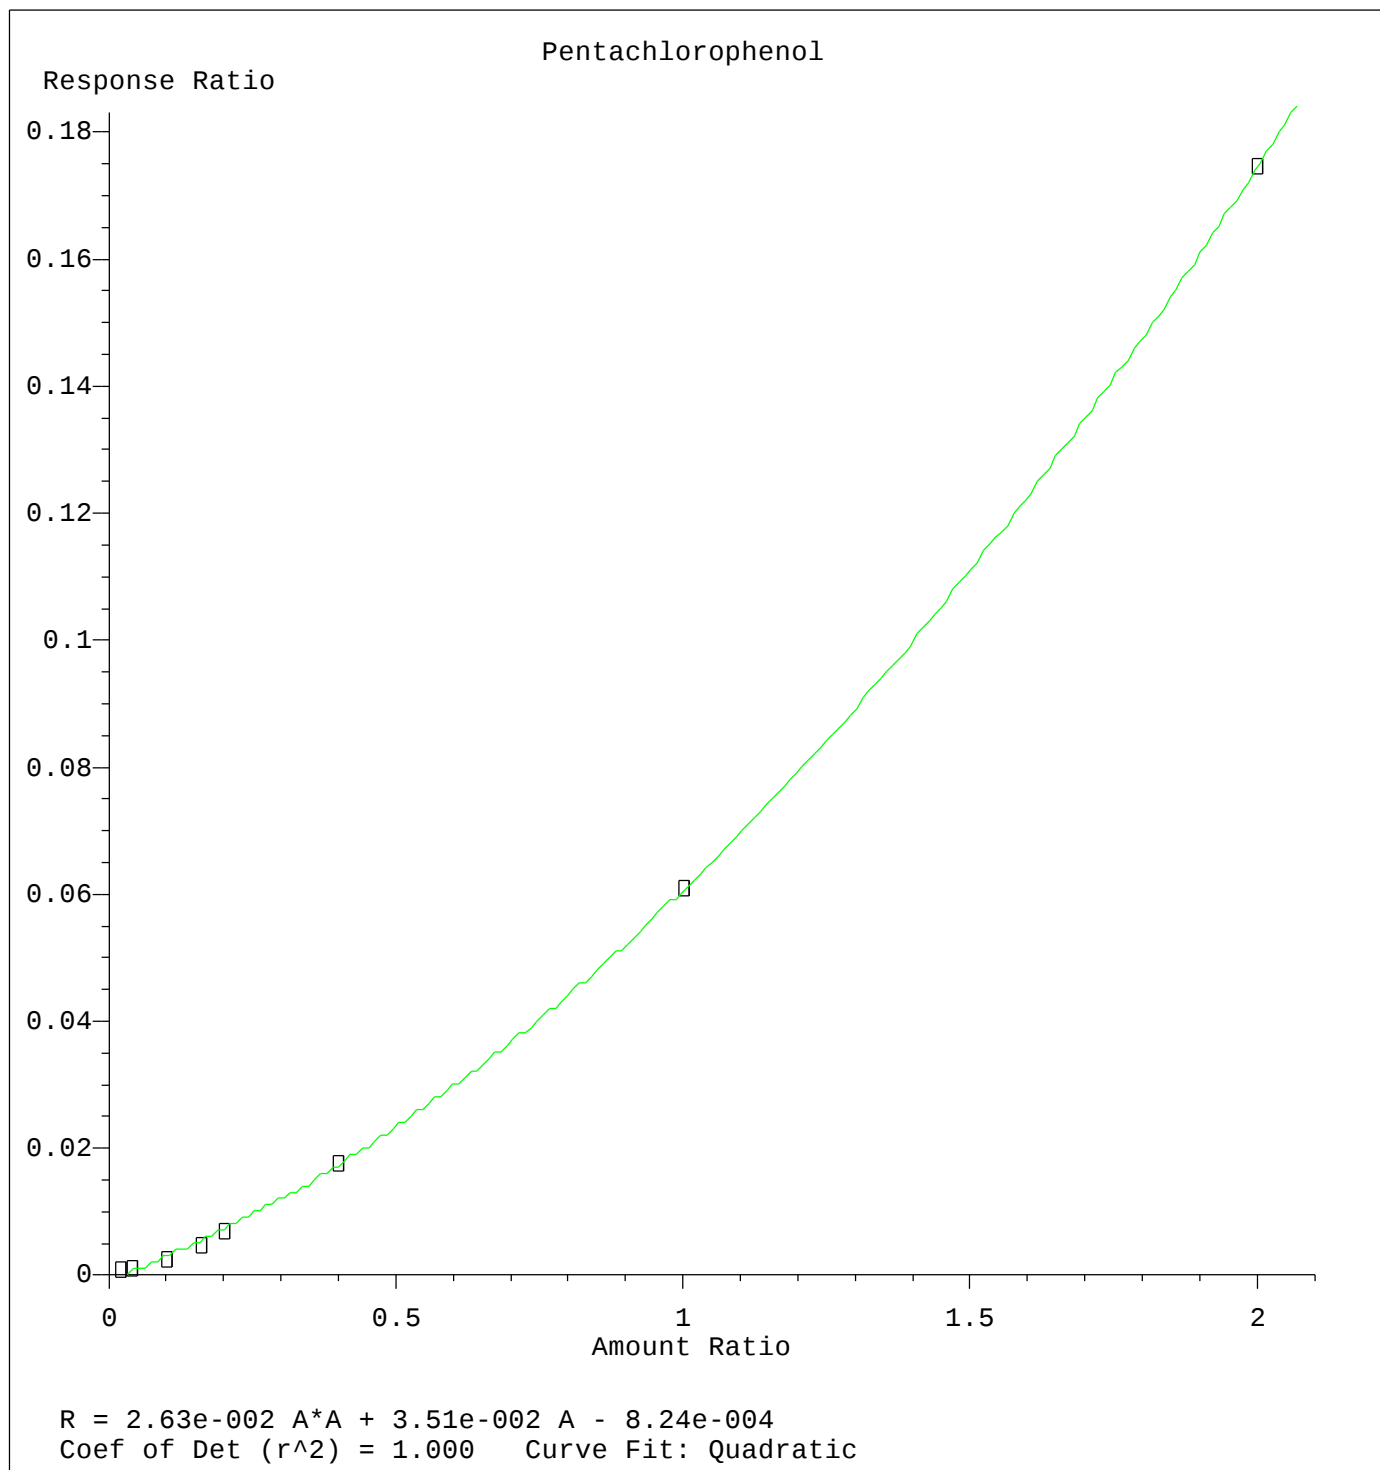

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM010216.M
Calibration Table Last Updated: Thu Dec 31 15:37:36 2015

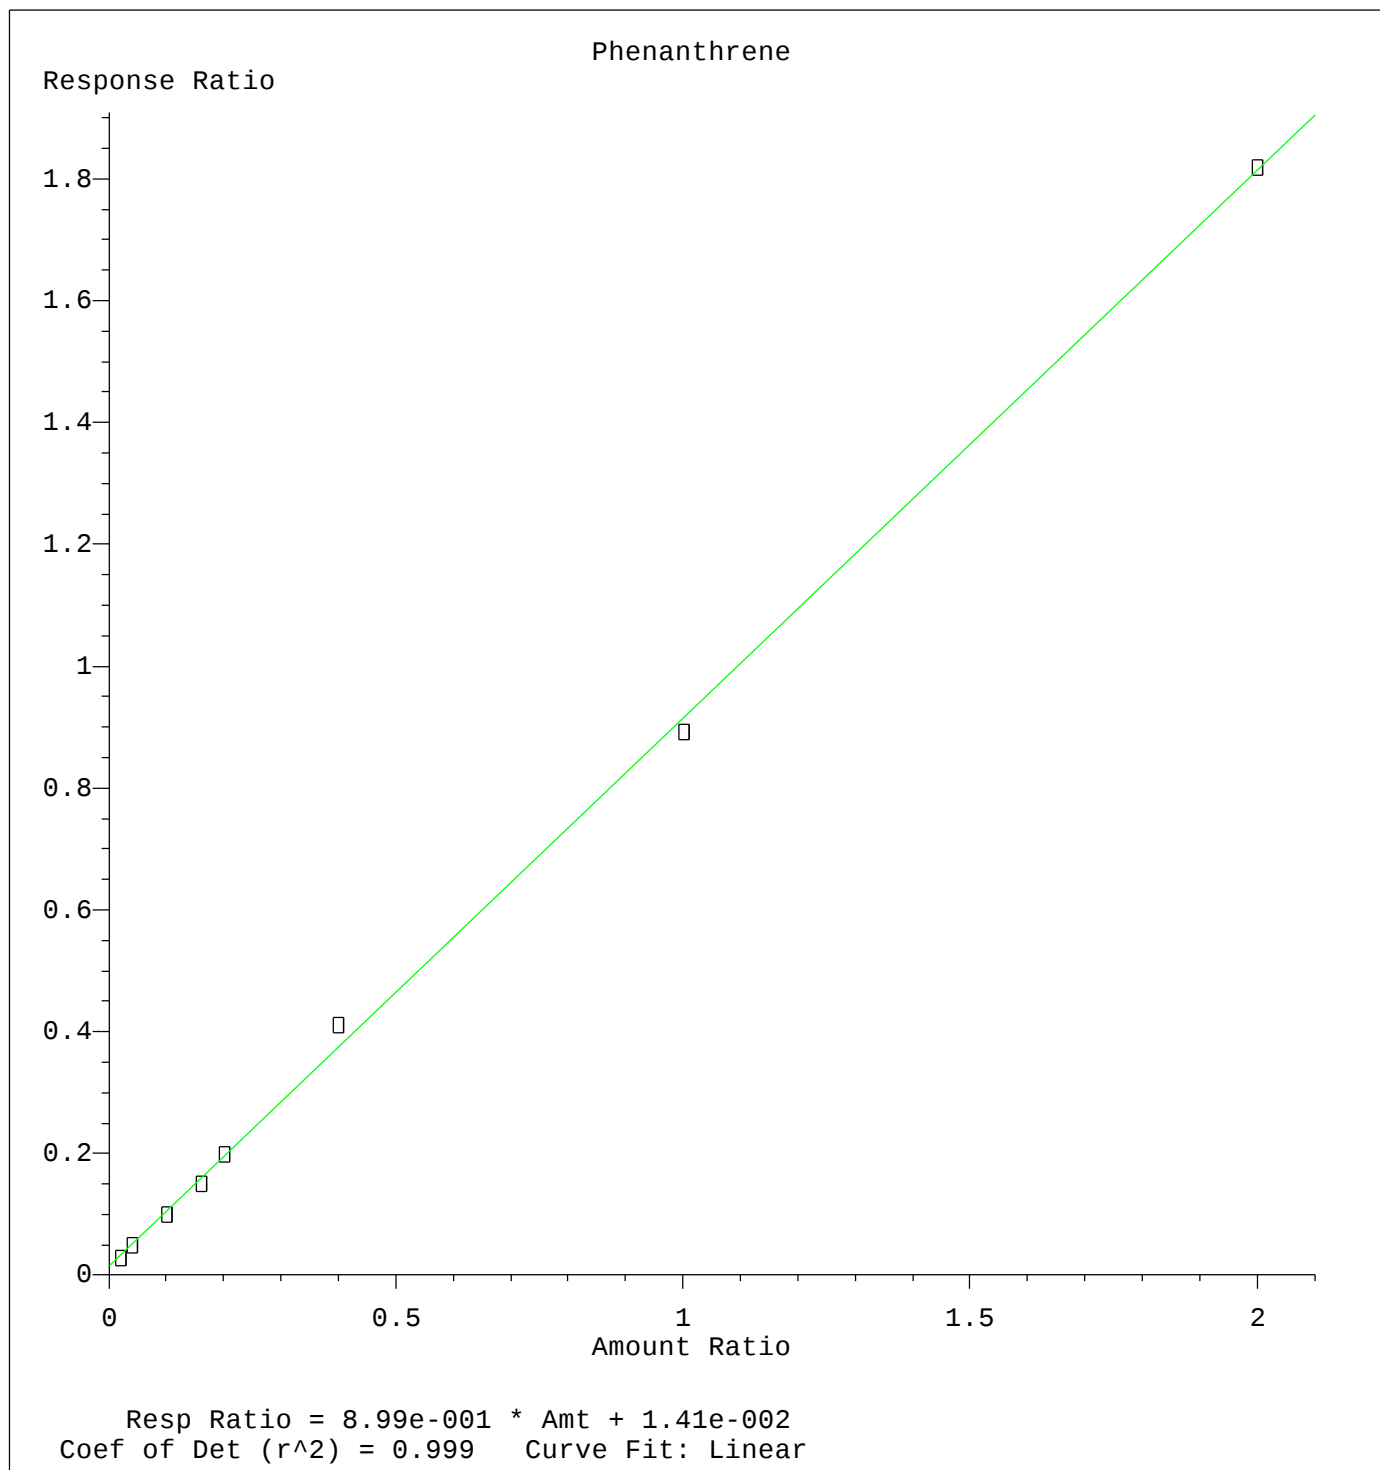


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM010216.M
Calibration Table Last Updated: Thu Dec 31 15:37:36 2015

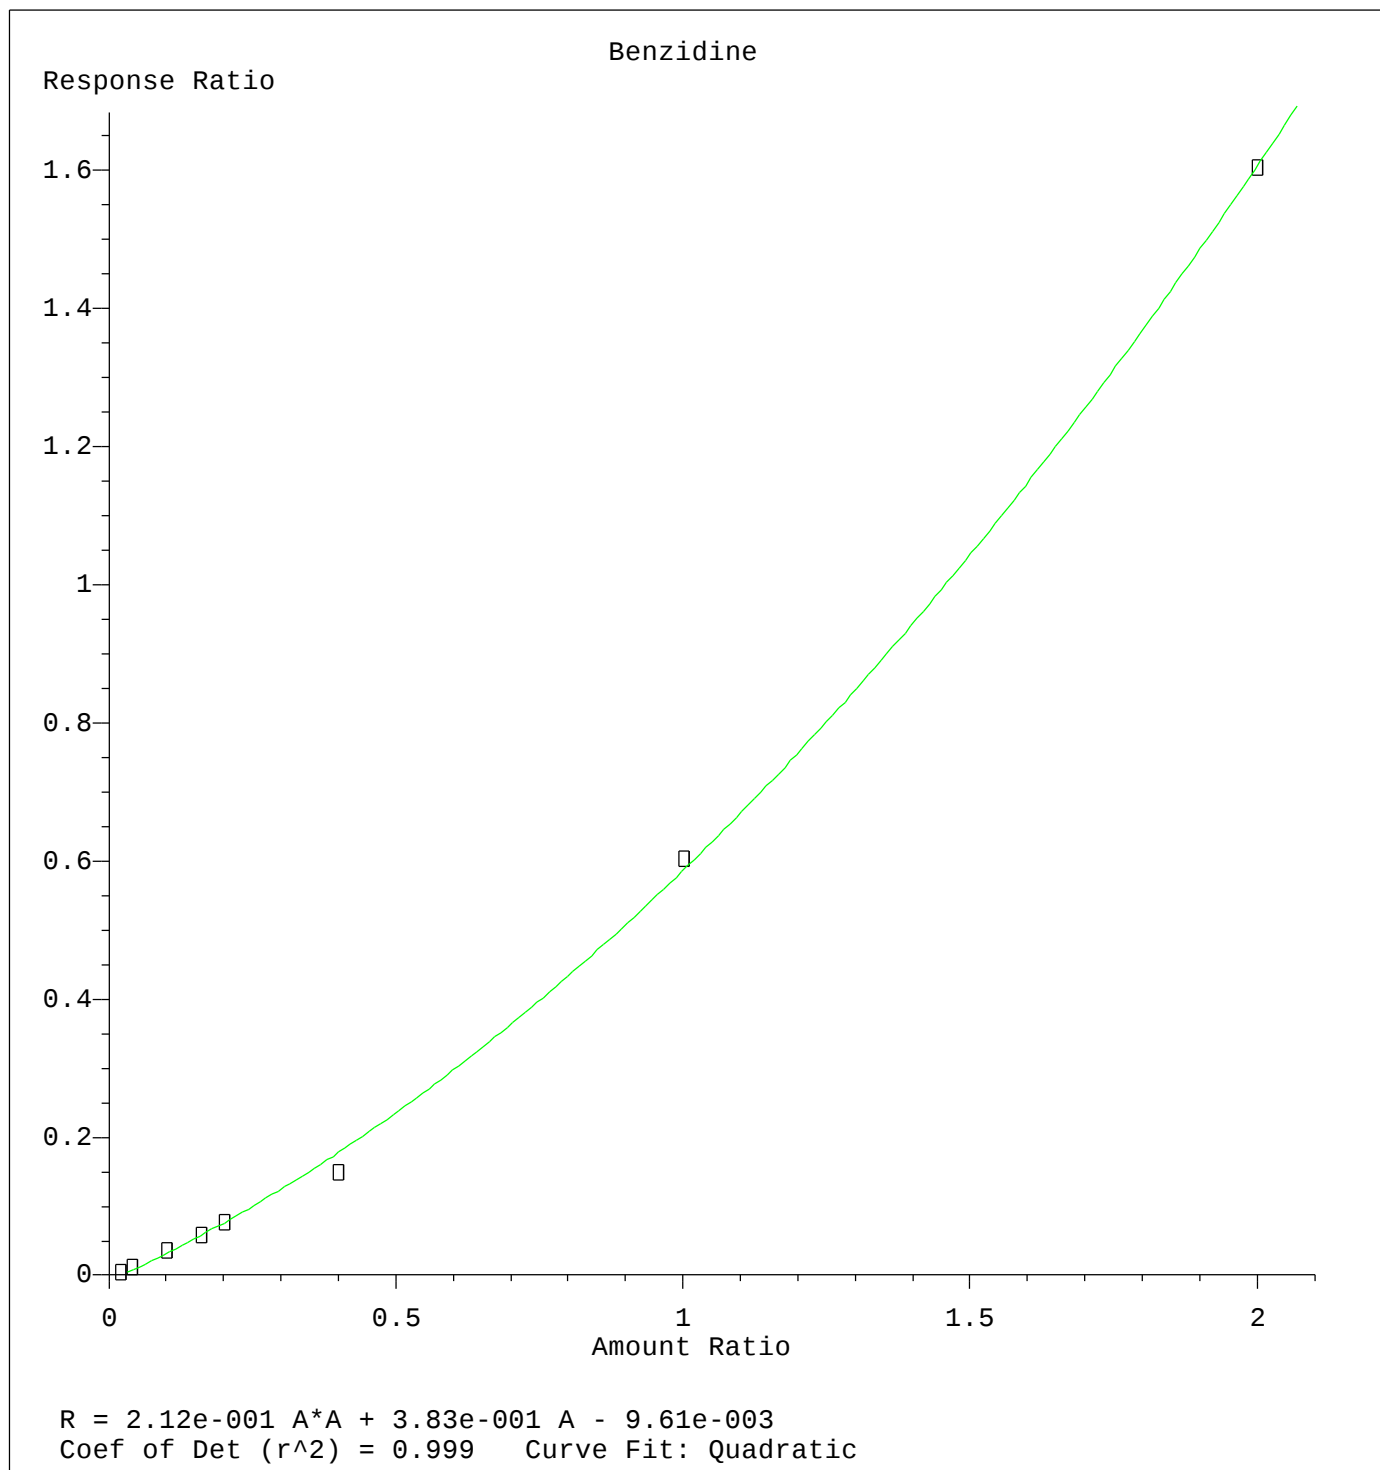

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM010216.M
Calibration Table Last Updated: Thu Dec 31 15:37:36 2015

3,3'-Dichlorobenzidine

Response Ratio

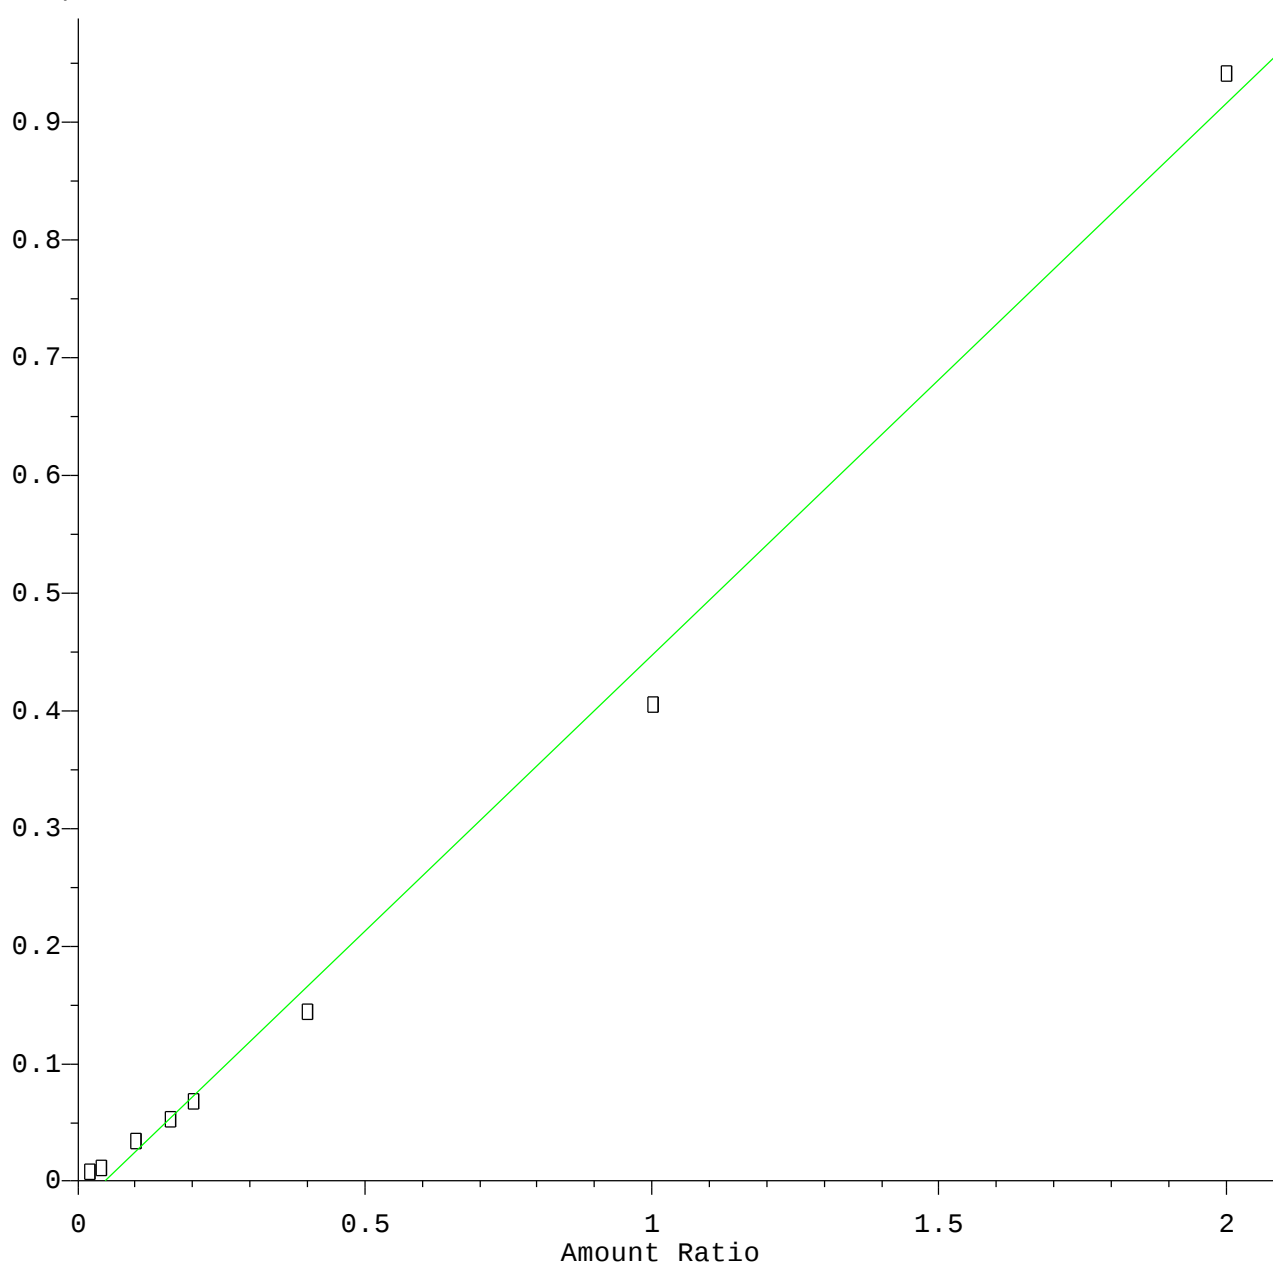


Resp Ratio = $4.69 \times 10^{-1} \times \text{Amt} - 2.22 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM010216.M
Calibration Table Last Updated: Thu Dec 31 15:37:36 2015

Bis(2-ethylhexyl)phthalate

Response Ratio

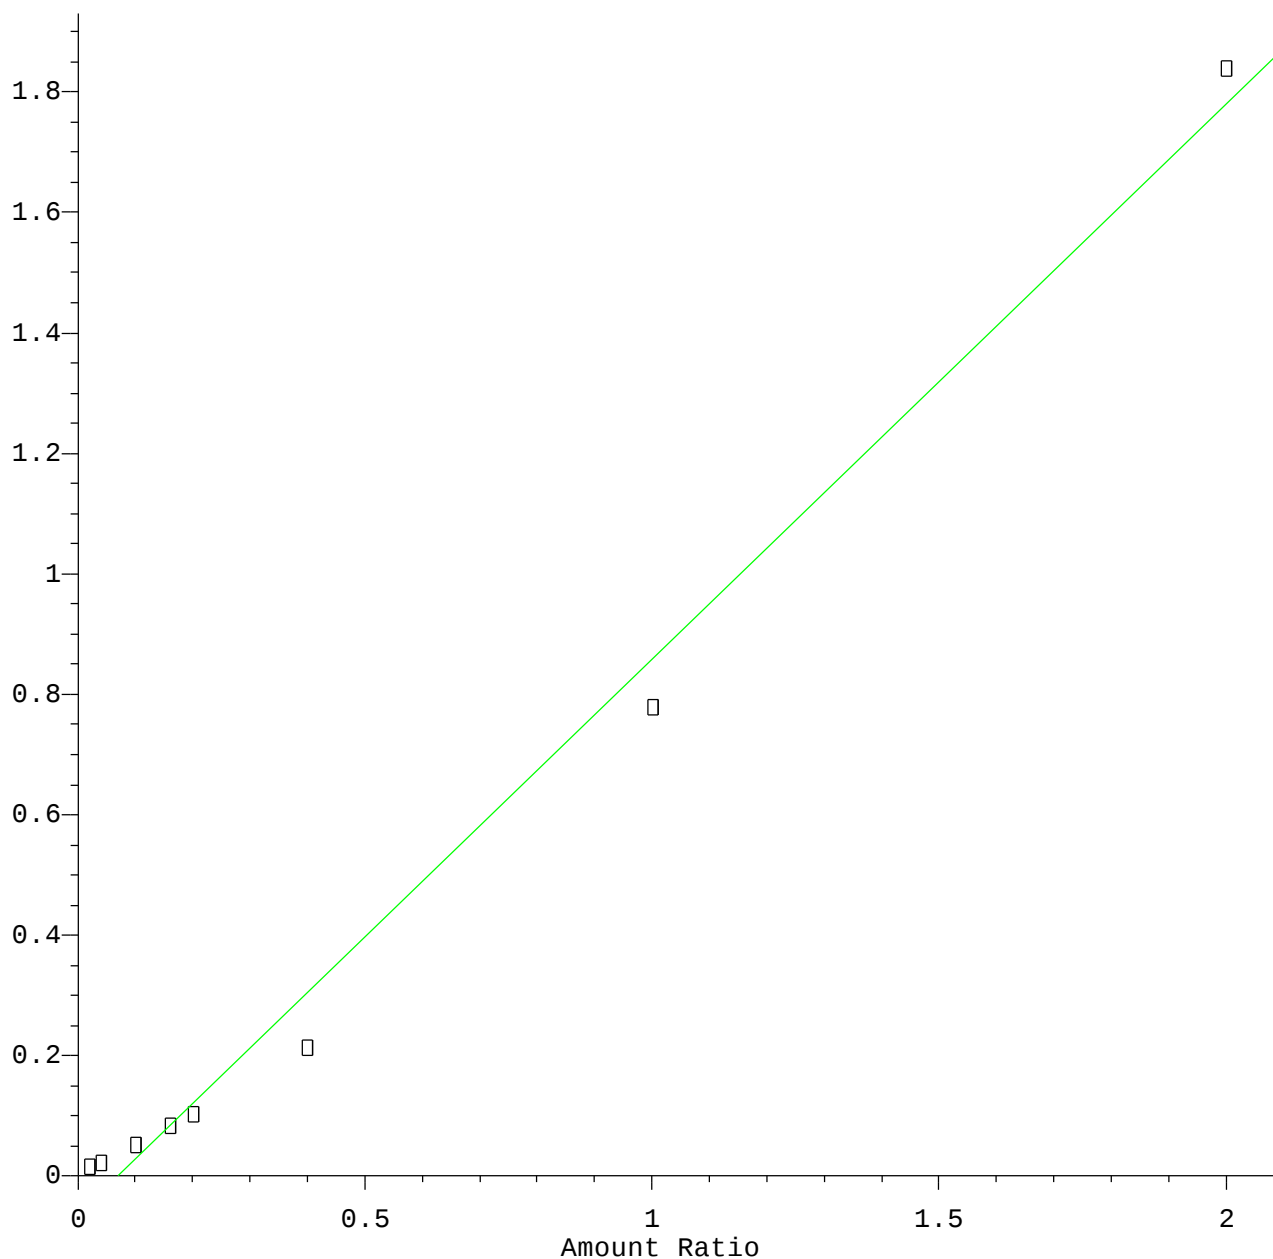

Resp Ratio = $9.22 \times 10^{-1} \times \text{Amt} - 6.43 \times 10^{-2}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM010216.M
Calibration Table Last Updated: Thu Dec 31 15:37:36 2015