
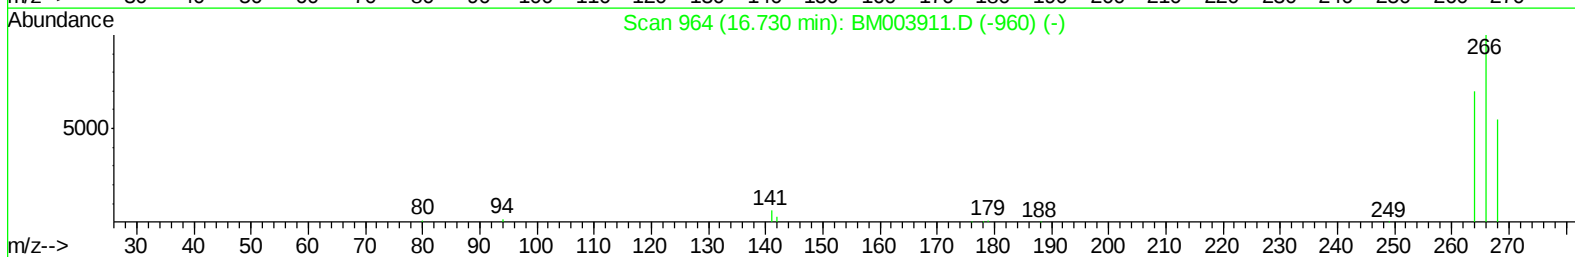
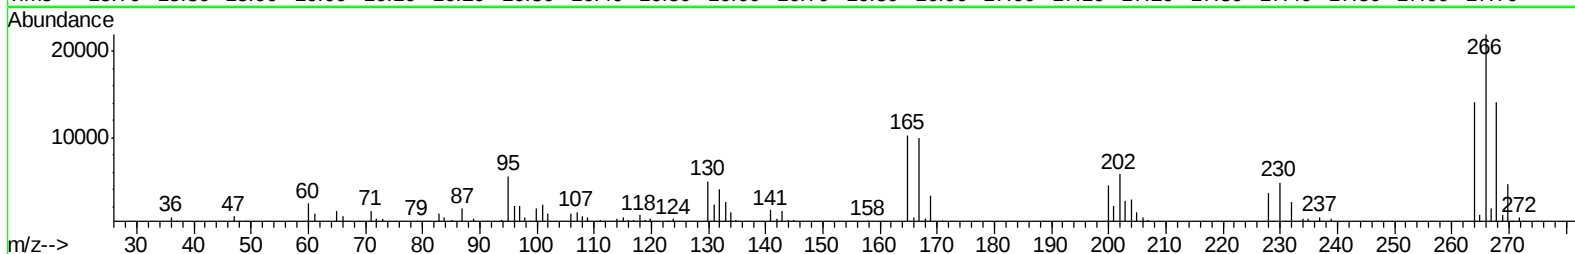


Data Path : Z:\HPCHEM1\BNA M\DATA\BM010216\
Data File : BM003905.D
Acq On : 31 Dec 2015 09:11
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 09:45:30 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM122415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 24 10:08:49 2015
Response via : Initial Calibration

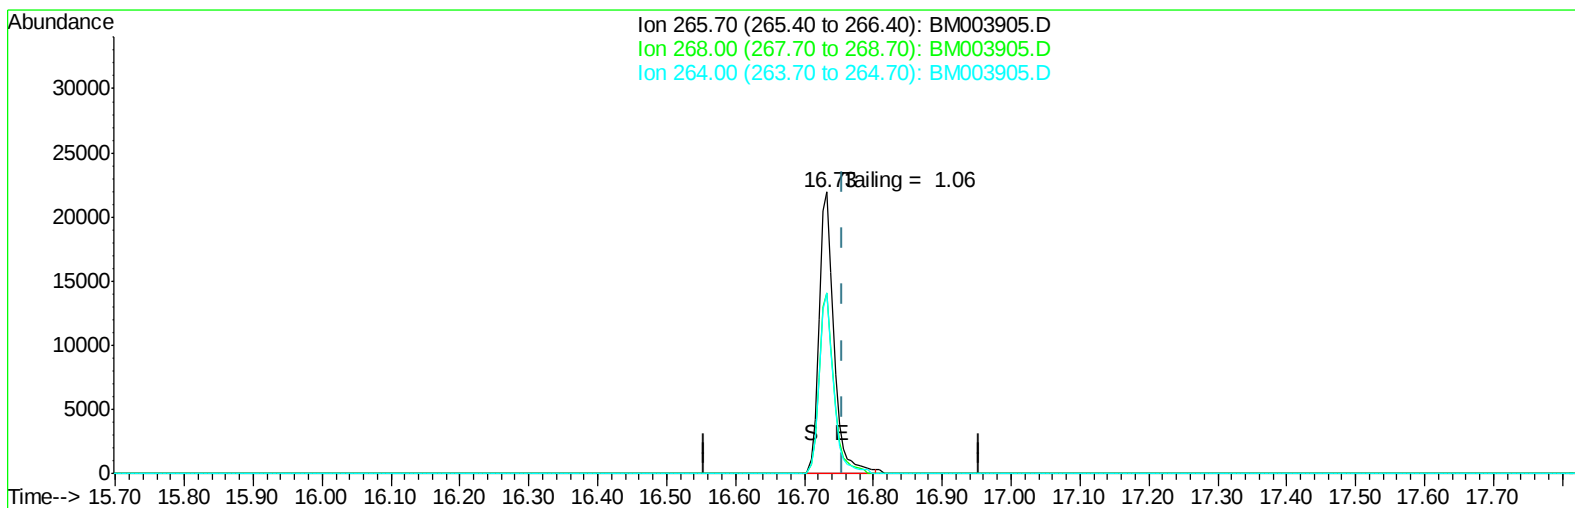

TIC: BM003905.D

(22) Pentachlorophenol




16.733min (-0.022) 0.00ng

response 33250

Ion	Exp%	Act%
265.70	100	100
268.00	78.40	63.94
264.00	57.10	64.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM010216\
 Data File : BM003905.D
 Acq On : 31 Dec 2015 09:11
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 09:45:30 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM122415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 24 10:08:49 2015
 Response via : Initial Calibration

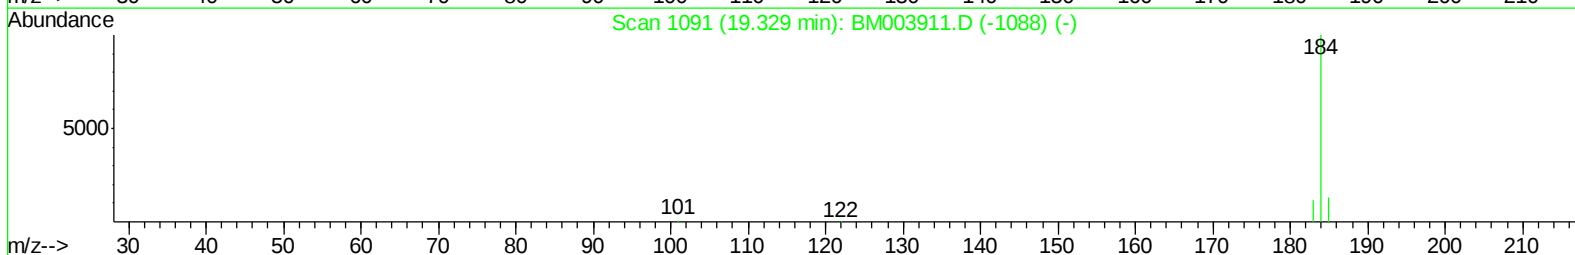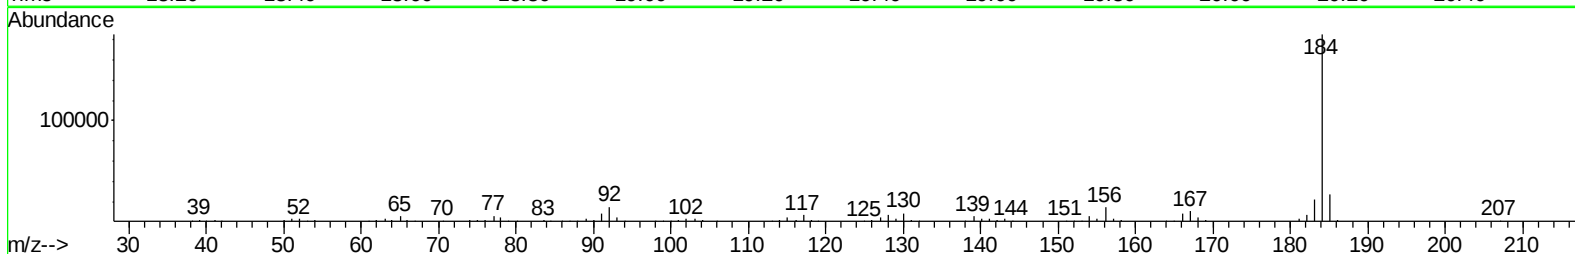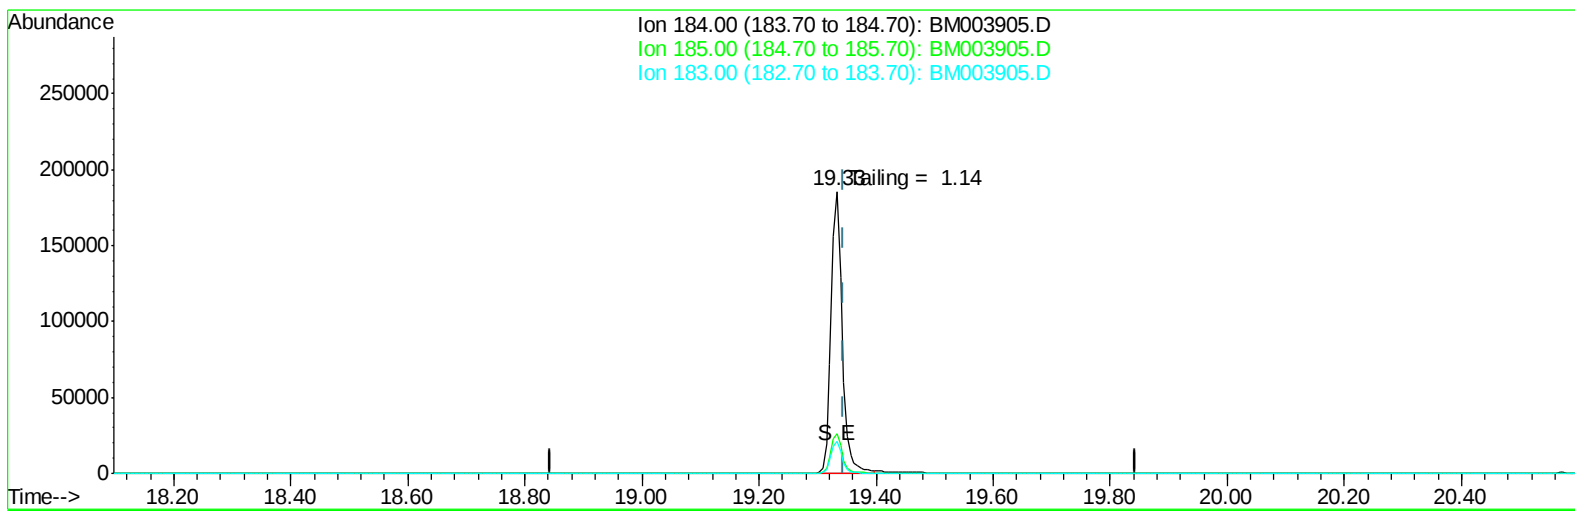

TIC: BM003905.D

(27) Benzidine

19.333min (-0.012) 0.00ng

response 246902

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	14.26
183.00	11.30	11.60
0.00	0.00	0.00