


Data Path : Z:\HPCHEM1\BNA M\Data\BM010216\
 Data File : BM003905.D
 Acq On : 31 Dec 2015 09:11
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM010216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 13:33:21 2016

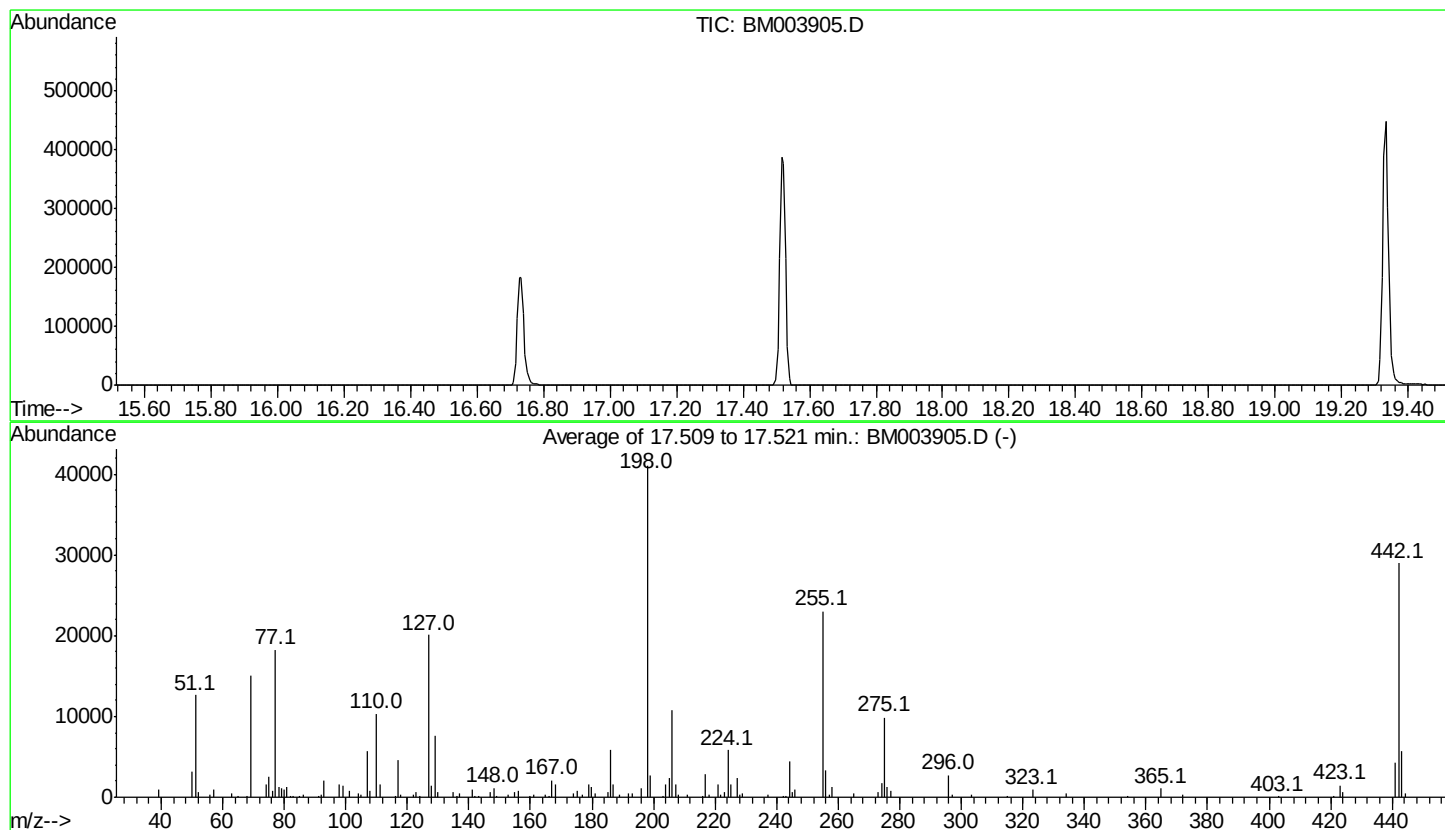

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	12642	PASS
68	69	0.00	2	0.7	102	PASS
69	198	0.00	100	36.7	15078	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	20084	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41045	PASS
199	198	5	9	6.7	2754	PASS
275	198	10	60	24.0	9837	PASS
365	198	1	100	2.6	1069	PASS
441	442	0.01	24	15.0	4335	PASS
442	198	50	100	70.6	28982	PASS
443	442	15	24	19.7	5702	PASS