

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043702.D
 Acq On : 02 Jan 2024 19:54
 Operator : MA/JU
 Sample : 05920-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF58

Quant Time: Jan 02 23:09:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	217096	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	901532	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.592	164	512733	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1049432	20.000	ng/ul	0.00
79) Chrysene-d12	21.521	240	881375	20.000	ng/ul	0.00
88) Perylene-d12	23.938	264	1011784	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	31193	4.670	ng/uL	0.00
4) Pyridine-d5	3.793	84	409532	21.302	ng/ul	0.00
7) Phenol-d5	7.128	99	712096	28.834	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.298	67	393191	25.139	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	520943	27.627	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	549131	28.654	ng/ul	0.00
21) Nitrobenzene-d5	9.133	128	261782	30.012	ng/ul	0.00
24) 2-Nitrophenol-d4	9.851	143	287331	31.882	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.392	165	526831	33.114	ng/ul	0.01
31) 4-Chloroaniline-d4	10.916	131	342183	14.620	ng/ul	0.00
46) Dimethylphthalate-d6	14.015	166	1480203	32.069	ng/ul	0.00
49) Acenaphthylene-d8	14.292	160	1856278	33.902	ng/ul	0.00
54) 4-Nitrophenol-d4	14.810	143	310036	35.490	ng/ul	0.02
60) Fluorene-d10	15.586	176	1362633	35.701	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.709	200	167780	24.174	ng/ul	0.00
73) Anthracene-d10	17.439	188	1857590	31.562	ng/ul	0.00
81) Pyrene-d10	19.733	212	2274866	32.692	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.780	264	2108908	33.777	ng/ul	0.00


Target Compounds					Qvalue	
10) Bis(2-Chloroethyl)ether	7.381	93	20722	1.051	ng/ul#	23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043702.D
Acq On : 02 Jan 2024 19:54
Operator : MA/JU
Sample : 05920-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF58

Quant Time: Jan 02 23:09:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

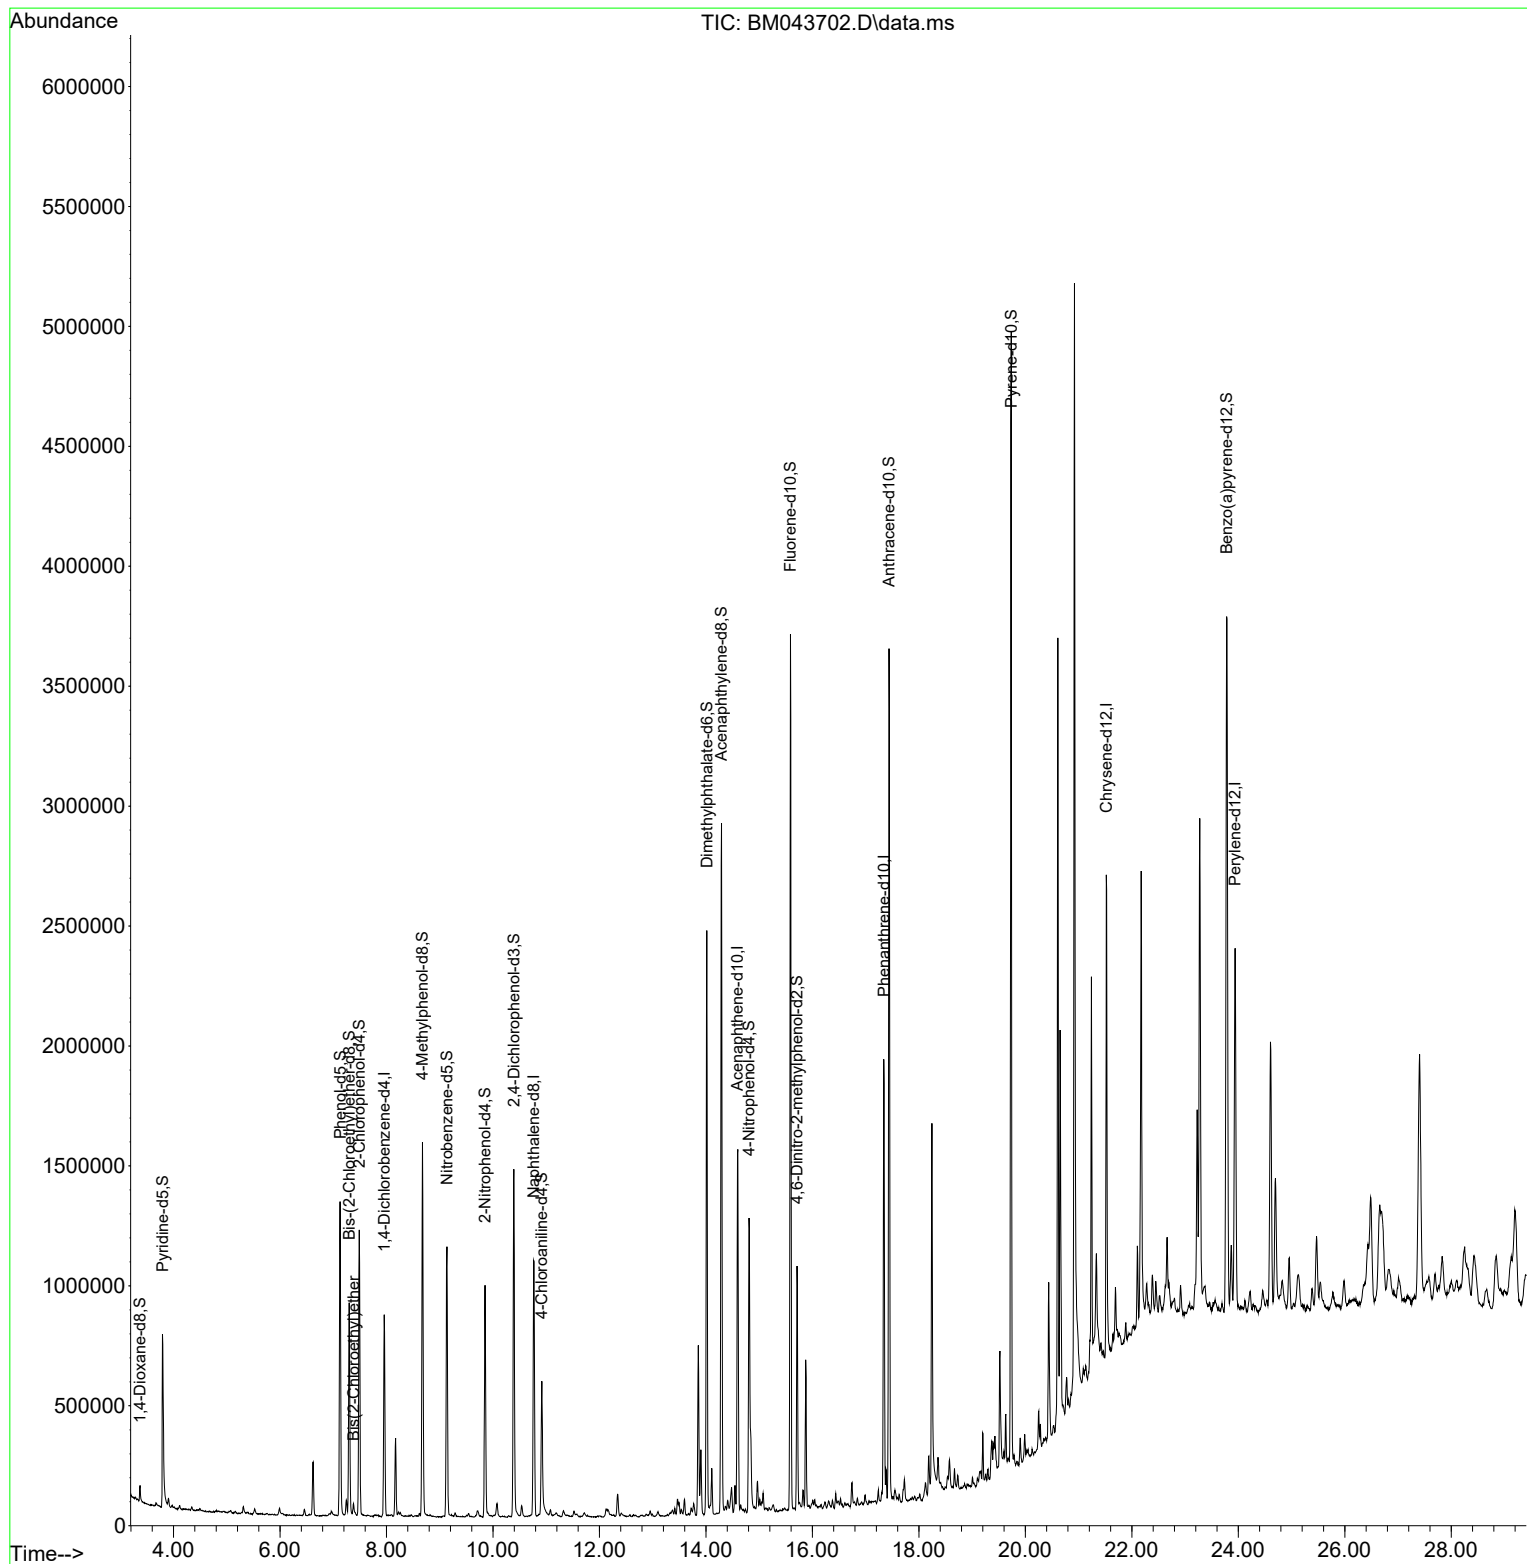

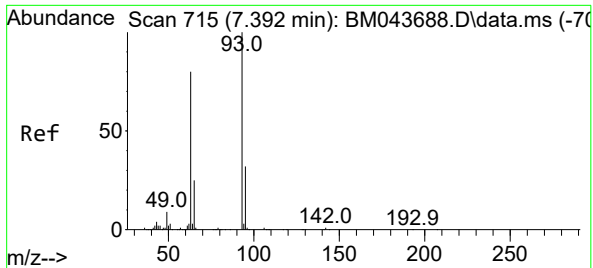

#10
 Bis(2-Chloroethyl)ether
 Concen: 1.051 ng/ul
 RT: 7.381 min Scan# 71
 Delta R.T. -0.012 min
 Lab File: BM043702.D
 Acq: 02 Jan 2024 19:54

Instrument :
 BNA_M
 ClientSampleId :
 GCF58

Tgt Ion:	93	Resp:	20722
Ion	Ratio	Lower	Upper
93	100		
63	3.7	65.8	98.8#
95	4.1	26.2	39.2#

