




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043731.D
 Acq On : 03 Jan 2024 13:55
 Operator : MA/JU
 Sample : 05952-07DL2 30X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF90DL2

Manual IntegrationsAPPROVED

Quant Time: Jan 04 00:29:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/04/2024
 Supervised By :mohammad ahmed 01/05/2024

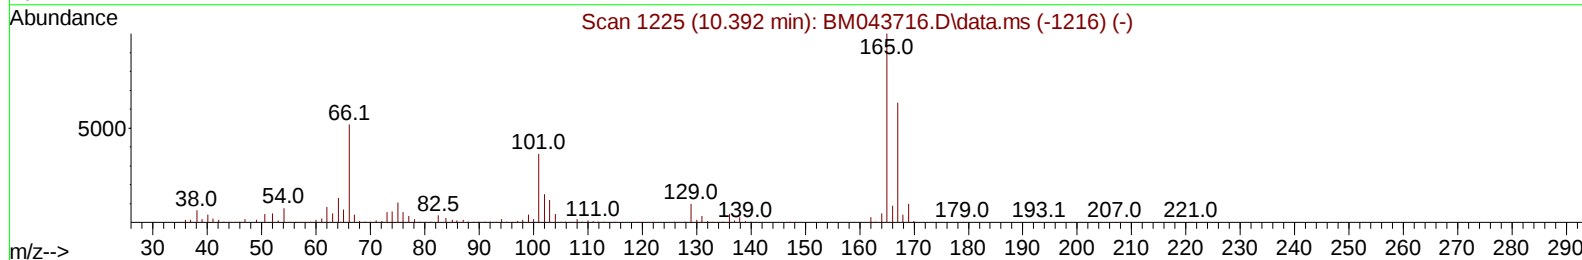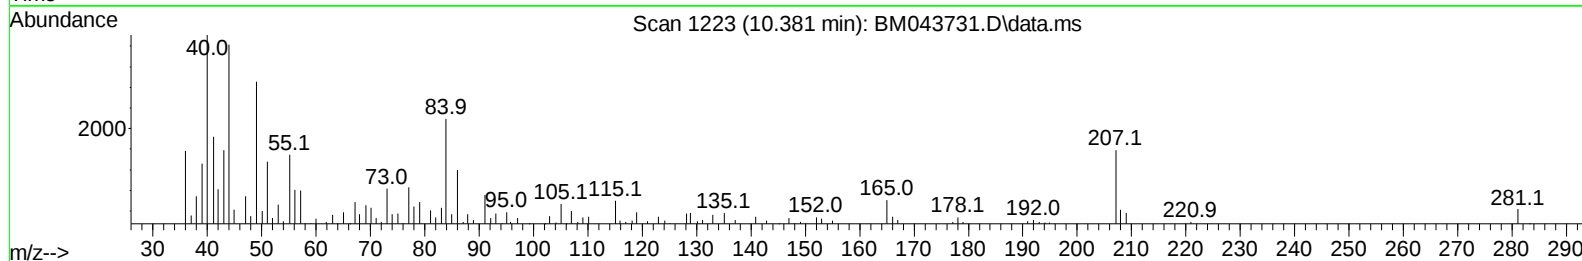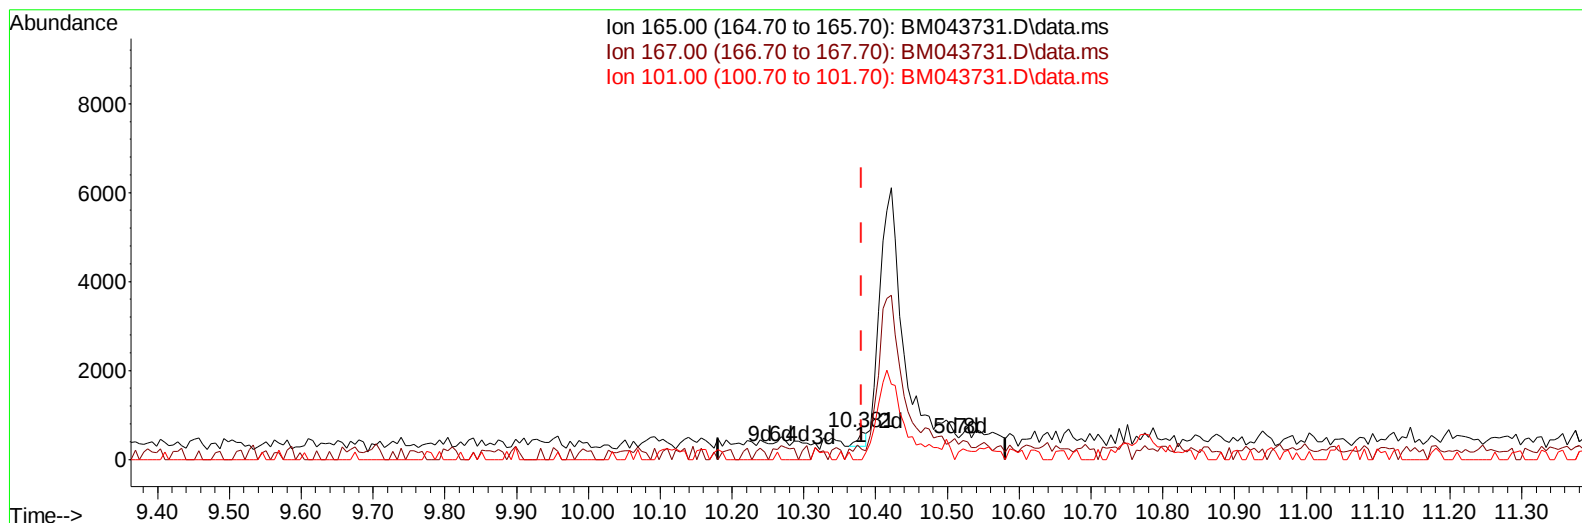

TIC: BM043731.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.381min (-0.000) 0.02 ng/u1

response 302

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	61.80	37.30#
101.00	37.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043731.D
 Acq On : 03 Jan 2024 13:55
 Operator : MA/JU
 Sample : 05952-07DL2 30X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF90DL2

Manual IntegrationsAPPROVED

Quant Time: Jan 04 00:29:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/04/2024
 Supervised By :mohammad ahmed 01/05/2024

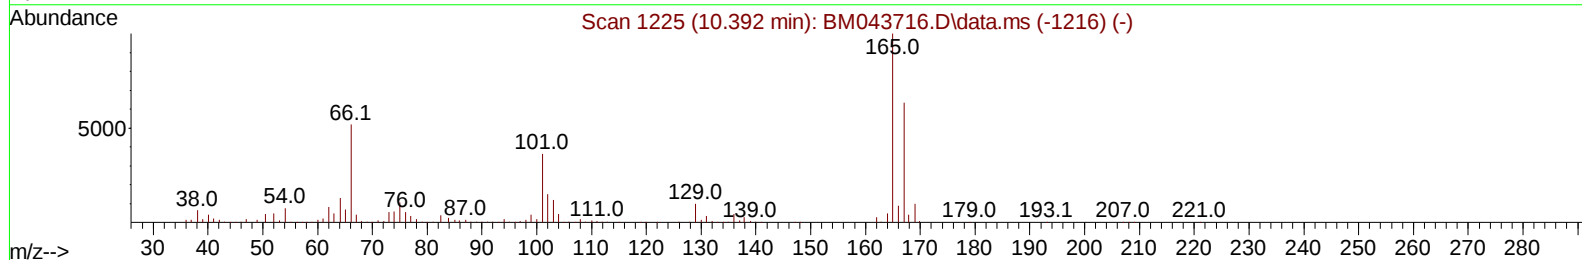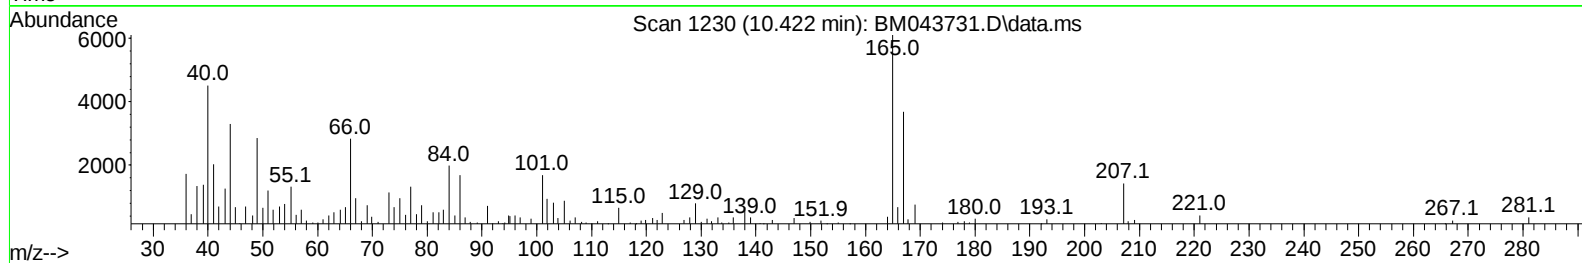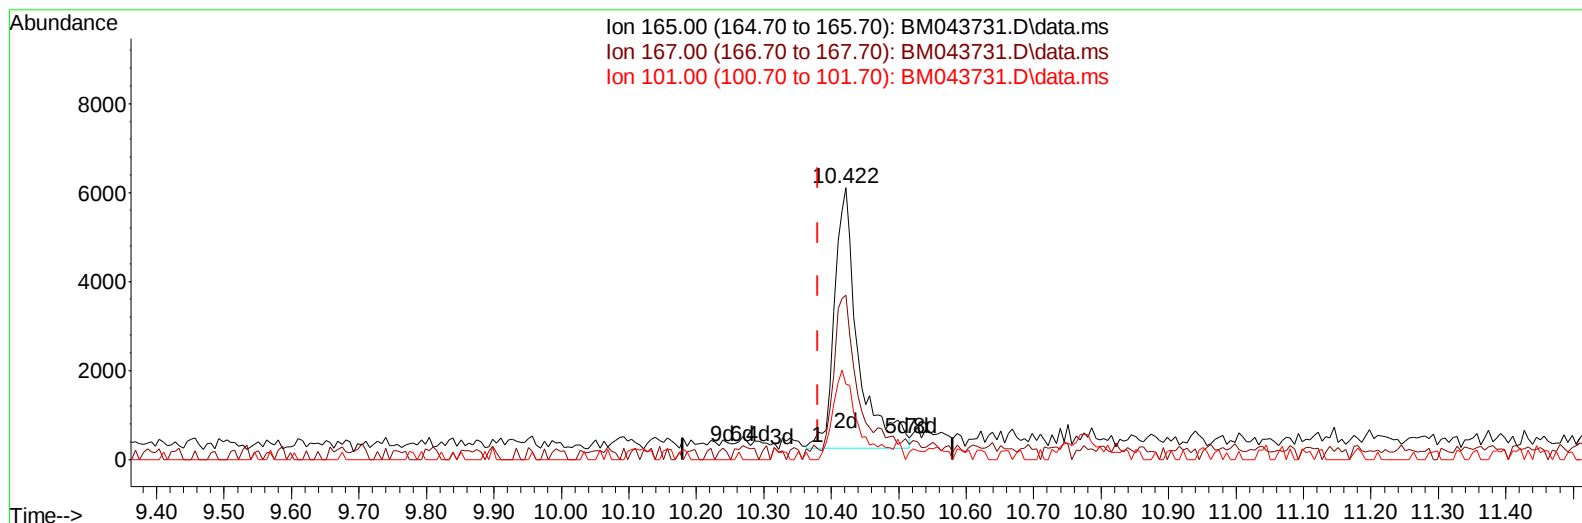

TIC: BM043731.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.422min (+ 0.041) 0.79 ng/ul m

response 14236

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	61.80	60.45
101.00	37.00	27.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043731.D
Acq On : 03 Jan 2024 13:55
Operator : MA/JU
Sample : 05952-07DL2 30X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF90DL2

Manual IntegrationsAPPROVED

Quant Time: Jan 09 09:00:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/04/2024
Supervised By :mohammad ahmed 01/05/2024

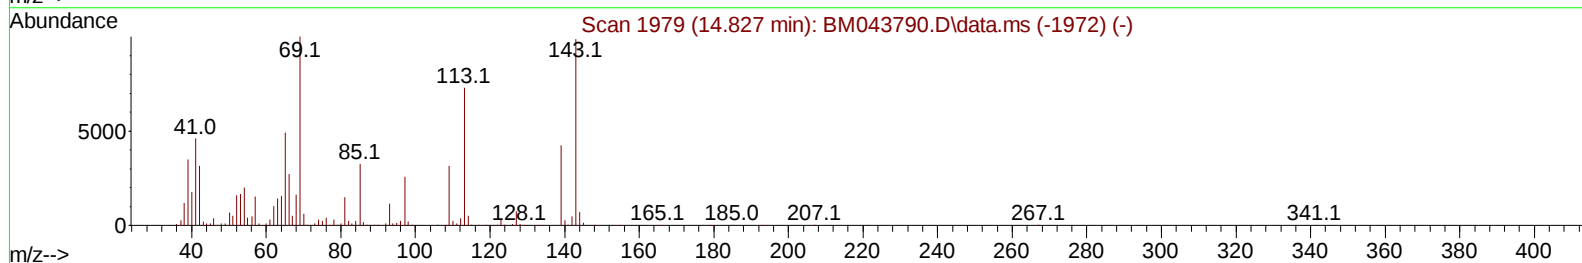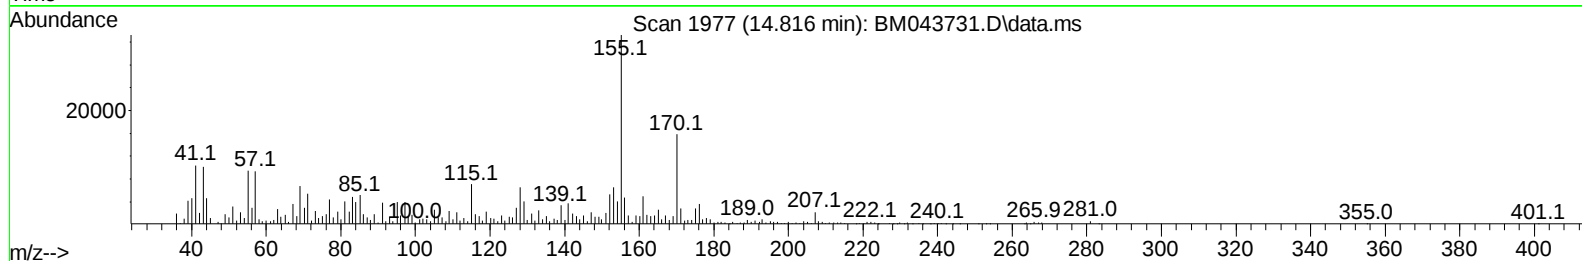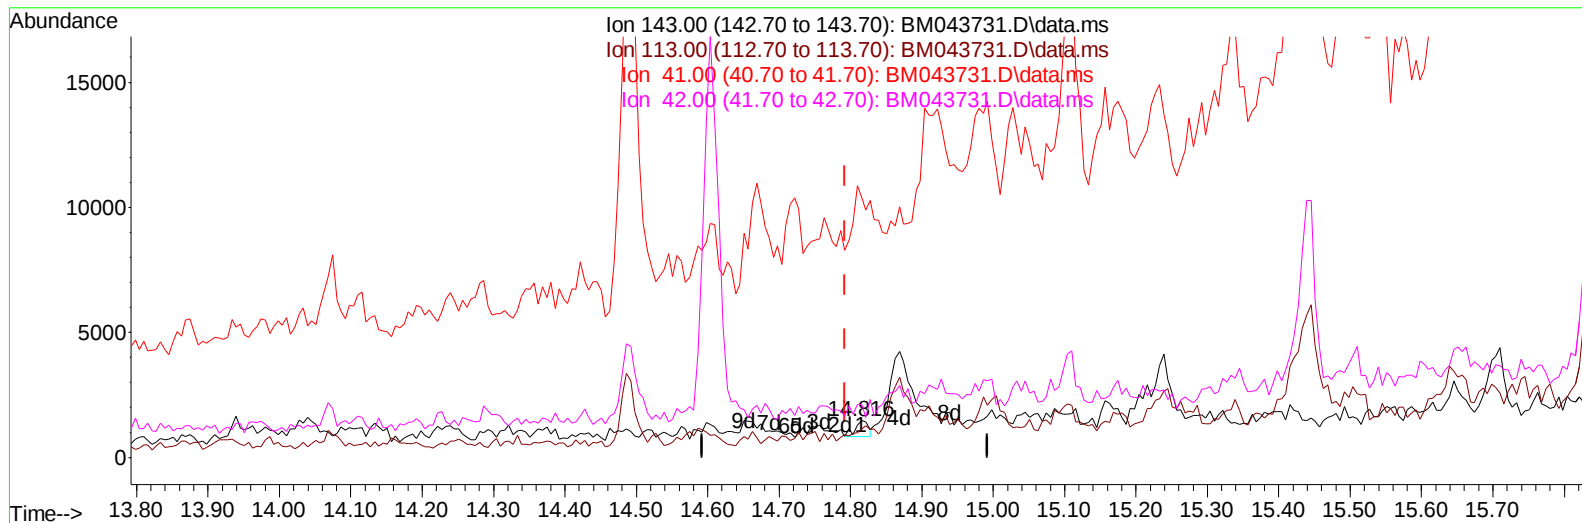

TIC: BM043731.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.816min (+ 0.023) 0.07 ng/u1

response 839

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.00	76.86
41.00	49.10	707.01#
42.00	33.20	143.36#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043731.D
 Acq On : 03 Jan 2024 13:55
 Operator : MA/JU
 Sample : 05952-07DL2 30X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF90DL2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 01/04/2024
 Supervised By :mohammad ahmed 01/05/2024

Quant Time: Jan 04 00:30:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	255348	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	1017641	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.604	164	658004	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.362	188	1367468	20.000	ng/ul	0.02
79) Chrysene-d12	21.545	240	1228019	20.000	ng/ul	0.02
88) Perylene-d12	23.974	264	1411206	20.000	ng/ul	0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	1171	0.149	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.157	99	19324	0.665	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	7.310	67	13743	0.747	ng/ul	0.01
11) 2-Chlorophenol-d4	7.498	132	16676	0.752	ng/ul	0.01
15) 4-Methylphenol-d8	8.704	113	12563	0.557	ng/ul	0.04
21) Nitrobenzene-d5	9.145	128	7955	0.808	ng/ul	0.02
24) 2-Nitrophenol-d4	9.863	143	7682	0.755	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.422	165	14236m	0.793	ng/ul	0.04
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	14.027	166	48180	0.813	ng/ul	0.01
49) Acenaphthylene-d8	14.304	160	62805	0.894	ng/ul	0.02
54) 4-Nitrophenol-d4	14.868	143	9345m	0.834	ng/ul	0.08
60) Fluorene-d10	15.598	176	45918	0.937	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.739	200	3422	0.378	ng/ul	0.03
73) Anthracene-d10	17.457	188	74137	0.967	ng/ul	0.02
81) Pyrene-d10	19.745	212	82444	0.850	ng/ul	0.02
92) Benzo(a)pyrene-d12	23.809	264	75006	0.861	ng/ul	0.04
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.239	232	124246	10.717	ng/ul#	94
71) Pentachlorophenol	17.021	266	8633451	769.414	ng/ul	97
72) Phenanthrene	17.404	178	624609	6.739	ng/ul	98
82) Pyrene	19.780	202	200592	1.625	ng/ul	96
83) Butylbenzylphthalate	20.680	149	60066	1.126	ng/ul#	82
86) Bis(2-ethylhexyl)phtha...	21.450	149	185118	2.437	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043731.D
Acq On : 03 Jan 2024 13:55
Operator : MA/JU
Sample : 05952-07DL2 30X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF90DL2

Manual IntegrationsAPPROVED

Quant Time: Jan 04 00:30:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/04/2024
Supervised By :mohammad ahmed 01/05/2024

