




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043739.D
Acq On : 03 Jan 2024 18:44
Operator : MA/JU
Sample : 05952-08DL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF91DL

Manual IntegrationsAPPROVED

Quant Time: Jan 03 21:54:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/04/2024
Supervised By :mohammad ahmed 01/05/2024

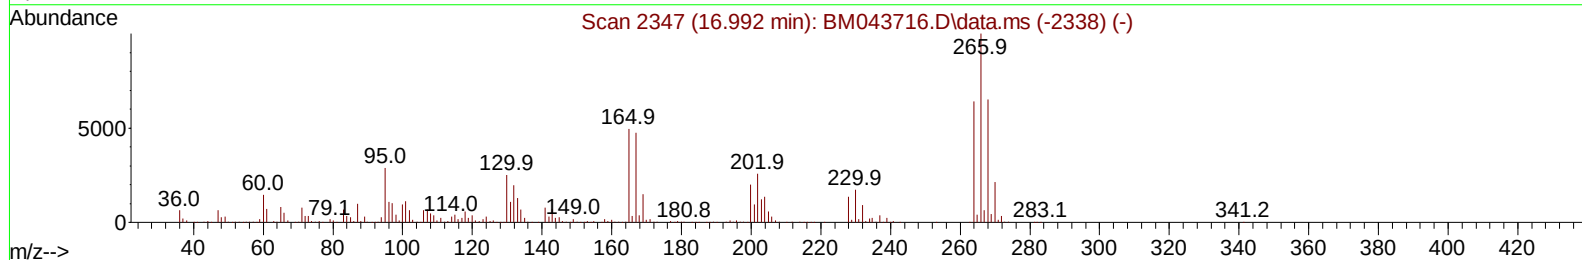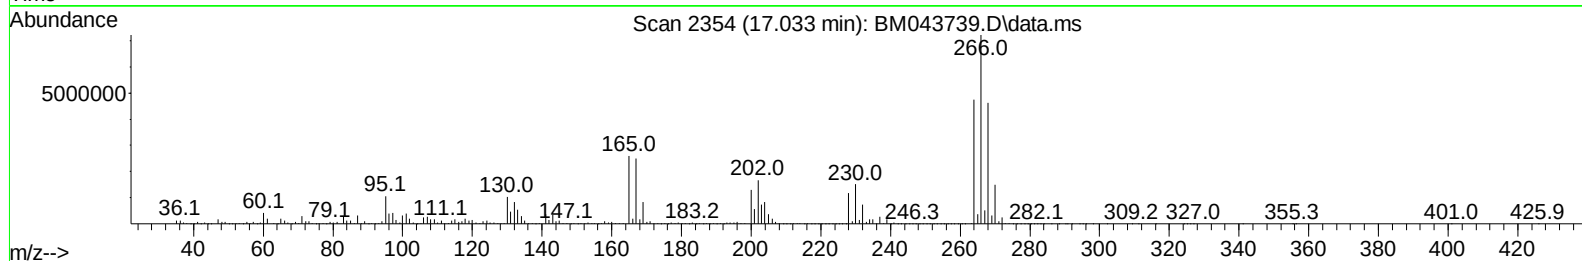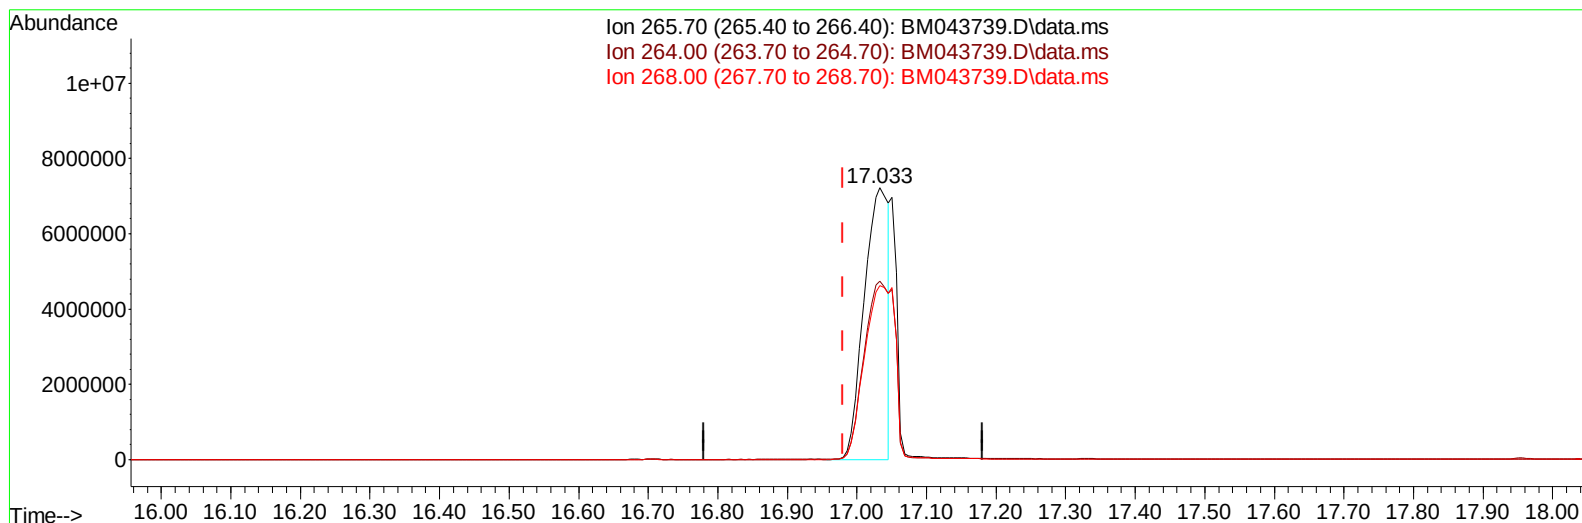

TIC: BM043739.D\data.ms

(71) Pentachlorophenol (C)

17.033min (+ 0.053) 1331.74 ng/uI

response 17369782

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	62.40	65.66
268.00	63.80	64.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043739.D
Acq On : 03 Jan 2024 18:44
Operator : MA/JU
Sample : 05952-08DL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF91DL

Manual IntegrationsAPPROVED

Quant Time: Jan 03 21:54:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/04/2024
Supervised By :mohammad ahmed 01/05/2024

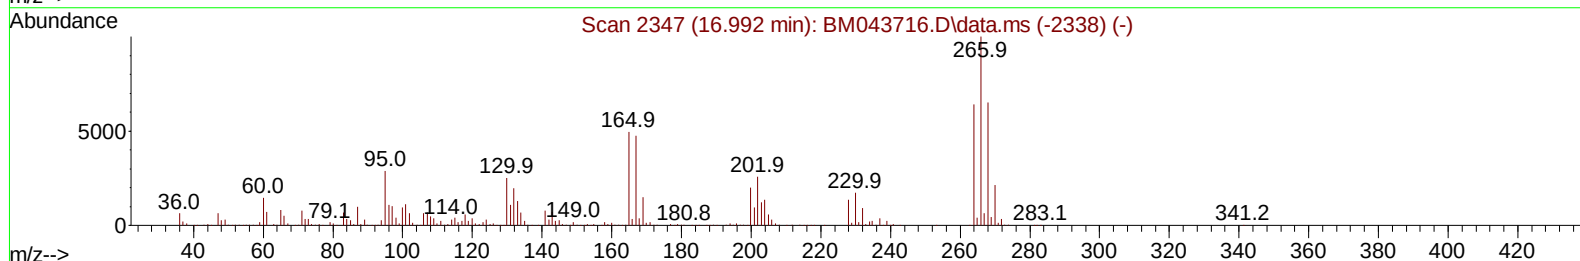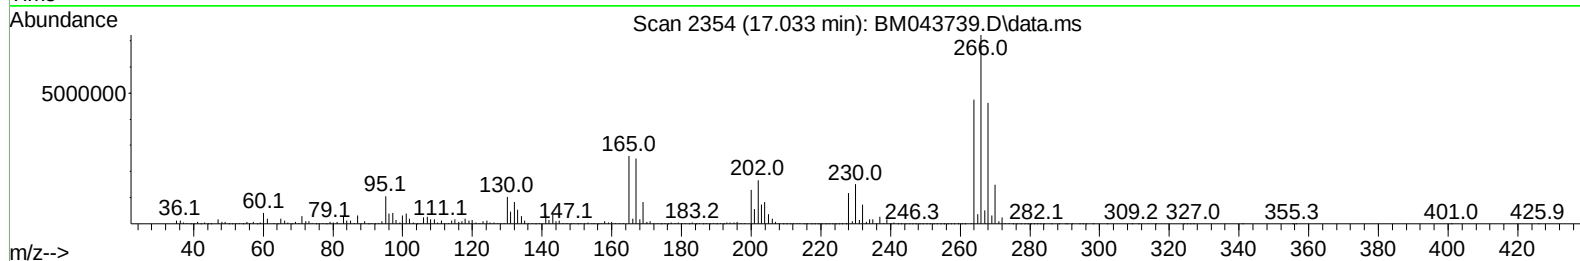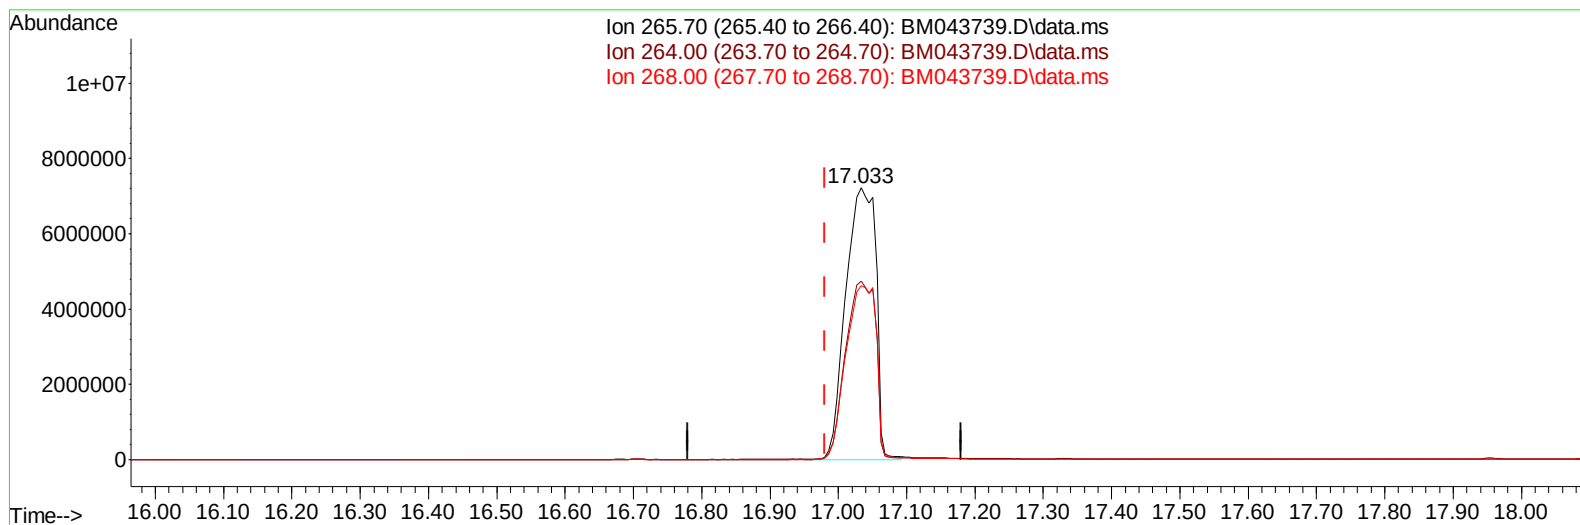

TIC: BM043739.D\data.ms

(71) Pentachlorophenol (C)

17.033min (+ 0.053) 1687.35 ng/ul m

response 22008047

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	62.40	65.66
268.00	63.80	64.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043739.D
 Acq On : 03 Jan 2024 18:44
 Operator : MA/JU
 Sample : 05952-08DL 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF91DL

Manual IntegrationsAPPROVED

Quant Time: Jan 03 22:37:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/04/2024
 Supervised By :mohammad ahmed 01/05/2024

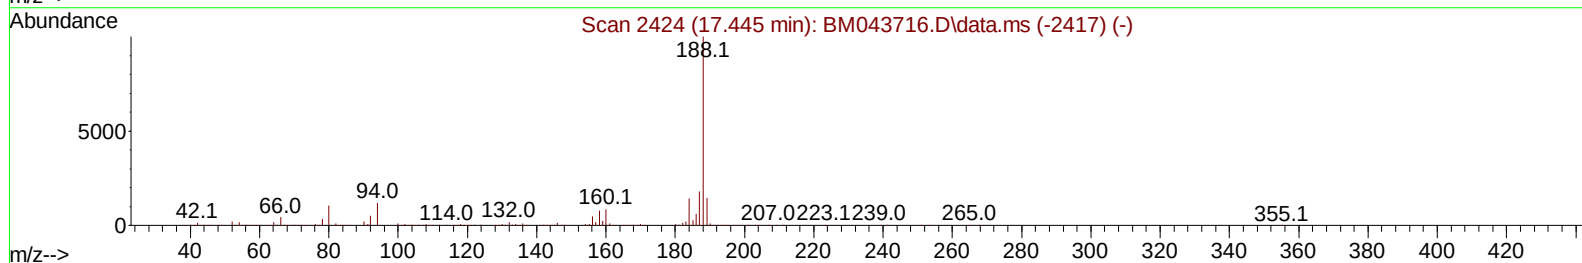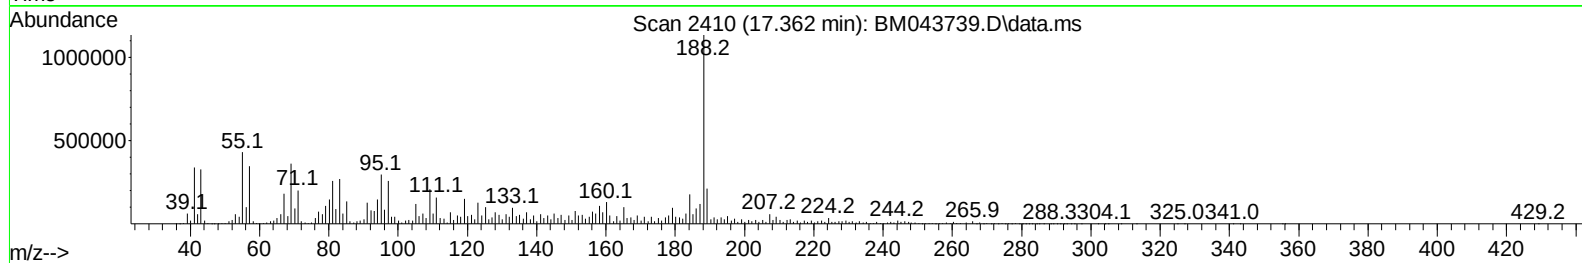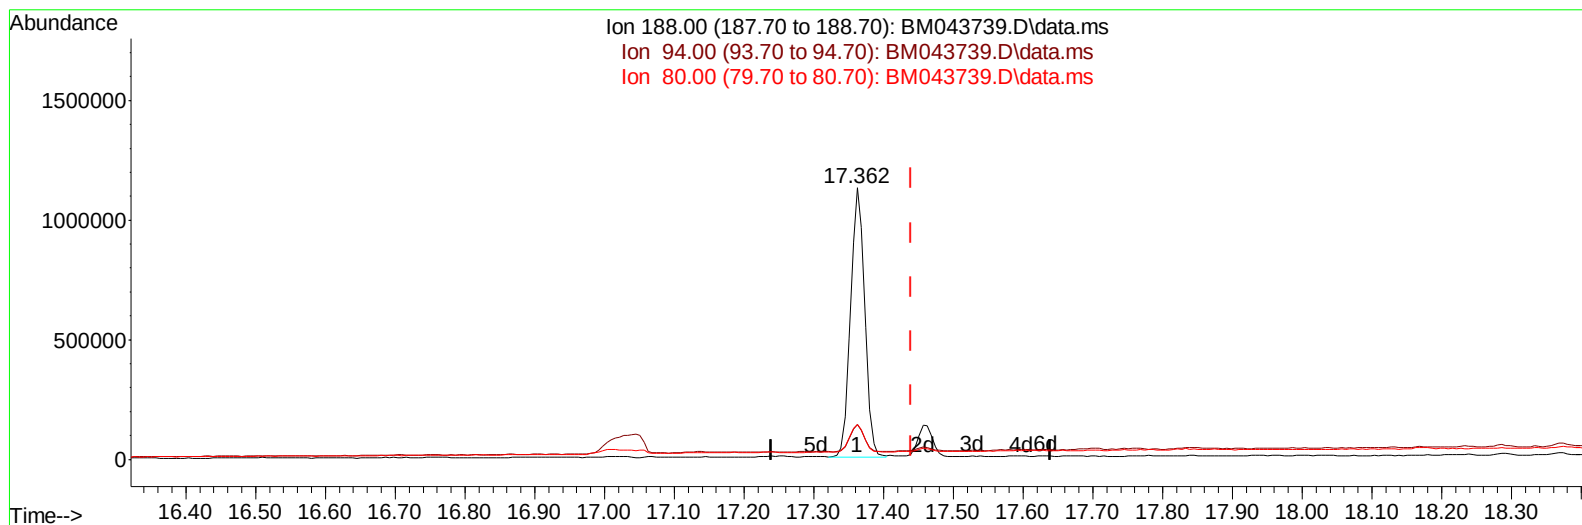

TIC: BM043739.D\data.ms

(73) Anthracene-d10 (S)

17.362min (-0.077) 17.83 ng/ul

response 1589229

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	14.20	12.77
80.00	11.90	12.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043739.D
Acq On : 03 Jan 2024 18:44
Operator : MA/JU
Sample : 05952-08DL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF91DL

Manual IntegrationsAPPROVED

Quant Time: Jan 03 22:37:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/04/2024
Supervised By :mohammad ahmed 01/05/2024

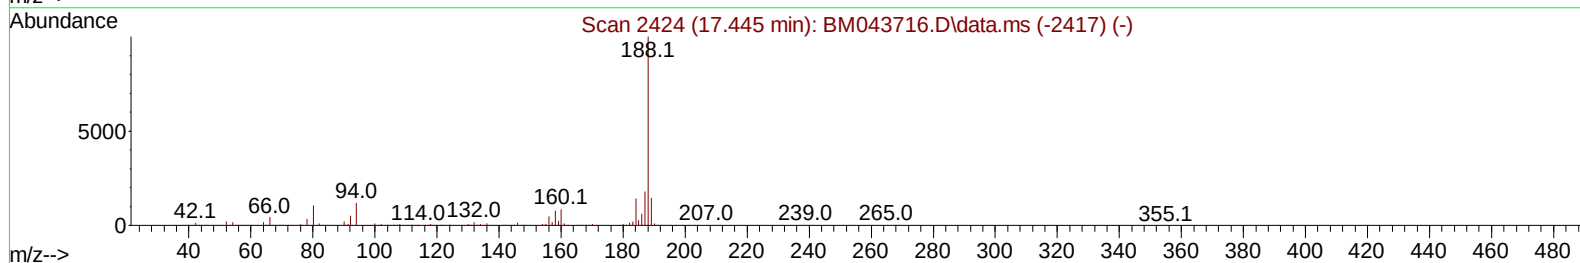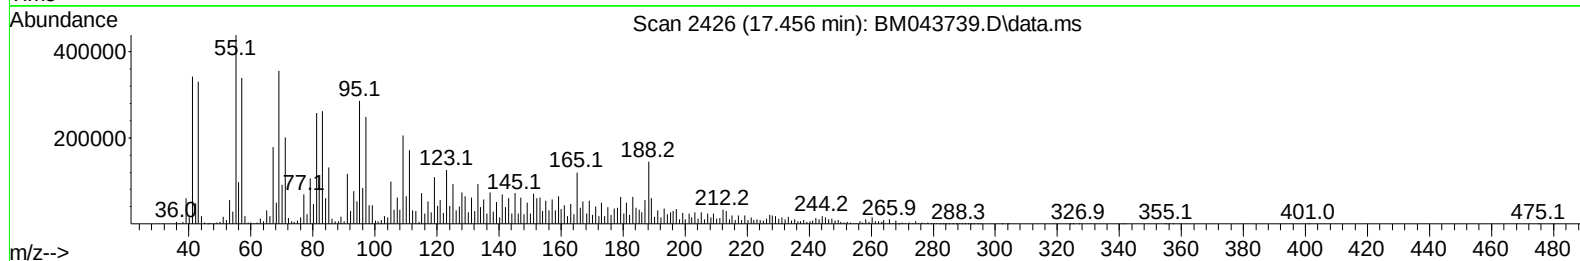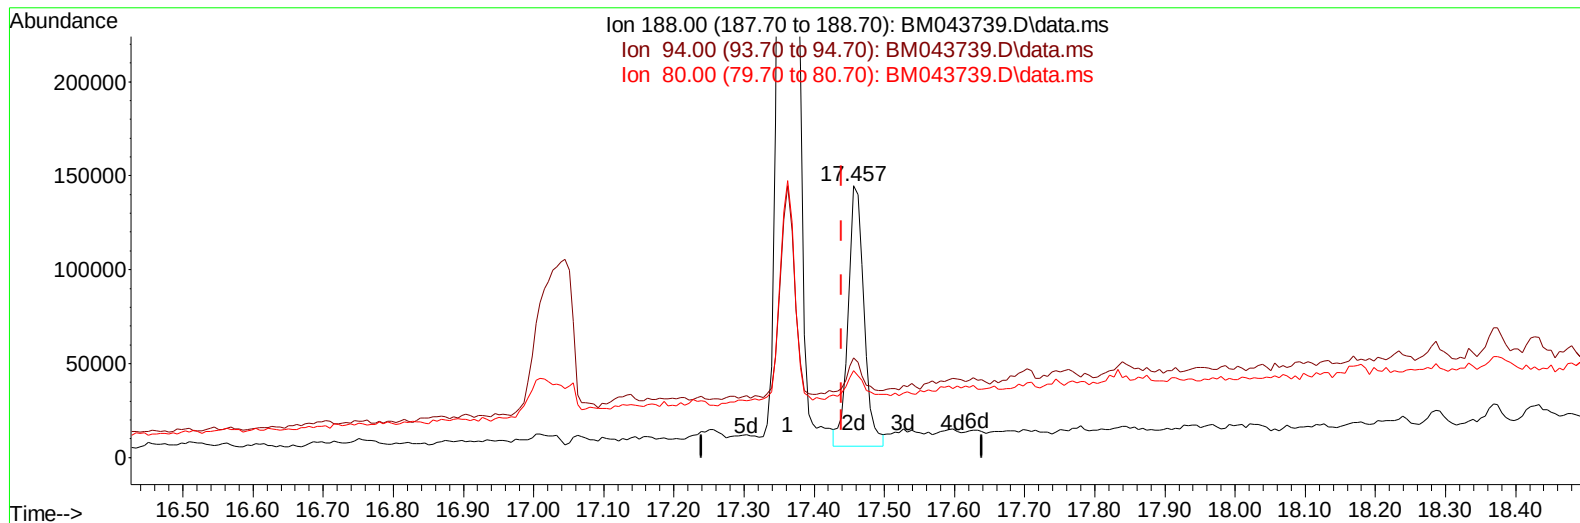

TIC: BM043739.D\data.ms

(73) Anthracene-d10 (S)

17.456min (+ 0.017) 2.46 ng/ul m

response 218955

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	14.20	36.62#
80.00	11.90	31.99#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043739.D
 Acq On : 03 Jan 2024 18:44
 Operator : MA/JU
 Sample : 05952-08DL 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF91DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 01/04/2024
 Supervised By :mohammad ahmed 01/05/2024

Quant Time: Jan 04 03:47:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	281344	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	1102024	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	752596	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.362	188	1589531	20.000	ng/ul	0.02
79) Chrysene-d12	21.539	240	1383110	20.000	ng/ul	0.02
88) Perylene-d12	23.968	264	1434020	20.000	ng/ul	0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	1841	0.213	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.145	99	49871	1.558	ng/ul	0.03
9) Bis-(2-Chloroethyl)eth...	7.304	67	31250	1.542	ng/ul	0.00
11) 2-Chlorophenol-d4	7.492	132	40667	1.664	ng/ul	0.00
15) 4-Methylphenol-d8	8.692	113	32933	1.326	ng/ul	0.02
21) Nitrobenzene-d5	9.145	128	16459	1.544	ng/ul	0.02
24) 2-Nitrophenol-d4	9.863	143	18394	1.670	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.410	165	30583	1.573	ng/ul	0.03
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	14.021	166	127425	1.881	ng/ul	0.00
49) Acenaphthylene-d8	14.298	160	162471	2.022	ng/ul	0.01
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.592	176	116272	2.075	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.456	188	218955m	2.456	ng/ul	0.02
81) Pyrene-d10	19.756	212	232705	2.131	ng/ul	0.03
92) Benzo(a)pyrene-d12	23.803	264	173631	1.962	ng/ul	0.03
Target Compounds						
						Qvalue
58) 2,3,4,6-Tetrachlorophenol	15.233	232	486098	36.659	ng/ul	93
71) Pentachlorophenol	17.033	266	22008047m	1687.351	ng/ul	
74) Anthracene	17.492	178	539999	4.967	ng/ul#	84
82) Pyrene	19.786	202	2184861	15.717	ng/ul#	93
86) Bis(2-ethylhexyl)phtha...	21.450	149	3608442	42.171	ng/ul#	97
87) Chrysene	21.556	228	349555	3.360	ng/ul#	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043739.D
Acq On : 03 Jan 2024 18:44
Operator : MA/JU
Sample : 05952-08DL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF91DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 01/04/2024
Supervised By :mohammad ahmed 01/05/2024

Quant Time: Jan 04 03:47:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

