

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043695.D
 Acq On : 02 Jan 2024 15:05
 Operator : MA/JU
 Sample : 05918-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF23

Quant Time: Jan 02 16:11:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	229082	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	932180	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.592	164	510405	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.339	188	1043916	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	920952	20.000	ng/u1	0.00
88) Perylene-d12	23.938	264	1071438	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	36174	5.132	ng/uL	0.00
4) Pyridine-d5	3.799	84	457035	22.529	ng/u1	0.01
7) Phenol-d5	7.128	99	744073	28.552	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.298	67	445383	26.986	ng/u1	0.00
11) 2-Chlorophenol-d4	7.487	132	566630	28.478	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	533788	26.396	ng/u1	0.00
21) Nitrobenzene-d5	9.134	128	279481	30.988	ng/u1	0.00
24) 2-Nitrophenol-d4	9.851	143	308249	33.078	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.392	165	522176	31.742	ng/u1	0.01
31) 4-Chloroaniline-d4	10.916	131	53672	2.218	ng/u1	0.00
46) Dimethylphthalate-d6	14.016	166	1405750	30.595	ng/u1	0.00
49) Acenaphthylene-d8	14.292	160	1808441	33.179	ng/u1	0.00
54) 4-Nitrophenol-d4	14.810	143	269924	31.039	ng/u1	0.02
60) Fluorene-d10	15.586	176	1296917	34.135	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.715	200	157304	22.784	ng/u1	0.00
73) Anthracene-d10	17.439	188	1927363	32.921	ng/u1	0.00
81) Pyrene-d10	19.733	212	2171153	29.861	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.786	264	2172560	32.859	ng/u1	0.01
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.986	266	164259	19.176	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043695.D
Acq On : 02 Jan 2024 15:05
Operator : MA/JU
Sample : 05918-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF23

Quant Time: Jan 02 16:11:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

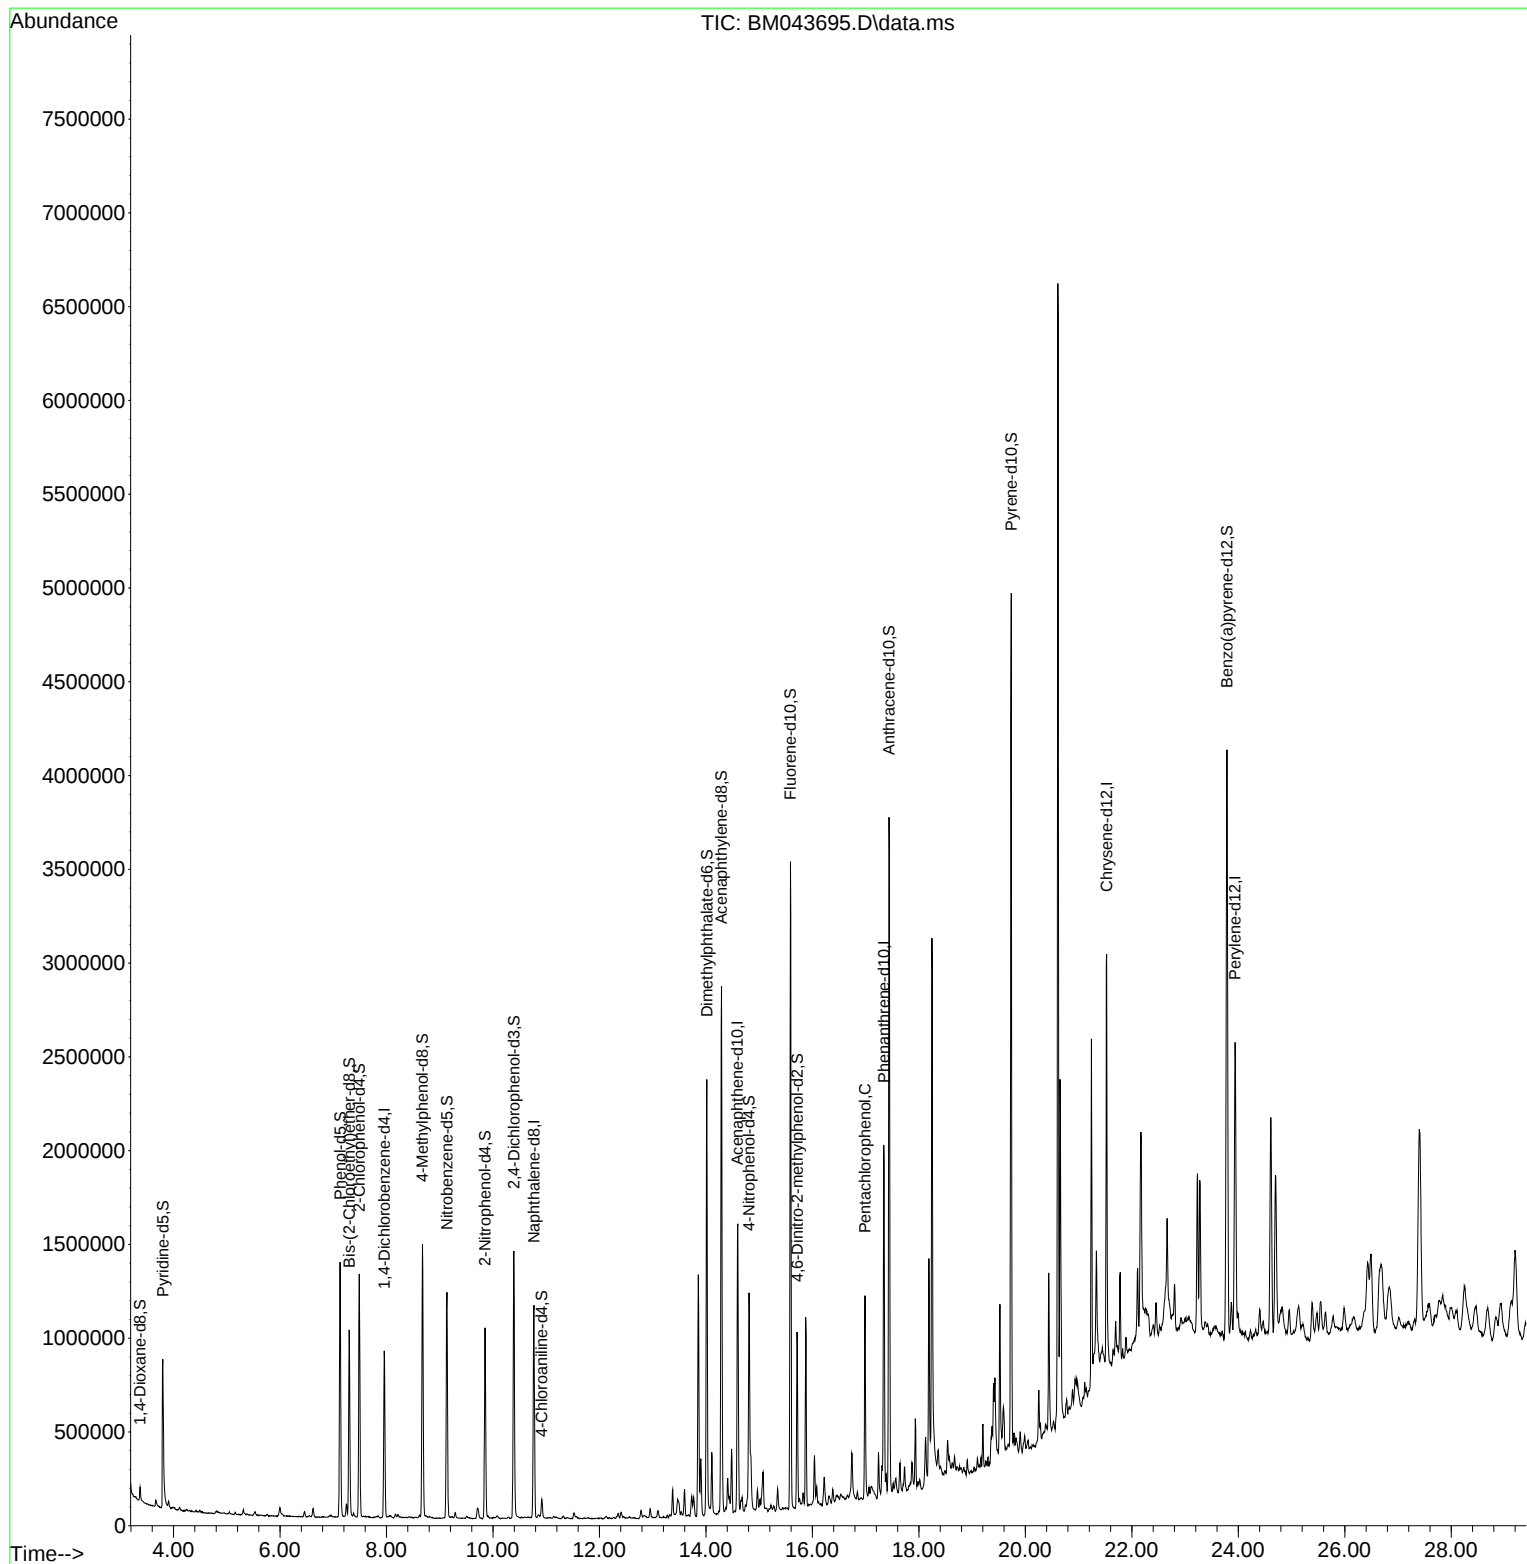

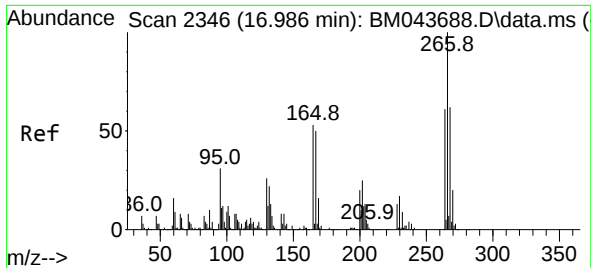

#71
Pentachlorophenol
Concen: 19.176 ng/ul
RT: 16.986 min Scan# 21
Delta R.T. 0.006 min
Lab File: BM043695.D
Acq: 02 Jan 2024 15:05

Instrument :
BNA_M
ClientSampleId :
GCF23

Tgt Ion:	266	Resp:	164259
Ion	Ratio	Lower	Upper
266	100		
264	63.6	49.9	74.9
268	63.5	51.0	76.6

