

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043710.D
 Acq On : 03 Jan 2024 00:42
 Operator : MA/JU
 Sample : 05919-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF39

Quant Time: Jan 03 01:32:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	263824	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	1051809	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.598	164	579033	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.345	188	1174604	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	1029350	20.000	ng/u1	0.00
88) Perylene-d12	23.944	264	1160307	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	48352	5.957	ng/uL	0.00
4) Pyridine-d5	3.799	84	627045	26.839	ng/u1	0.01
7) Phenol-d5	7.134	99	932814	31.081	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.298	67	565276	29.740	ng/u1	0.00
11) 2-Chlorophenol-d4	7.493	132	732546	31.968	ng/u1	0.00
15) 4-Methylphenol-d8	8.681	113	631347	27.109	ng/u1	0.01
21) Nitrobenzene-d5	9.134	128	352521	34.641	ng/u1	0.00
24) 2-Nitrophenol-d4	9.851	143	387575	36.860	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.392	165	653123	35.187	ng/u1	0.01
31) 4-Chloroaniline-d4	10.928	131	4876	0.179	ng/u1	0.02
46) Dimethylphthalate-d6	14.016	166	1671089	32.059	ng/u1	0.00
49) Acenaphthylene-d8	14.292	160	2137638	34.571	ng/u1	0.00
54) 4-Nitrophenol-d4	14.821	143	362085	36.702	ng/u1	0.03
60) Fluorene-d10	15.592	176	1518689	35.234	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	167376	21.546	ng/u1	0.00
73) Anthracene-d10	17.445	188	2182865	33.137	ng/u1	0.00
81) Pyrene-d10	19.733	212	2456804	30.231	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.791	264	2399278	33.508	ng/u1	0.02
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.992	266	116146	12.051	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043710.D
Acq On : 03 Jan 2024 00:42
Operator : MA/JU
Sample : 05919-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF39

Quant Time: Jan 03 01:32:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

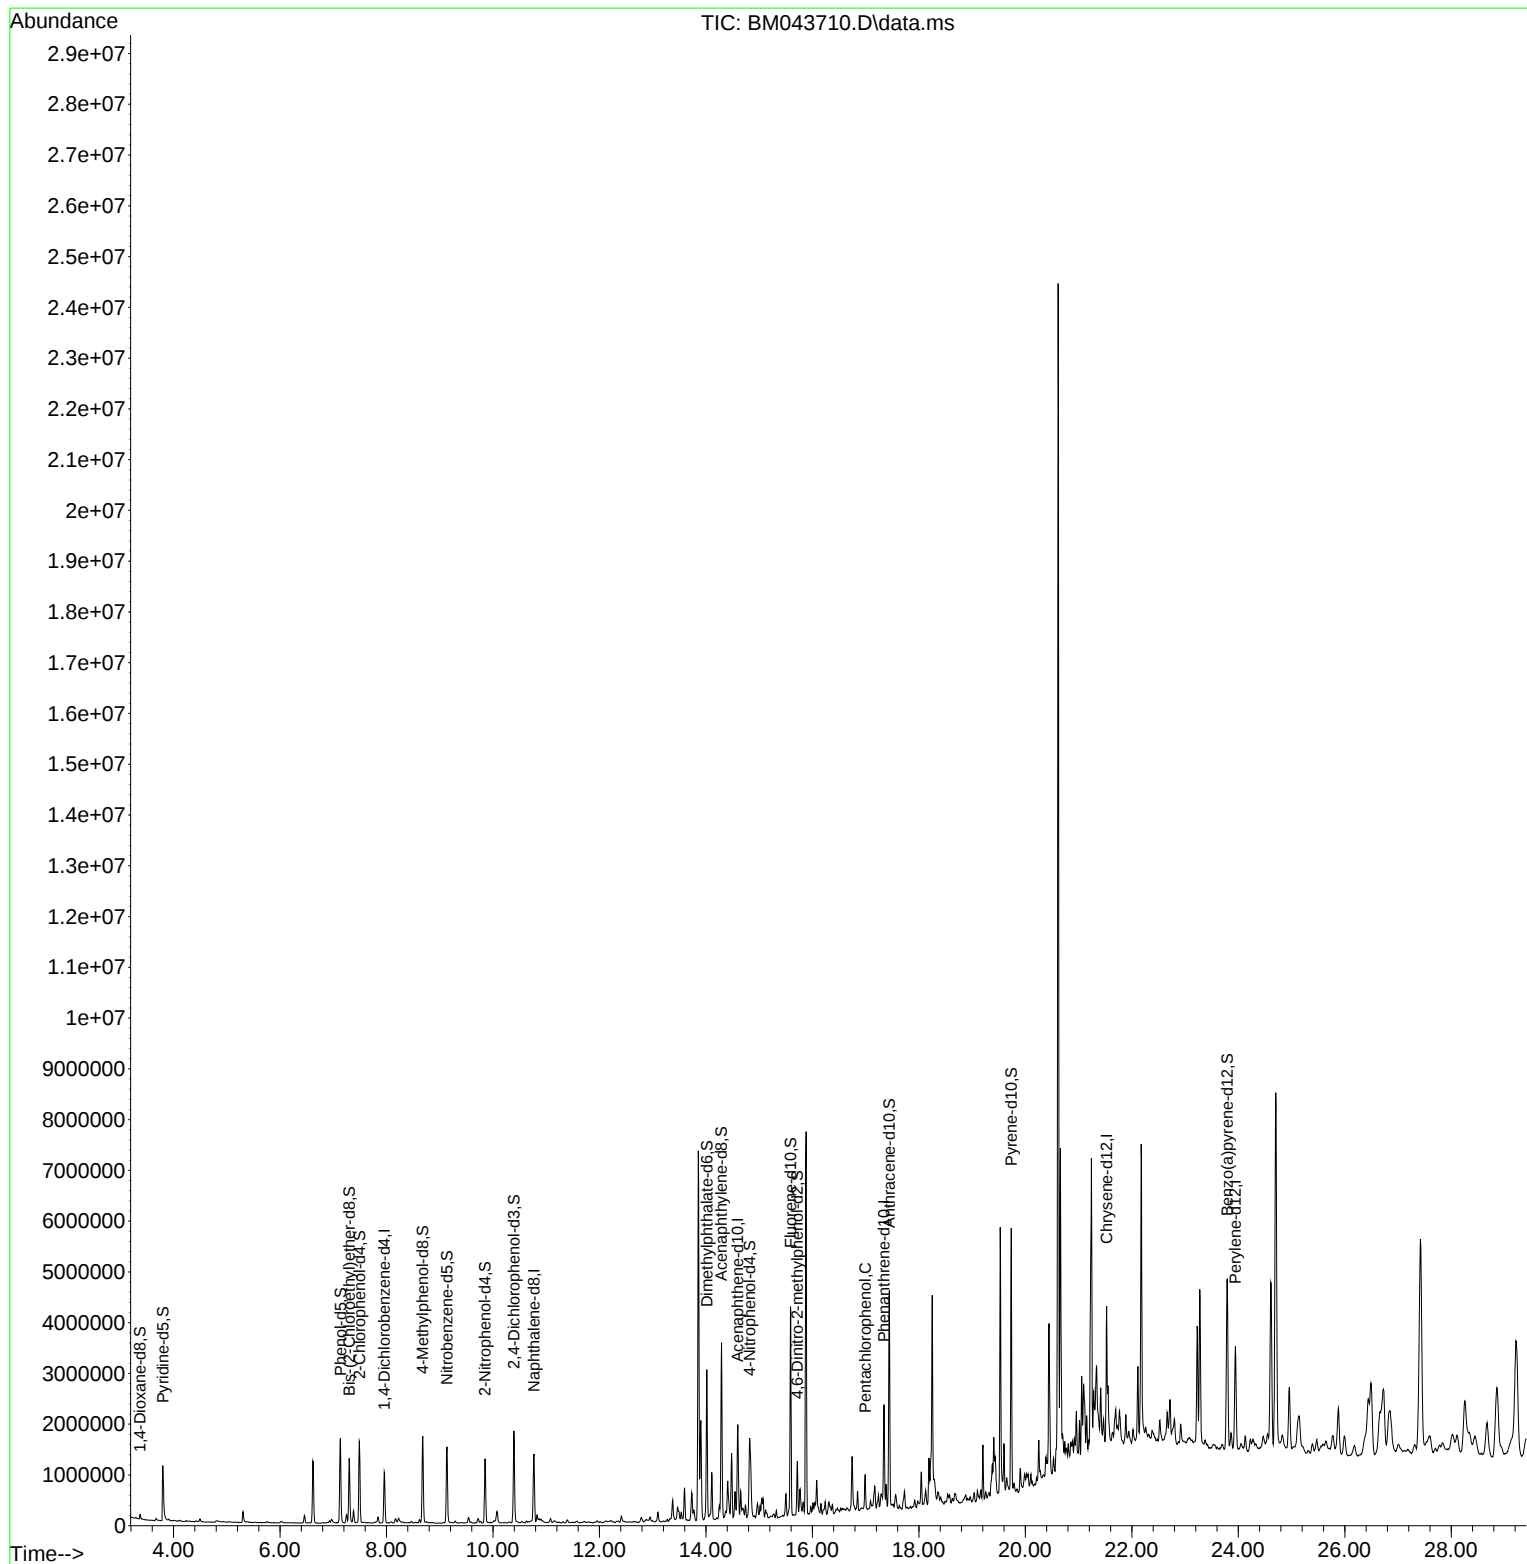

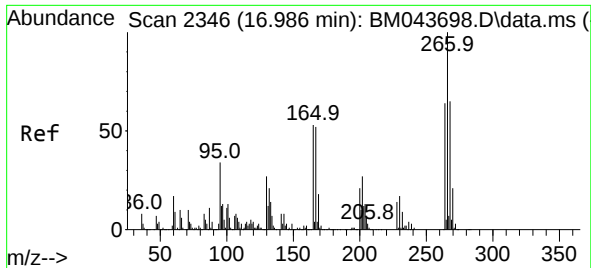

#71
 Pentachlorophenol
 Concen: 12.051 ng/ul
 RT: 16.992 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: BM043710.D
 Acq: 03 Jan 2024 00:42

Instrument :
 BNA_M
 ClientSampleId :
 GCF39

Tgt Ion:266 Resp: 116146
 Ion Ratio Lower Upper
 266 100
 264 59.3 49.9 74.9
 268 63.1 51.0 76.6

