

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043715.D
 Acq On : 03 Jan 2024 03:42
 Operator : MA/JU
 Sample : 05919-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF38

Quant Time: Jan 03 04:50:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	162653	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	718702	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.598	164	439805	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.345	188	936197	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	817619	20.000	ng/u1	0.00
88) Perylene-d12	23.944	264	925700	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	18855	3.768	ng/uL	0.00
4) Pyridine-d5	3.799	84	216657	15.042	ng/u1	0.01
7) Phenol-d5	7.134	99	444488	24.022	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.298	67	257255	21.953	ng/u1	0.00
11) 2-Chlorophenol-d4	7.492	132	337550	23.893	ng/u1	0.00
15) 4-Methylphenol-d8	8.681	113	302980	21.101	ng/u1	0.01
21) Nitrobenzene-d5	9.133	128	167932	24.151	ng/u1	0.00
24) 2-Nitrophenol-d4	9.851	143	186449	25.951	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.398	165	326276	25.725	ng/u1	0.02
31) 4-Chloroaniline-d4	10.922	131	208300	11.163	ng/u1	0.01
46) Dimethylphthalate-d6	14.015	166	940178	23.747	ng/u1	0.00
49) Acenaphthylene-d8	14.292	160	1182292	25.173	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	213223	28.455	ng/u1	0.04
60) Fluorene-d10	15.592	176	870873	26.601	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.715	200	99669	16.097	ng/u1	0.00
73) Anthracene-d10	17.445	188	1239840	23.614	ng/u1	0.00
81) Pyrene-d10	19.733	212	1446717	22.412	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.791	264	1378052	24.124	ng/u1	0.02
Target Compounds						
71) Pentachlorophenol	16.998	266	68228	8.882	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043715.D
Acq On : 03 Jan 2024 03:42
Operator : MA/JU
Sample : 05919-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF38

Quant Time: Jan 03 04:50:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

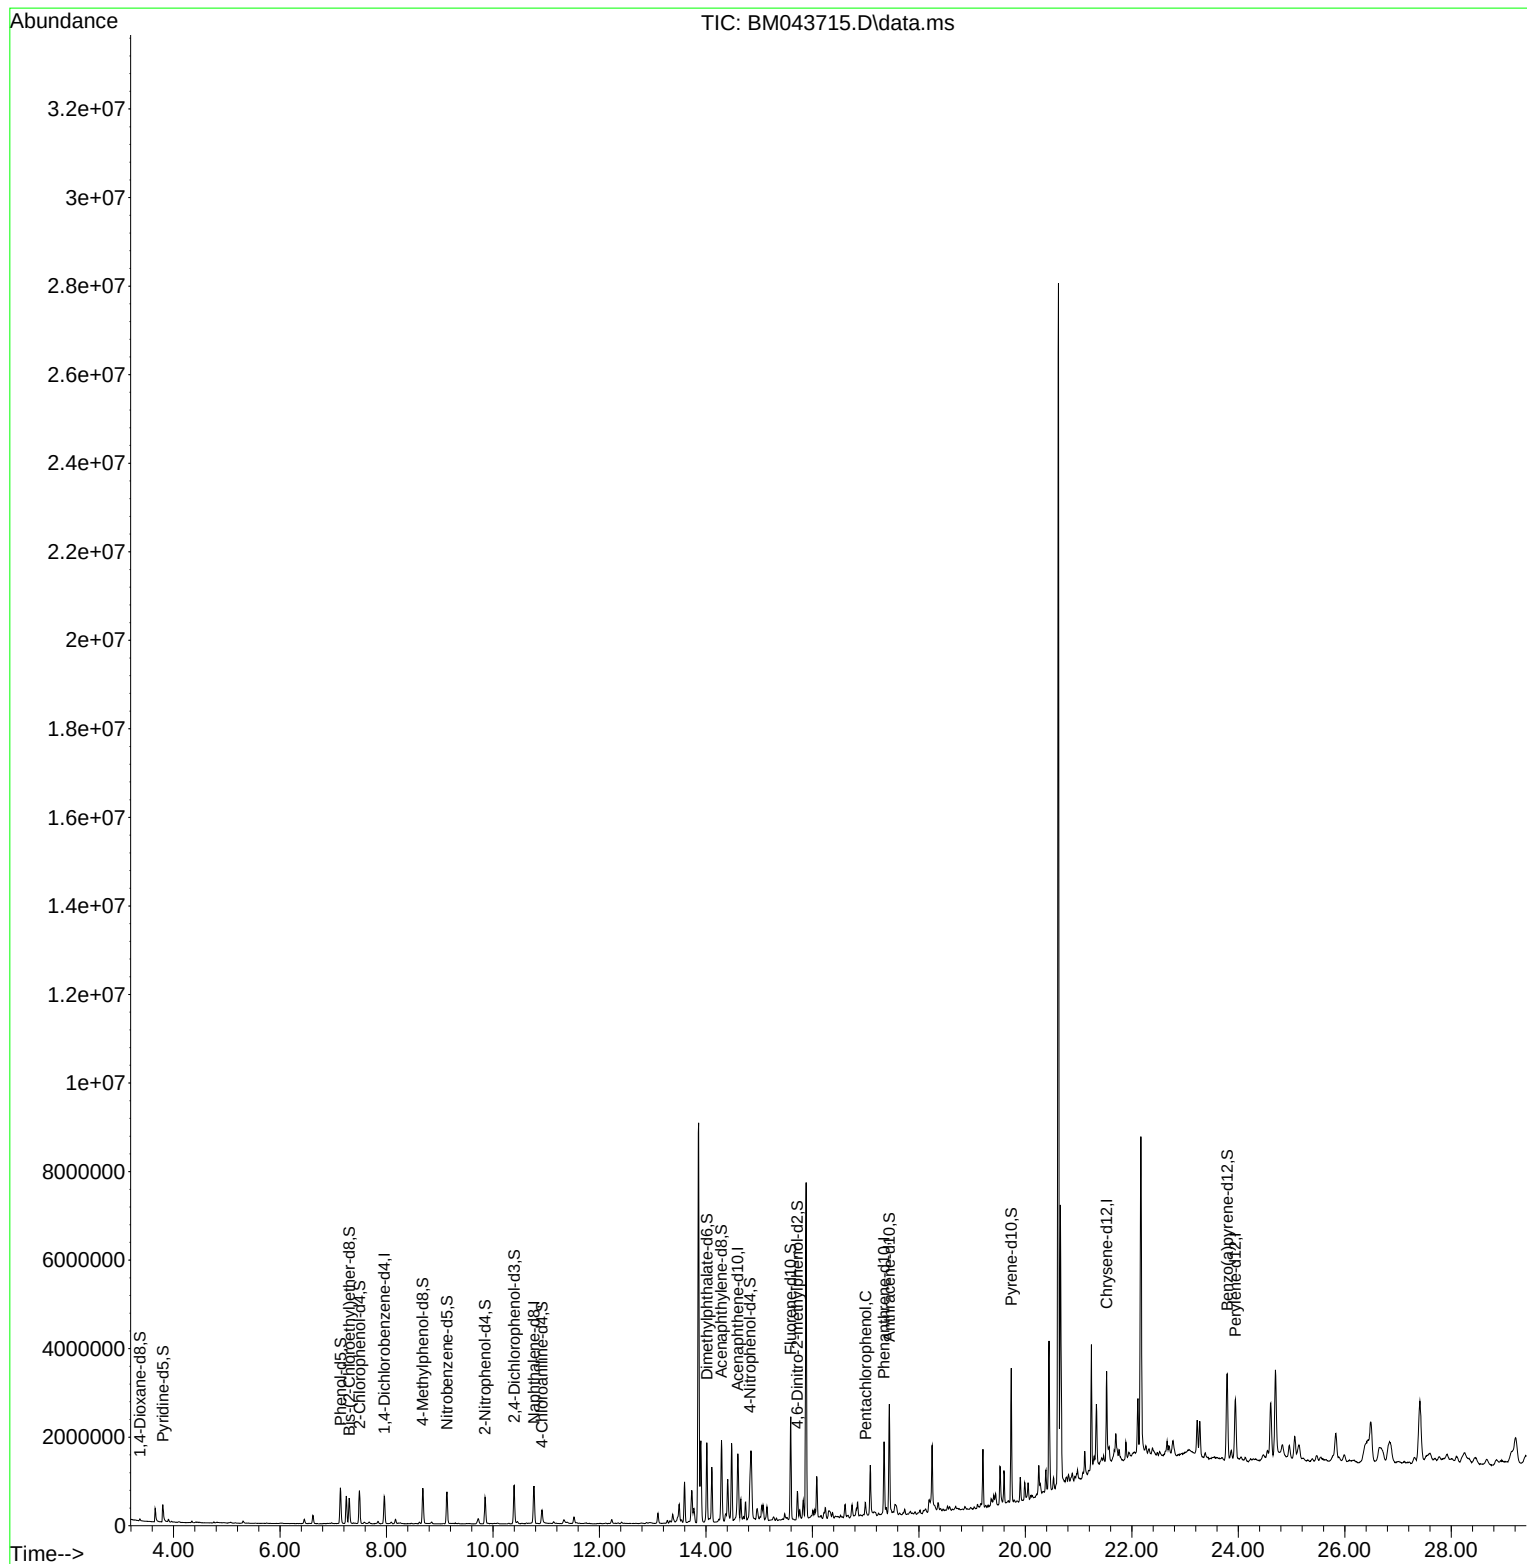

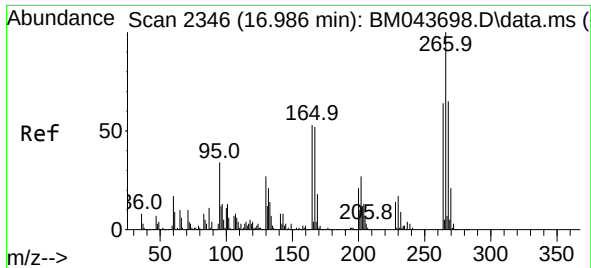

#71
 Pentachlorophenol
 Concen: 8.882 ng/ul
 RT: 16.998 min Scan# 21
 Delta R.T. 0.017 min
 Lab File: BM043715.D
 Acq: 03 Jan 2024 03:42

Instrument :
 BNA_M
 ClientSampleId :
 GCF38

Tgt Ion:266 Resp: 68228
 Ion Ratio Lower Upper
 266 100
 264 61.4 49.9 74.9
 268 61.1 51.0 76.6

