

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043689.D
 Acq On : 02 Jan 2024 11:29
 Operator : MA/JU
 Sample : PB158064BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	41	rVB	75365	110199	2.47%	0.224%
2	3.793	99	103	118	rBV	816828	1342091	30.05%	2.725%
3	7.122	661	669	678	rBV	978958	1567722	35.10%	3.183%
4	7.299	692	699	709	rBV	746759	1193804	26.73%	2.424%
5	7.487	724	731	740	rBV	965505	1523540	34.11%	3.093%
6	7.957	804	811	819	rBV	720753	1138569	25.49%	2.311%
7	8.669	925	932	943	rBV	1110160	1787743	40.03%	3.629%
8	9.128	1003	1010	1020	rBV	842303	1456615	32.61%	2.957%
9	9.851	1125	1133	1142	rBV	703096	1173132	26.27%	2.382%
10	10.387	1215	1224	1239	rBV	957572	1701557	38.10%	3.454%
11	10.763	1280	1288	1301	rBV	937498	1600784	35.84%	3.250%
12	10.910	1306	1313	1332	rBV	1013441	1831293	41.00%	3.718%
13	12.351	1553	1558	1563	rBV	16917	32062	0.72%	0.065%
14	13.492	1745	1752	1757	rBV2	17829	29671	0.66%	0.060%
15	14.010	1833	1840	1857	rBV	1553510	2273106	50.89%	4.615%
16	14.286	1880	1887	1899	rBV2	1905012	2799535	62.68%	5.684%
17	14.592	1931	1939	1948	rBV	1308590	1912574	42.82%	3.883%
18	14.804	1966	1975	1999	rBV	741101	1393196	31.19%	2.828%
19	15.010	2006	2010	2016	rBV7	12681	22830	0.51%	0.046%
20	15.586	2100	2108	2121	rBV	2378679	3407588	76.29%	6.918%
21	15.710	2123	2129	2140	rVV	713045	1027675	23.01%	2.086%
22	15.827	2145	2149	2153	rVV6	14297	23785	0.53%	0.048%
23	16.157	2202	2205	2210	rVB7	4030	4576	0.10%	0.009%
24	16.386	2236	2244	2248	rBV6	30930	51108	1.14%	0.104%
25	17.016	2348	2351	2354	rBV5	4164	4969	0.11%	0.010%
26	17.339	2399	2406	2416	rBV	1589262	2208188	49.44%	4.483%
27	17.439	2416	2423	2433	rBV	2666238	3701454	82.87%	7.515%
28	18.021	2518	2522	2524	rVB5	4547	5166	0.12%	0.010%
29	18.239	2553	2559	2566	rBV	102182	176555	3.95%	0.358%
30	19.292	2734	2738	2743	rBV3	26593	38405	0.86%	0.078%
31	19.368	2746	2751	2754	rBV	27505	41685	0.93%	0.085%
32	19.515	2772	2776	2782	rBV3	48716	82575	1.85%	0.168%
33	19.668	2798	2802	2805	rBV6	17003	22682	0.51%	0.046%
34	19.727	2806	2812	2820	rBV	3210894	4134659	92.57%	8.394%
35	21.521	3112	3117	3127	rBV	1819213	2369230	53.05%	4.810%
36	23.774	3493	3500	3509	rBV2	2273019	4466449	100.00%	9.068%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043689.D
Acq On : 02 Jan 2024 11:29
Operator : MA/JU
Sample : PB158064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK064

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	23.933	3520	3527	3537	rVB	1270657	2600448	58.22%	5.279%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 49257220

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043689.D
Acq On : 02 Jan 2024 11:29
Operator : MA/JU
Sample : PB158064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

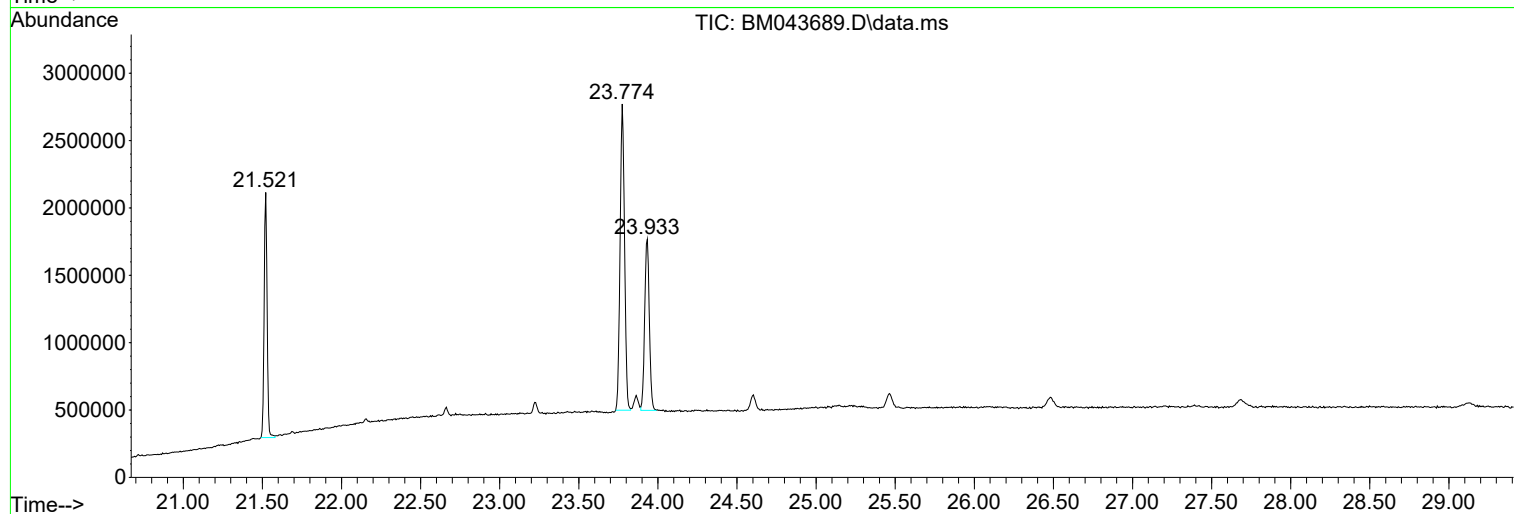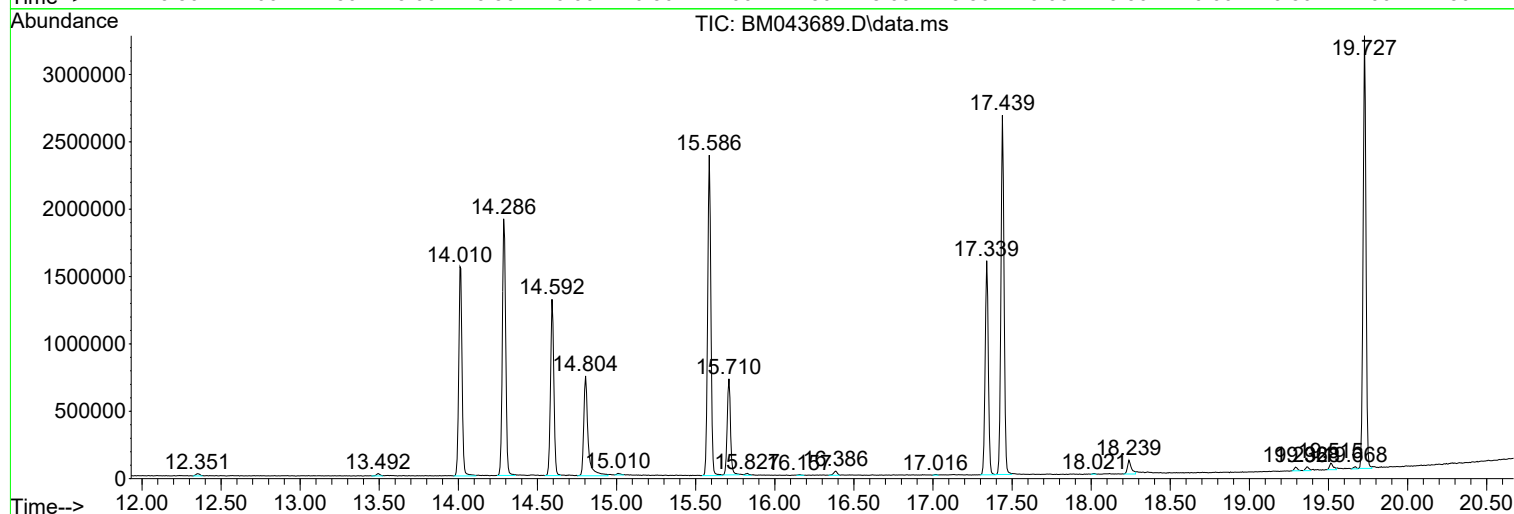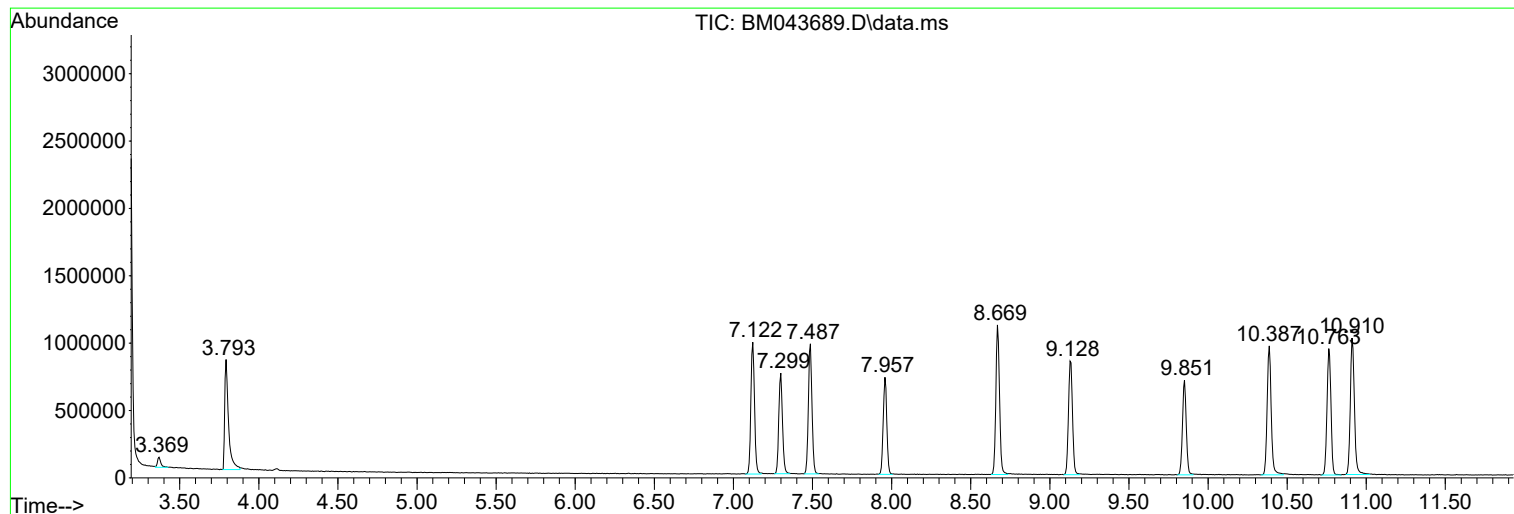

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043689.D
Acq On : 02 Jan 2024 11:29
Operator : MA/JU
Sample : PB158064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043689.D
Acq On : 02 Jan 2024 11:29
Operator : MA/JU
Sample : PB158064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------