

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043699.D
 Acq On : 02 Jan 2024 18:06
 Operator : MA/JU
 Sample : PB158101BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK101

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	38	rVB	75039	103344	2.39%	0.205%
2	3.793	100	103	126	rBV	779006	1287465	29.77%	2.548%
3	4.116	154	158	162	rBV	16894	26182	0.61%	0.052%
4	6.669	589	592	594	rBV3	4167	4471	0.10%	0.009%
5	7.128	663	670	688	rBV	1014914	1633854	37.78%	3.234%
6	7.298	693	699	712	rVB	736925	1162438	26.88%	2.301%
7	7.487	724	731	741	rBV	973310	1553375	35.92%	3.074%
8	7.957	803	811	820	rBV	828752	1326394	30.67%	2.625%
9	8.675	926	933	944	rBV	1121487	1824696	42.19%	3.611%
10	8.781	950	951	956	rVB5	5652	5189	0.12%	0.010%
11	9.134	1004	1011	1026	rBV	854814	1444962	33.41%	2.860%
12	9.445	1058	1064	1067	rBV8	2769	4901	0.11%	0.010%
13	9.851	1125	1133	1141	rBV	721096	1195378	27.64%	2.366%
14	10.392	1217	1225	1237	rBV	989776	1759790	40.69%	3.483%
15	10.769	1279	1289	1298	rBV	1025927	1810392	41.86%	3.583%
16	10.916	1306	1314	1331	rBV	982996	1807768	41.80%	3.578%
17	12.227	1534	1537	1542	rVB6	3698	5644	0.13%	0.011%
18	12.357	1554	1559	1563	rBV2	17947	29524	0.68%	0.058%
19	12.422	1566	1570	1571	rBV4	4112	5094	0.12%	0.010%
20	12.810	1630	1636	1638	rVB7	2920	4452	0.10%	0.009%
21	13.492	1747	1752	1757	rBV2	17058	28372	0.66%	0.056%
22	13.569	1763	1765	1769	rVB4	4848	4812	0.11%	0.010%
23	13.874	1813	1817	1819	rVB5	3727	4592	0.11%	0.009%
24	14.016	1833	1841	1852	rBV	1490729	2117618	48.96%	4.191%
25	14.292	1881	1888	1897	rBV	1896075	2814692	65.08%	5.571%
26	14.351	1897	1898	1906	rVV8	7321	12437	0.29%	0.025%
27	14.474	1915	1919	1928	rVB8	4001	9102	0.21%	0.018%
28	14.598	1933	1940	1950	rBV	1369848	2118410	48.98%	4.193%
29	14.810	1970	1976	1997	rBV	708522	1391811	32.18%	2.755%
30	15.004	2007	2009	2017	rVB9	12886	23108	0.53%	0.046%
31	15.268	2052	2054	2058	rVB5	4643	5527	0.13%	0.011%
32	15.586	2101	2108	2122	rBV	2251999	3338634	77.20%	6.608%
33	15.710	2124	2129	2139	rBV	558267	829821	19.19%	1.642%
34	15.827	2145	2149	2152	rVB6	10841	15927	0.37%	0.032%
35	16.386	2239	2244	2250	rBV9	30843	52141	1.21%	0.103%
36	16.521	2265	2267	2272	rVB6	6735	8835	0.20%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043699.D
 Acq On : 02 Jan 2024 18:06
 Operator : MA/JU
 Sample : PB158101BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK101

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	16.745	2300	2305	2311	rBV7	14978	26404	0.61%	0.052%
38	16.851	2321	2323	2329	rVB7	9727	14199	0.33%	0.028%
39	17.133	2368	2371	2373	rBV3	8294	8840	0.20%	0.017%
40	17.345	2400	2407	2417	rBV	1702426	2471523	57.15%	4.891%
41	17.439	2417	2423	2434	rBV	2567112	3676479	85.01%	7.276%
42	17.621	2450	2454	2459	rBV7	11316	25493	0.59%	0.050%
43	18.180	2546	2549	2553	rBV6	14347	24246	0.56%	0.048%
44	18.239	2555	2559	2568	rVV2	81206	148552	3.43%	0.294%
45	18.357	2575	2579	2590	rVB	116320	182927	4.23%	0.362%
46	19.298	2736	2739	2745	rVB2	32521	45279	1.05%	0.090%
47	19.368	2748	2751	2754	rVV	27326	32890	0.76%	0.065%
48	19.515	2774	2776	2780	rBV2	26011	31341	0.72%	0.062%
49	19.733	2807	2813	2820	rBV	3087447	4134439	95.60%	8.183%
50	21.521	3112	3117	3124	rBV	2059271	2646681	61.20%	5.238%
51	23.780	3495	3501	3509	rVB2	2162058	4324914	100.00%	8.560%
52	23.938	3521	3528	3537	rVB	1441245	2962190	68.49%	5.863%




Sum of corrected areas: 50527549

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043699.D
Acq On : 02 Jan 2024 18:06
Operator : MA/JU
Sample : PB158101BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK101

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

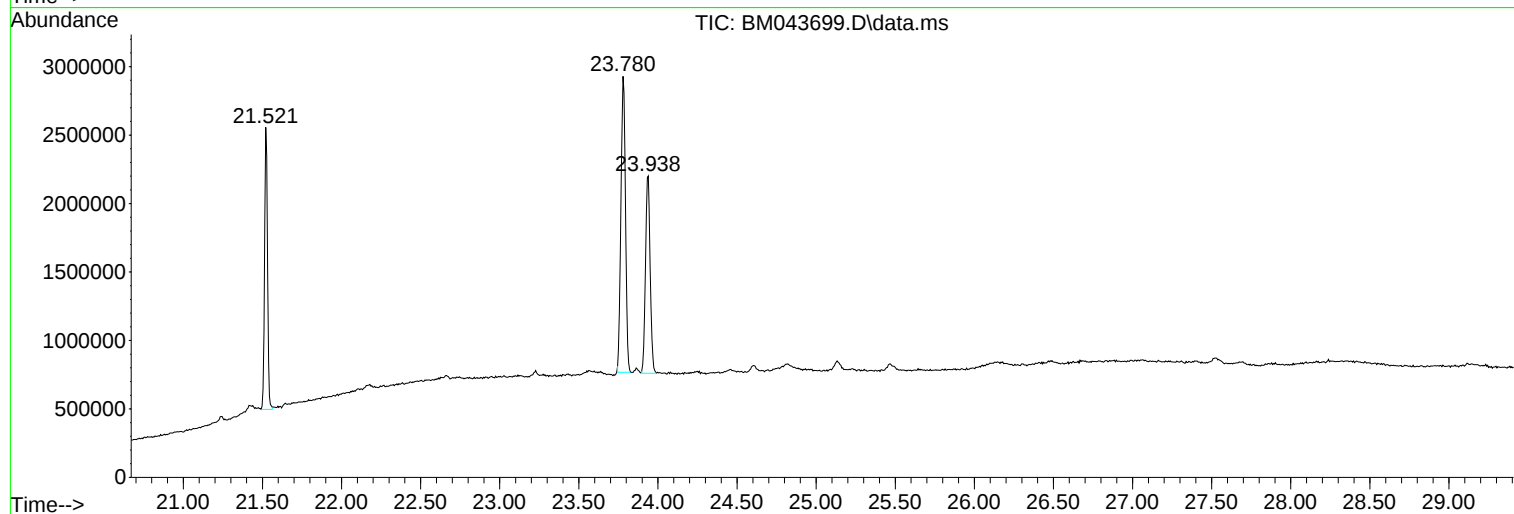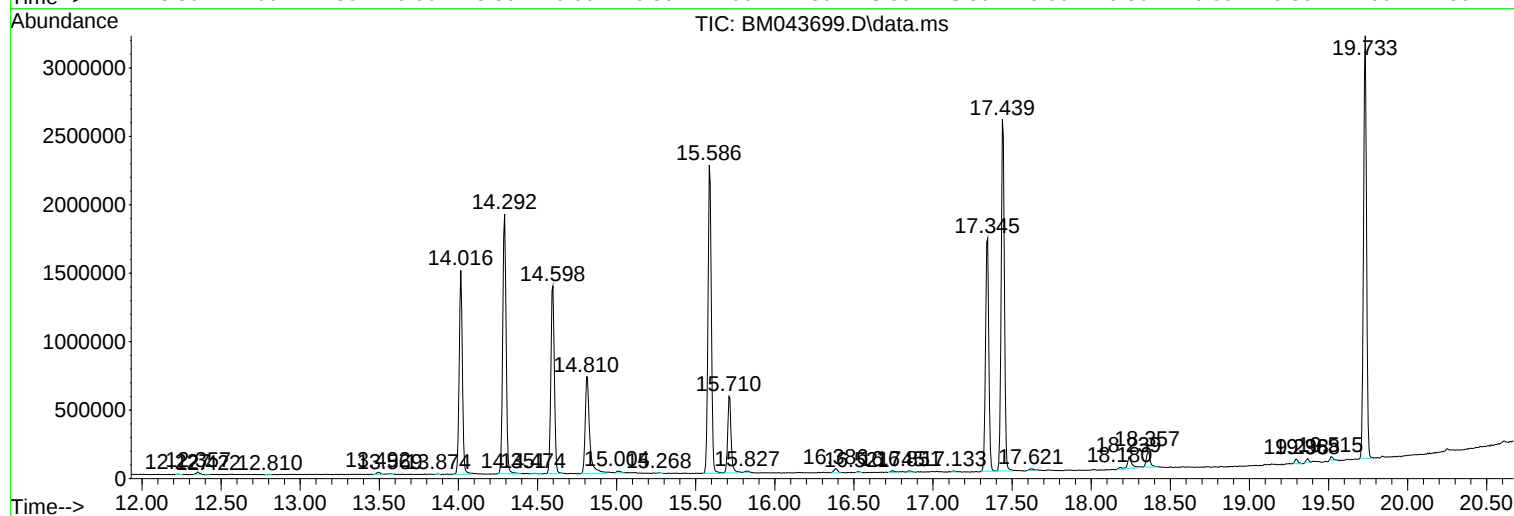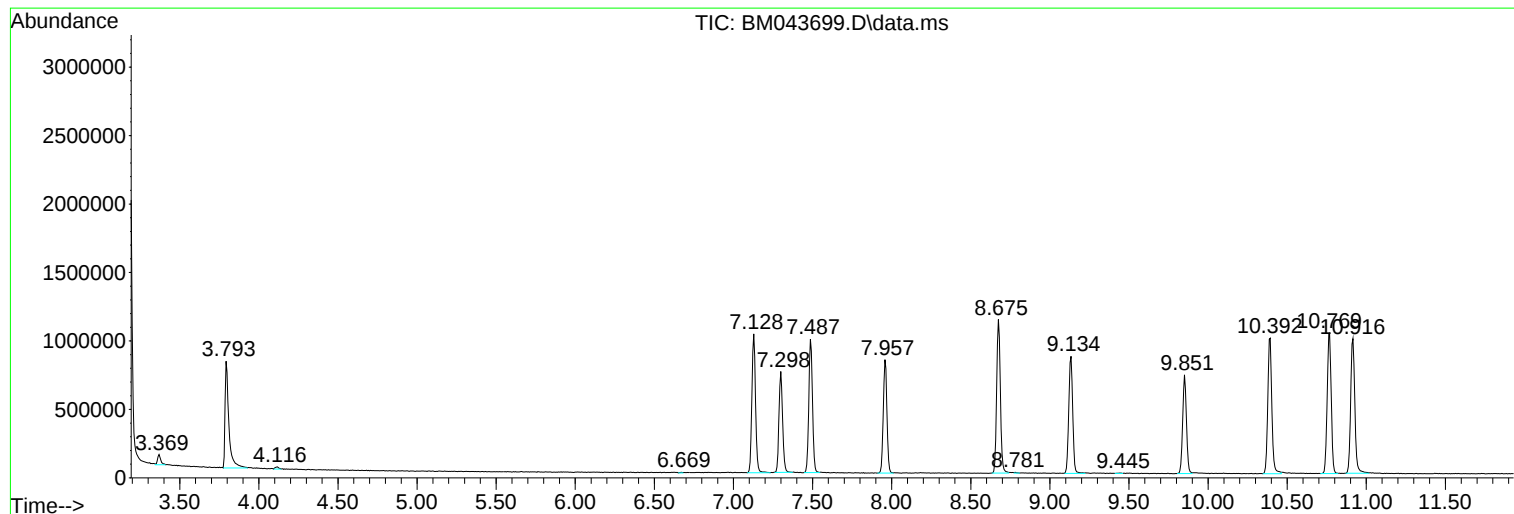

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043699.D
Acq On : 02 Jan 2024 18:06
Operator : MA/JU
Sample : PB158101BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK101

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043699.D
Acq On : 02 Jan 2024 18:06
Operator : MA/JU
Sample : PB158101BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK101

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------