

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043717.D
 Acq On : 03 Jan 2024 05:30
 Operator : MA/JU
 Sample : PB158129BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK129

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	36	rVB	62443	82057	1.58%	0.152%
2	3.793	100	103	119	rBV	726525	1146371	22.07%	2.121%
3	7.134	664	671	680	rBV	942027	1525064	29.35%	2.821%
4	7.299	693	699	708	rBV	701910	1102938	21.23%	2.040%
5	7.487	724	731	740	rBV	893366	1443514	27.78%	2.670%
6	7.957	803	811	822	rBV	683252	1070912	20.61%	1.981%
7	8.681	927	934	947	rBV	1129107	1842078	35.46%	3.407%
8	9.134	1003	1011	1025	rBV	844763	1446062	27.83%	2.675%
9	9.469	1062	1068	1072	rBV8	3394	6953	0.13%	0.013%
10	9.851	1125	1133	1142	rBV	713337	1220283	23.49%	2.257%
11	10.393	1217	1225	1243	rBV	1031253	1821394	35.06%	3.369%
12	10.769	1281	1289	1301	rBV	911766	1576772	30.35%	2.917%
13	10.916	1304	1314	1335	rBV	1059984	1946865	37.47%	3.601%
14	12.351	1552	1558	1567	rVB2	19909	42051	0.81%	0.078%
15	13.492	1747	1752	1757	rBV2	18343	29933	0.58%	0.055%
16	14.016	1834	1841	1855	rBV	1806587	2467152	47.49%	4.564%
17	14.292	1881	1888	1900	rBV	2190923	3222817	62.03%	5.961%
18	14.475	1915	1919	1921	rBV5	4851	5964	0.11%	0.011%
19	14.598	1933	1940	1951	rBV	1343286	2079518	40.03%	3.847%
20	14.822	1971	1978	1995	rBV	877099	1620606	31.19%	2.998%
21	15.016	2006	2011	2019	rVB10	19558	43185	0.83%	0.080%
22	15.586	2102	2108	2120	rBV	2739270	3898772	75.04%	7.212%
23	15.716	2124	2130	2142	rBV	704450	1040900	20.04%	1.925%
24	15.827	2144	2149	2154	rVV8	12201	21144	0.41%	0.039%
25	16.369	2239	2241	2246	rVB5	11219	14913	0.29%	0.028%
26	16.751	2301	2306	2312	rBV9	16328	34483	0.66%	0.064%
27	16.992	2344	2347	2357	rVB9	26196	46487	0.89%	0.086%
28	17.104	2362	2366	2367	rBV4	11450	15085	0.29%	0.028%
29	17.345	2401	2407	2417	rBV	1736900	2490871	47.94%	4.608%
30	17.445	2417	2424	2433	rBV	3092538	4393057	84.56%	8.126%
31	17.621	2450	2454	2459	rBV7	19711	41601	0.80%	0.077%
32	17.839	2489	2491	2495	rVB3	15104	16226	0.31%	0.030%
33	18.239	2556	2559	2570	rVB2	58315	100688	1.94%	0.186%
34	18.363	2575	2580	2585	rVB	154669	236411	4.55%	0.437%
35	18.533	2607	2609	2613	rVB3	20455	20023	0.39%	0.037%
36	19.733	2807	2813	2820	rBV	3822012	5007375	96.38%	9.263%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043717.D
Acq On : 03 Jan 2024 05:30
Operator : MA/JU
Sample : PB158129BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK129

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	21.527	3113	3118	3127	rBV	2051815	2773587	53.39%	5.131%
38	23.786	3496	3502	3511	rVB2	2583121	5195307	100.00%	9.610%
39	23.945	3523	3529	3542	rVB	1473399	2971258	57.19%	5.496%




Sum of corrected areas: 54060677

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043717.D
Acq On : 03 Jan 2024 05:30
Operator : MA/JU
Sample : PB158129BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK129

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

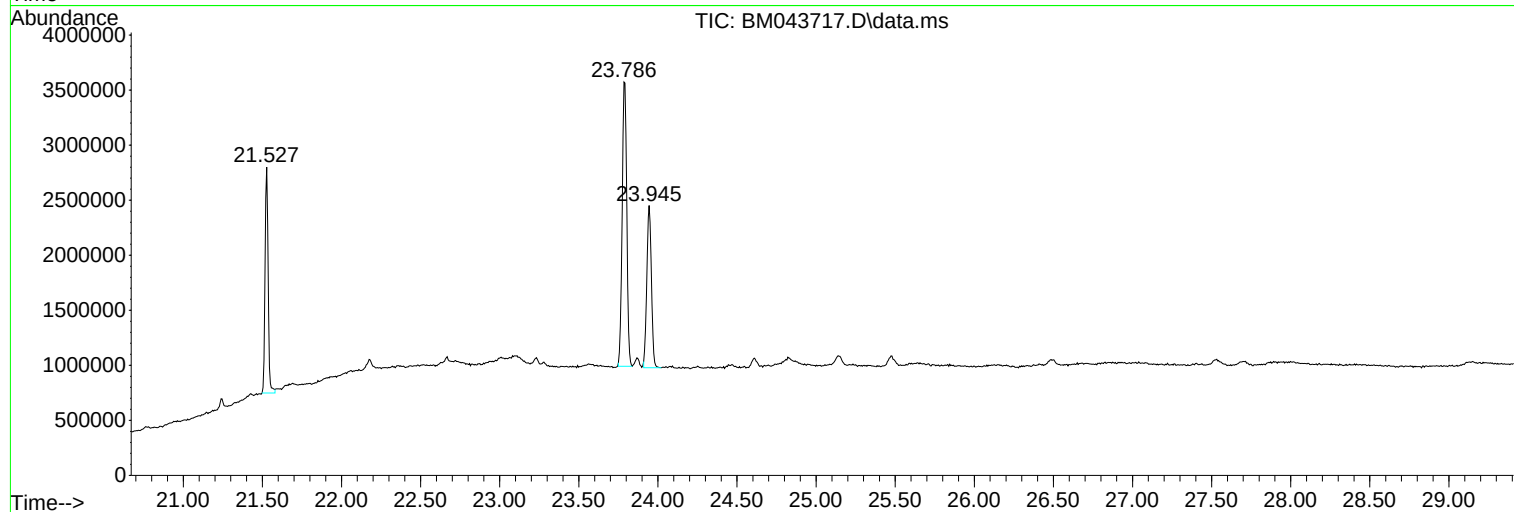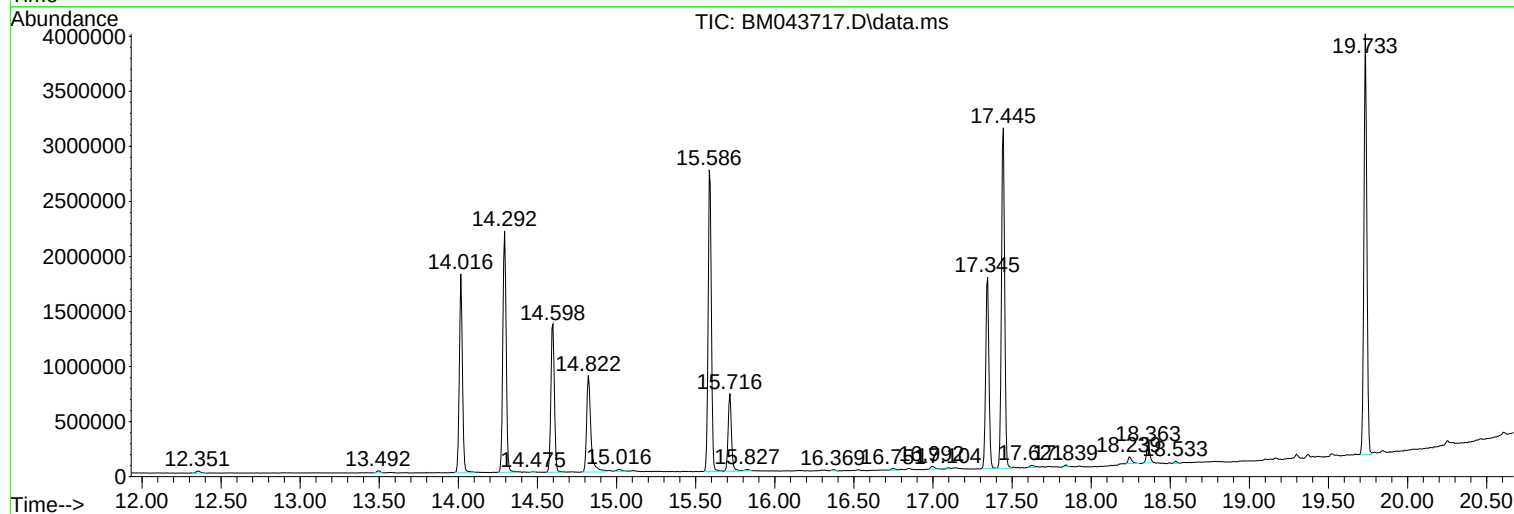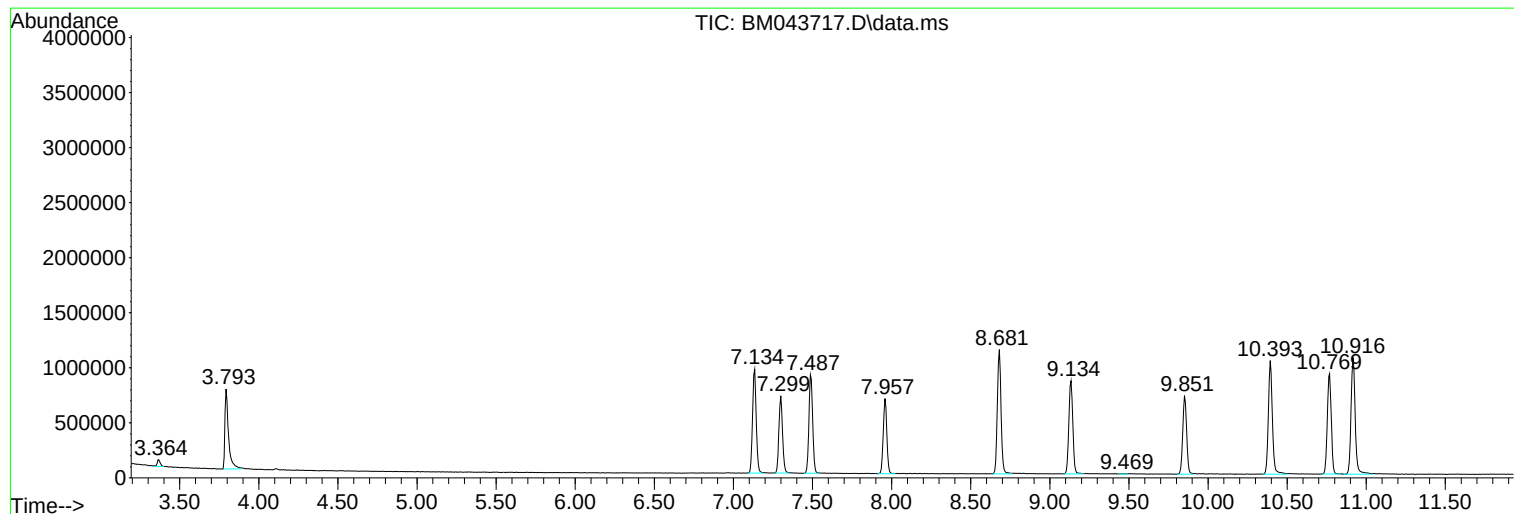

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043717.D
Acq On : 03 Jan 2024 05:30
Operator : MA/JU
Sample : PB158129BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK129

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043717.D
Acq On : 03 Jan 2024 05:30
Operator : MA/JU
Sample : PB158129BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK129

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------