

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
 Data File : BM043753.D
 Acq On : 04 Jan 2024 03:44
 Operator : MA/JU
 Sample : PB158129BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK129

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043753.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	43	rVB	113188	183176	2.32%	0.201%
2	3.799	100	104	129	rVB	1273042	2192576	27.78%	2.410%
3	4.111	154	157	165	rVB2	27591	39551	0.50%	0.043%
4	7.134	664	671	688	rBV	1589811	2711352	34.36%	2.980%
5	7.299	692	699	711	rVV	1253866	1977535	25.06%	2.174%
6	7.493	724	732	745	rBV	1587932	2630917	33.34%	2.892%
7	7.957	803	811	821	rBV	1364941	2205135	27.94%	2.424%
8	8.681	927	934	953	rBV	1771420	3164206	40.09%	3.478%
9	9.134	1004	1011	1025	rBV	1425770	2468890	31.28%	2.714%
10	9.287	1033	1037	1040	rBV5	5452	9537	0.12%	0.010%
11	9.857	1126	1134	1147	rBV	1178416	2107741	26.71%	2.317%
12	10.398	1217	1226	1246	rBV	1664831	3192806	40.46%	3.509%
13	10.769	1281	1289	1303	rBV	1818253	3134169	39.71%	3.445%
14	10.922	1306	1315	1339	rBV	1580809	3208567	40.66%	3.527%
15	11.575	1422	1426	1430	rBV8	5489	10247	0.13%	0.011%
16	12.357	1553	1559	1564	rBV2	31922	58753	0.74%	0.065%
17	13.322	1718	1723	1727	rBV8	4240	8288	0.11%	0.009%
18	13.492	1747	1752	1758	rVB	35761	63423	0.80%	0.070%
19	13.569	1762	1765	1771	rVB6	5310	9354	0.12%	0.010%
20	14.016	1835	1841	1855	rBV	2888561	4302253	54.52%	4.729%
21	14.145	1861	1863	1868	rVB5	6069	9201	0.12%	0.010%
22	14.292	1880	1888	1907	rBV	3516139	5678627	71.96%	6.241%
23	14.598	1932	1940	1954	rBV	2687420	4112598	52.11%	4.520%
24	14.839	1974	1981	1999	rBV	1000717	2266327	28.72%	2.491%
25	15.110	2024	2027	2029	rVB3	11496	10941	0.14%	0.012%
26	15.592	2102	2109	2125	rBV	4490761	6656779	84.35%	7.317%
27	15.727	2126	2132	2144	rVV	884437	1377284	17.45%	1.514%
28	15.827	2146	2149	2155	rVB3	24060	43880	0.56%	0.048%
29	16.374	2238	2242	2246	rVB5	14856	22266	0.28%	0.024%
30	16.445	2253	2254	2258	rBV4	8085	9381	0.12%	0.010%
31	16.851	2320	2323	2328	rVB6	14242	21856	0.28%	0.024%
32	16.998	2344	2348	2357	rBV4	43415	91134	1.15%	0.100%
33	17.345	2400	2407	2417	rBV	3144723	4640777	58.80%	5.101%
34	17.445	2418	2424	2438	rVV	4743649	7050012	89.33%	7.749%
35	18.245	2556	2560	2564	rBV6	26199	48491	0.61%	0.053%
36	18.357	2575	2579	2590	rVB	145216	224429	2.84%	0.247%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043753.D
Acq On : 04 Jan 2024 03:44
Operator : MA/JU
Sample : PB158129BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK129

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	18.580	2615	2617	2622	rBV5	18484	25920	0.33%	0.028%
38	19.298	2736	2739	2744	rVB3	58073	75893	0.96%	0.083%
39	19.374	2749	2752	2757	rVB	47031	65809	0.83%	0.072%
40	19.739	2808	2814	2824	rBV	5675464	7891811	100.00%	8.674%
41	21.533	3114	3119	3130	rBV	3083553	4481936	56.79%	4.926%
42	23.798	3497	3504	3511	rBV2	3693542	7550057	95.67%	8.298%
43	23.956	3524	3531	3544	rVB	2284487	4948938	62.71%	5.439%




Sum of corrected areas: 90982823

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043753.D
Acq On : 04 Jan 2024 03:44
Operator : MA/JU
Sample : PB158129BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK129

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

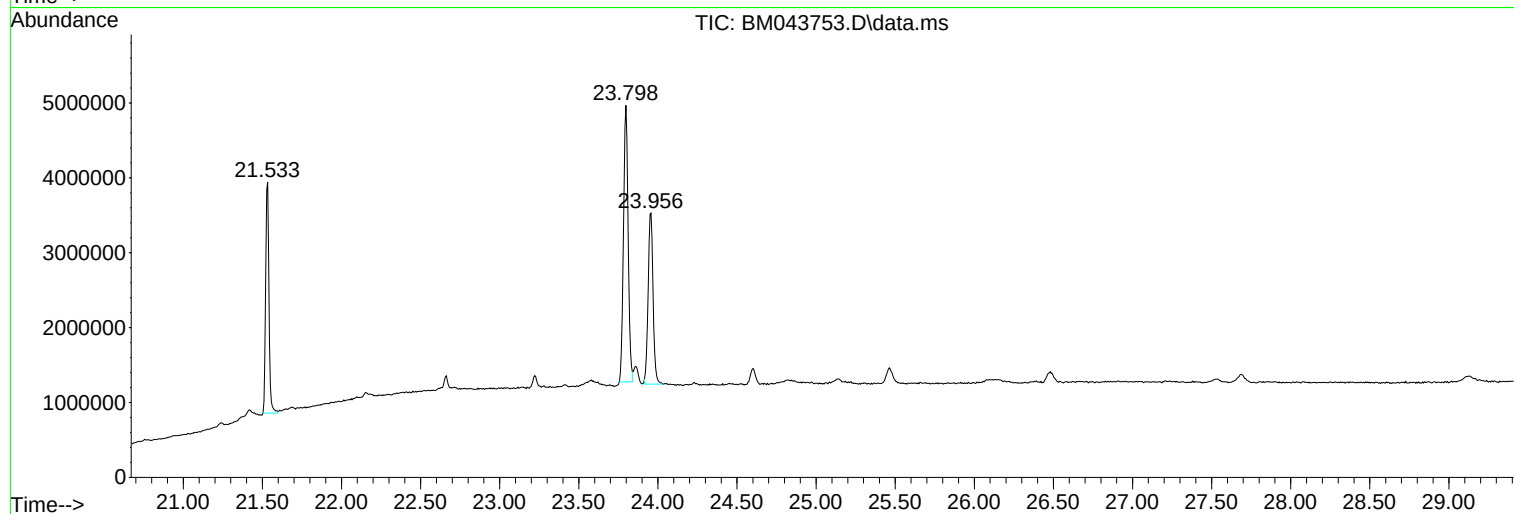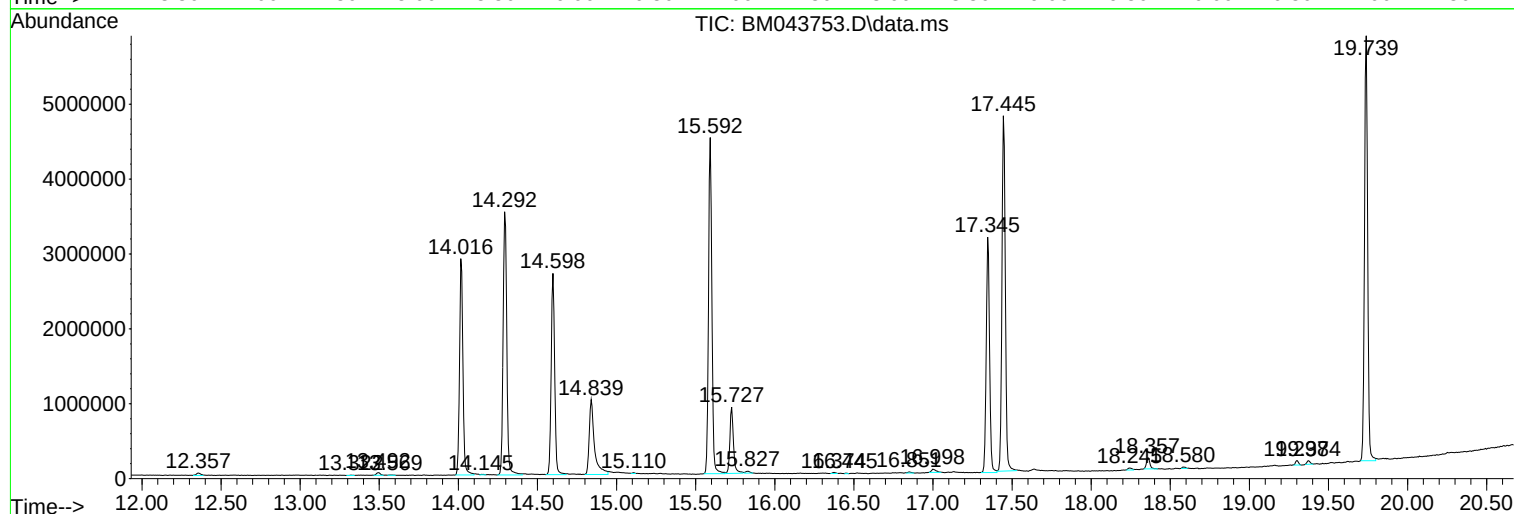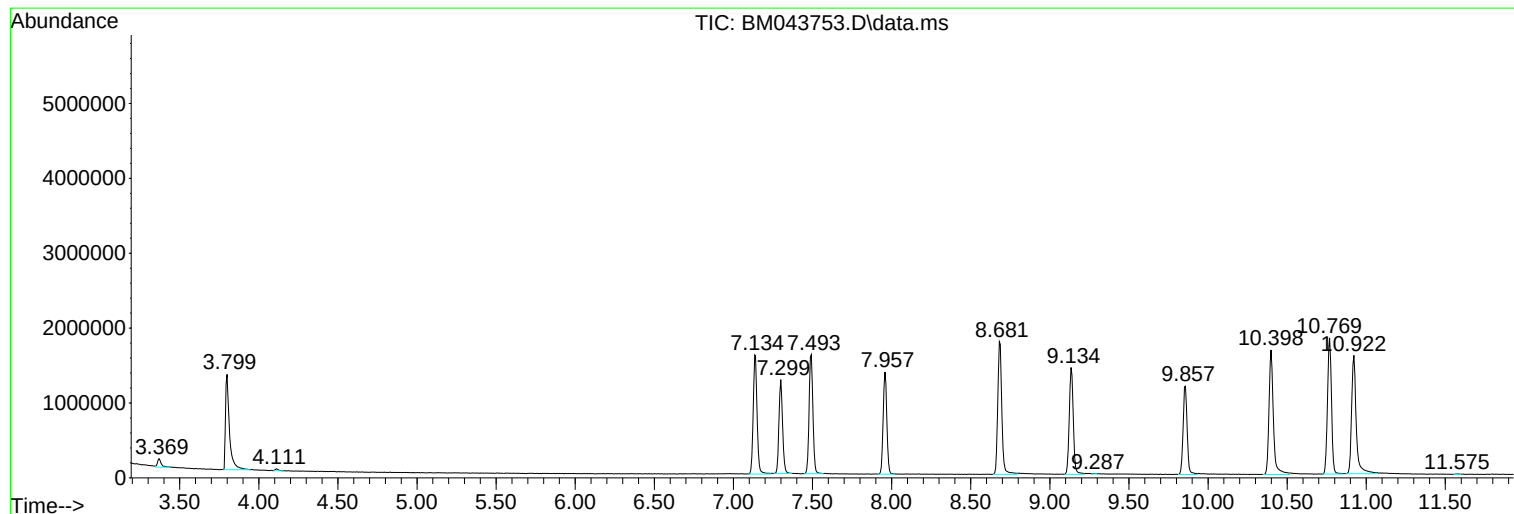

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043753.D
Acq On : 04 Jan 2024 03:44
Operator : MA/JU
Sample : PB158129BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK129

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010224\
Data File : BM043753.D
Acq On : 04 Jan 2024 03:44
Operator : MA/JU
Sample : PB158129BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK129

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------