

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
 Data File : BM049313.D
 Acq On : 02 Jan 2025 10:07
 Operator : RC/JU
 Sample : SSTDICC2.5
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC2.5

Quant Time: Jan 02 17:28:19 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 02 17:24:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.528	152	142435	20.000	ng	0.00
21) Naphthalene-d8	10.286	136	517360	20.000	ng	0.00
39) Acenaphthene-d10	14.169	164	341529	20.000	ng	0.00
64) Phenanthrene-d10	16.921	188	740209	20.000	ng	0.00
76) Chrysene-d12	21.150	240	653018	20.000	ng	0.00
86) Perylene-d12	23.933	264	721687	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	0.000	112	0d	0.000	ng	
7) Phenol-d6	0.000	99	0d	0.000	ng	
23) Nitrobenzene-d5	0.000	82	0d	0.000	ng	
42) 2,4,6-Tribromophenol	0.000	330	0d	0.000	ng	
45) 2-Fluorobiphenyl	0.000	172	0d	0.000	ng	
79) Terphenyl-d14	0.000	244	0d	0.000	ng	
Target Compounds						
19) n-Nitroso-di-n-propyla...	8.334	70	16043	2.107	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049313.D
Acq On : 02 Jan 2025 10:07
Operator : RC/JU
Sample : SSTDICC2.5
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC2.5

Quant Time: Jan 02 17:28:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 02 17:24:39 2025
Response via : Initial Calibration

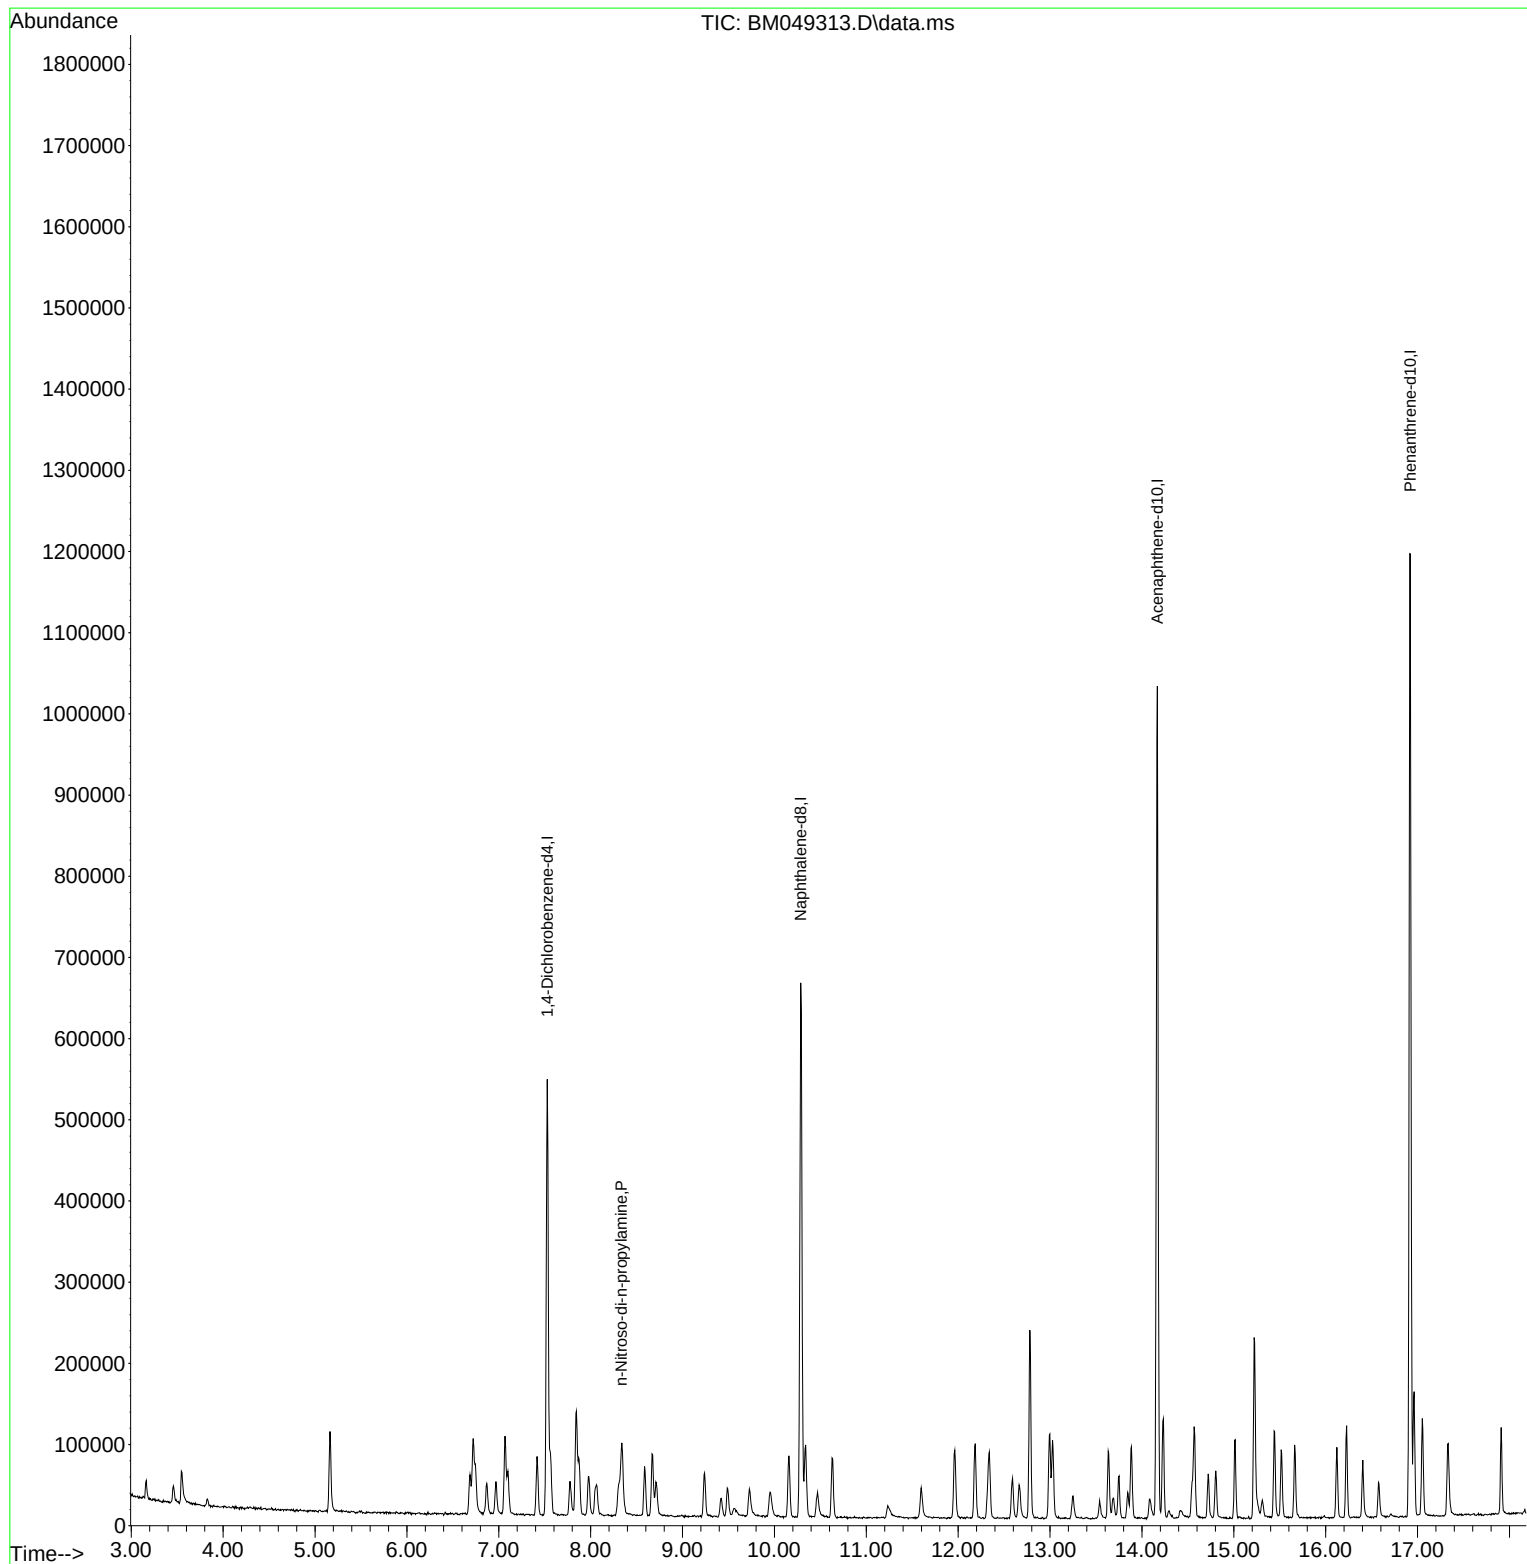

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049313.D
Acq On : 02 Jan 2025 10:07
Operator : RC/JU
Sample : SSTDICC2.5
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC2.5

Quant Time: Jan 02 17:28:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 02 17:24:39 2025
Response via : Initial Calibration

