
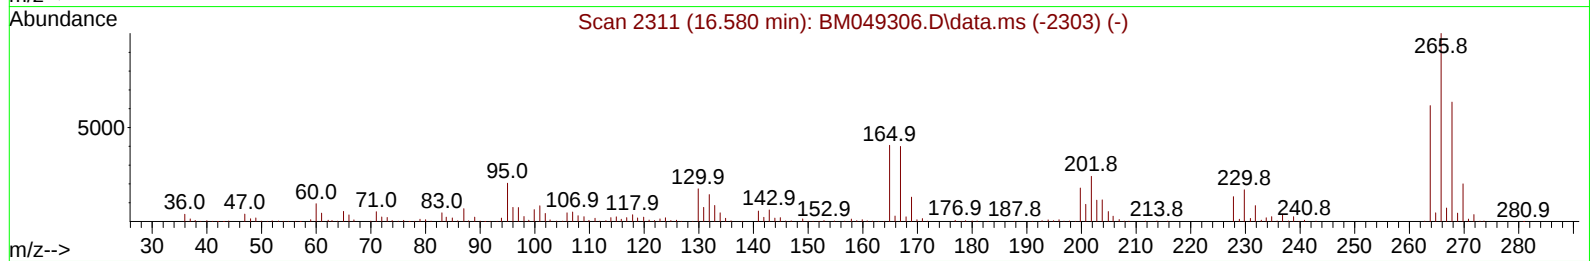
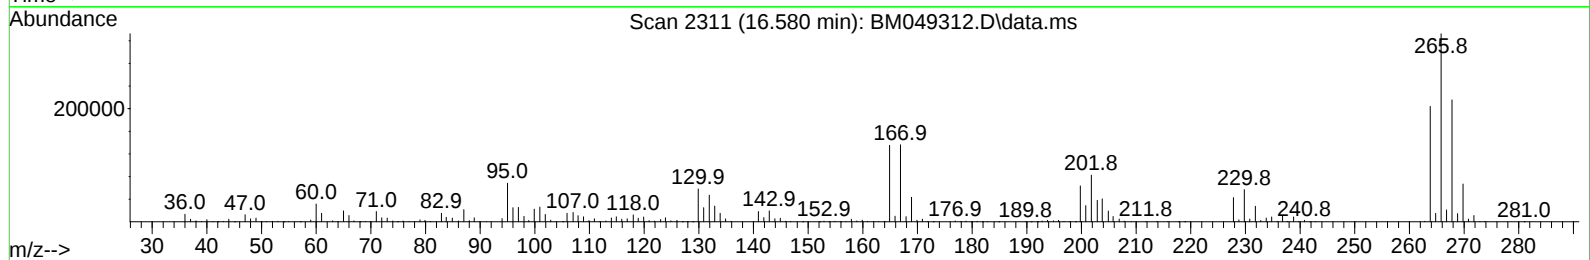


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049312.D
Acq On : 02 Jan 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 11:23:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 02 11:23:13 2025
Response via : Initial Calibration

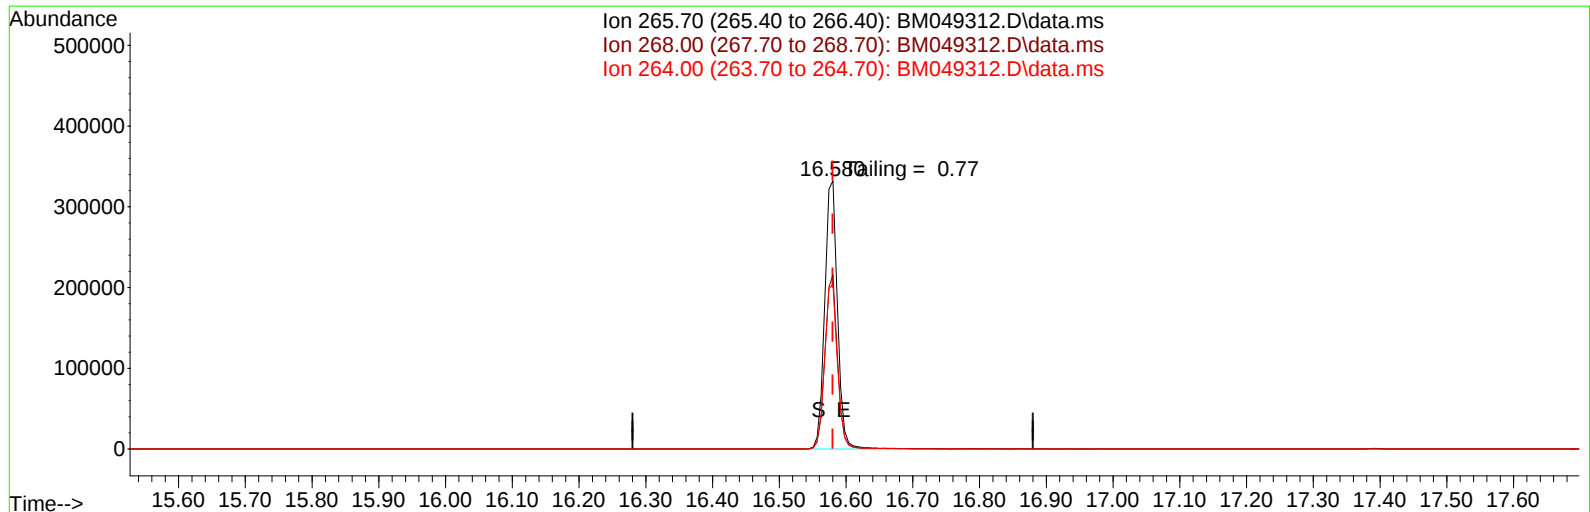

TIC: BM049312.D\data.ms

(70) Pentachlorophenol (C)




16.580min (+ 0.000) 46790.76 ng

response 442387

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.86
264.00	61.60	61.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049312.D
Acq On : 02 Jan 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 11:23:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 02 11:23:13 2025
Response via : Initial Calibration

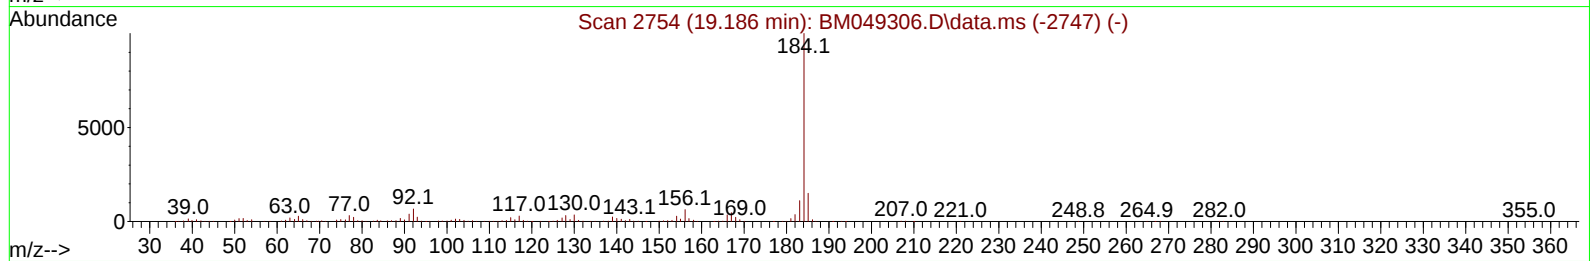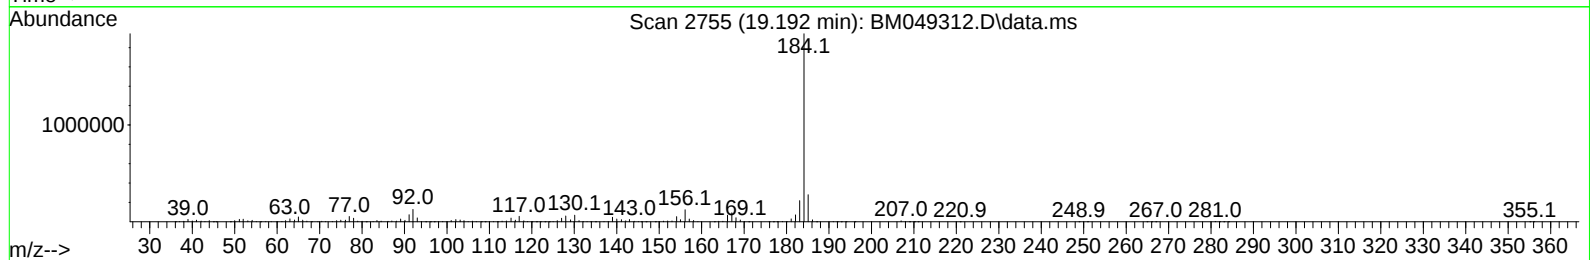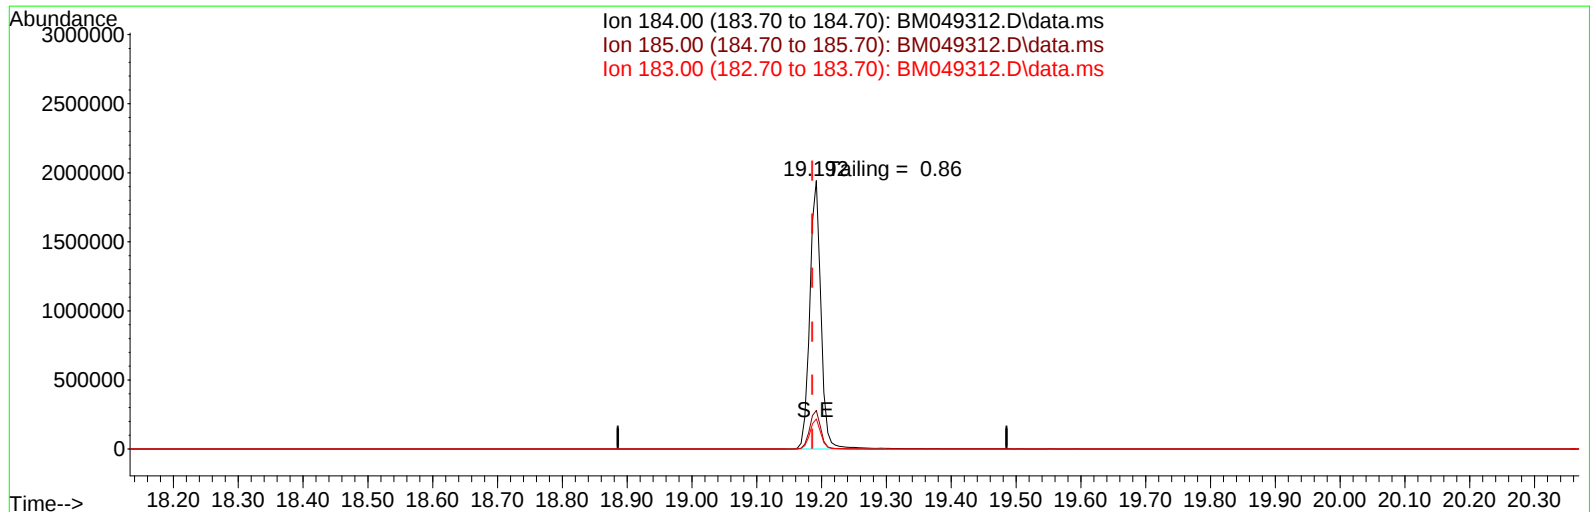

TIC: BM049312.D\data.ms

(77) Benzidine

19.192min (+ 0.006) 13166.69 ng

response 2334817

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.40
183.00	11.10	11.25
0.00	0.00	0.00