

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049322.D
Acq On : 02 Jan 2025 18:51
Operator : RC/JU
Sample : PB165929BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB165929BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM049322.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.163	364	370	388	rBV	4104543	5585389	56.10%	12.360%
2	6.722	627	635	650	rBV	3647171	5494202	55.19%	12.158%
3	7.528	765	772	780	rBV	660077	1002915	10.07%	2.219%
4	8.669	957	966	981	rBV	2021598	3333446	33.48%	7.377%
5	10.287	1235	1241	1259	rBV	701997	1230012	12.35%	2.722%
6	12.780	1658	1665	1678	rBV	5125760	7355642	73.88%	16.278%
7	14.169	1894	1901	1913	rBV	1002645	1484022	14.91%	3.284%
8	15.663	2149	2155	2176	rBV	3649043	5098978	51.22%	11.284%
9	16.921	2362	2369	2384	rBV	1093011	1605806	16.13%	3.554%
10	19.568	2814	2819	2832	rBV	8243398	9955751	100.00%	22.032%
11	21.151	3083	3088	3100	rBV	1141815	1529352	15.36%	3.384%
12	23.933	3554	3561	3576	rVB2	658140	1512796	15.20%	3.348%




Sum of corrected areas: 45188311

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049322.D
Acq On : 02 Jan 2025 18:51
Operator : RC/JU
Sample : PB165929BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB165929BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

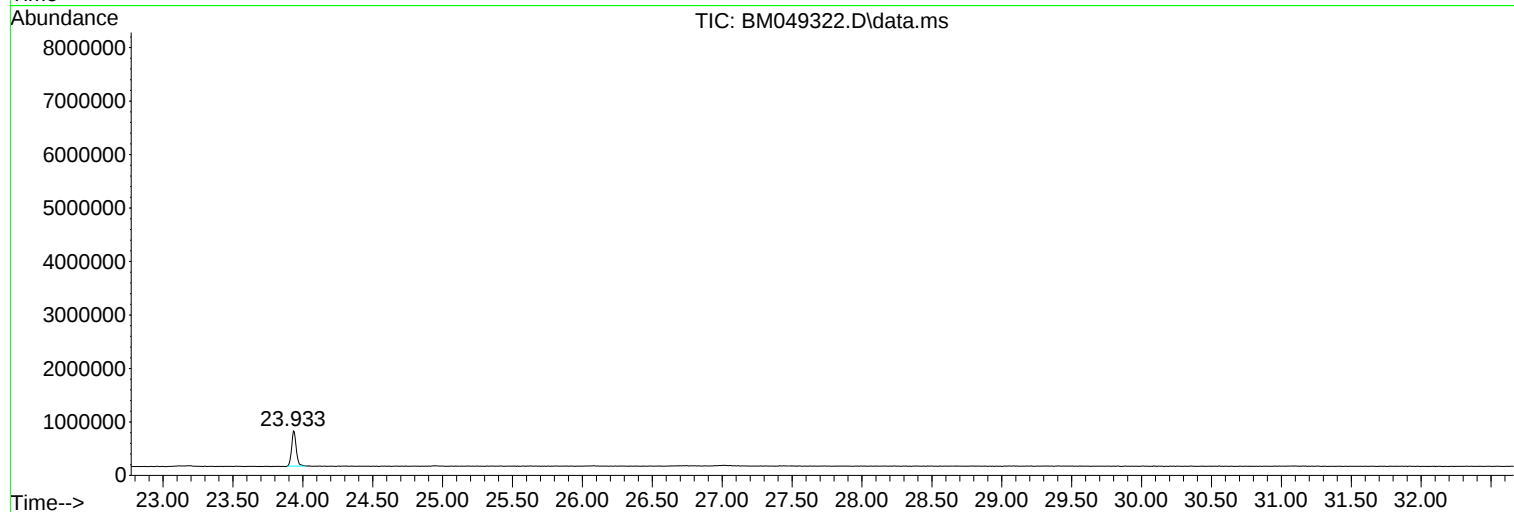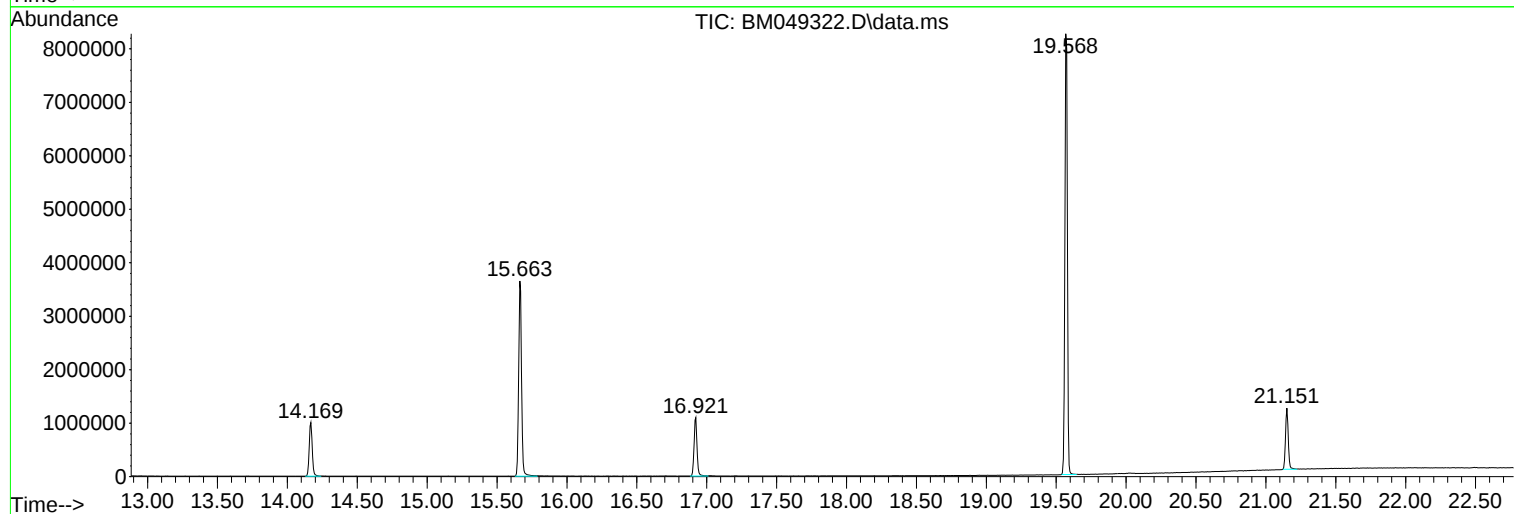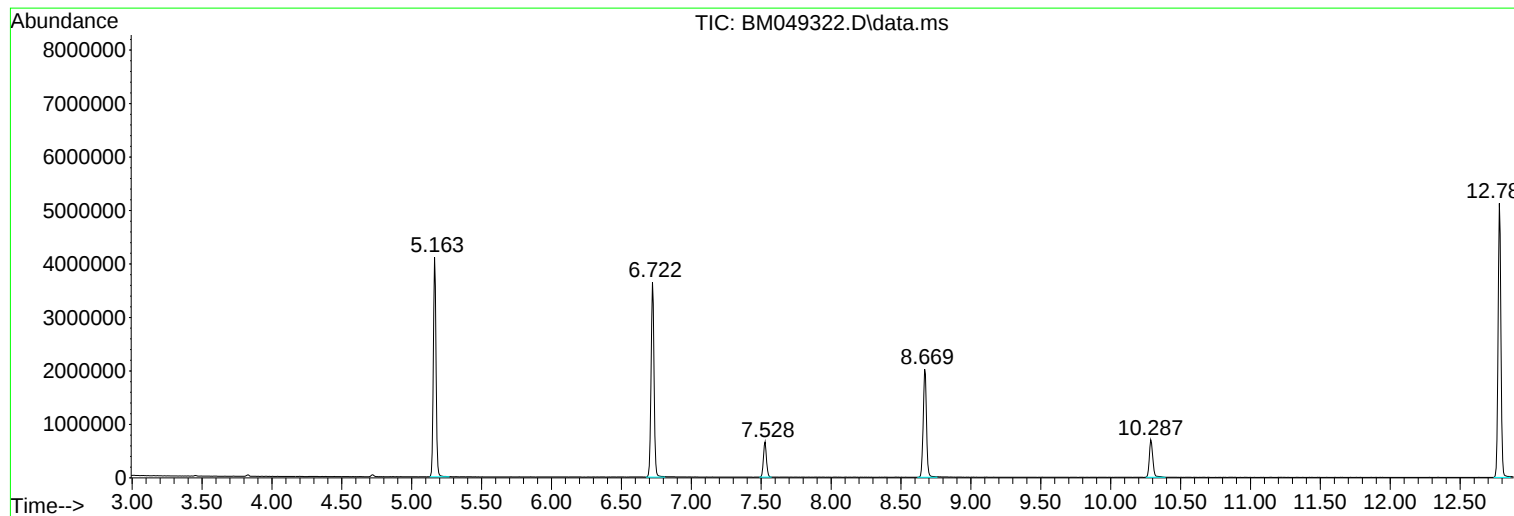

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049322.D
Acq On : 02 Jan 2025 18:51
Operator : RC/JU
Sample : PB165929BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB165929BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049322.D
Acq On : 02 Jan 2025 18:51
Operator : RC/JU
Sample : PB165929BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB165929BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------