


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049312.D
Acq On : 02 Jan 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 02 17:54:55 2025

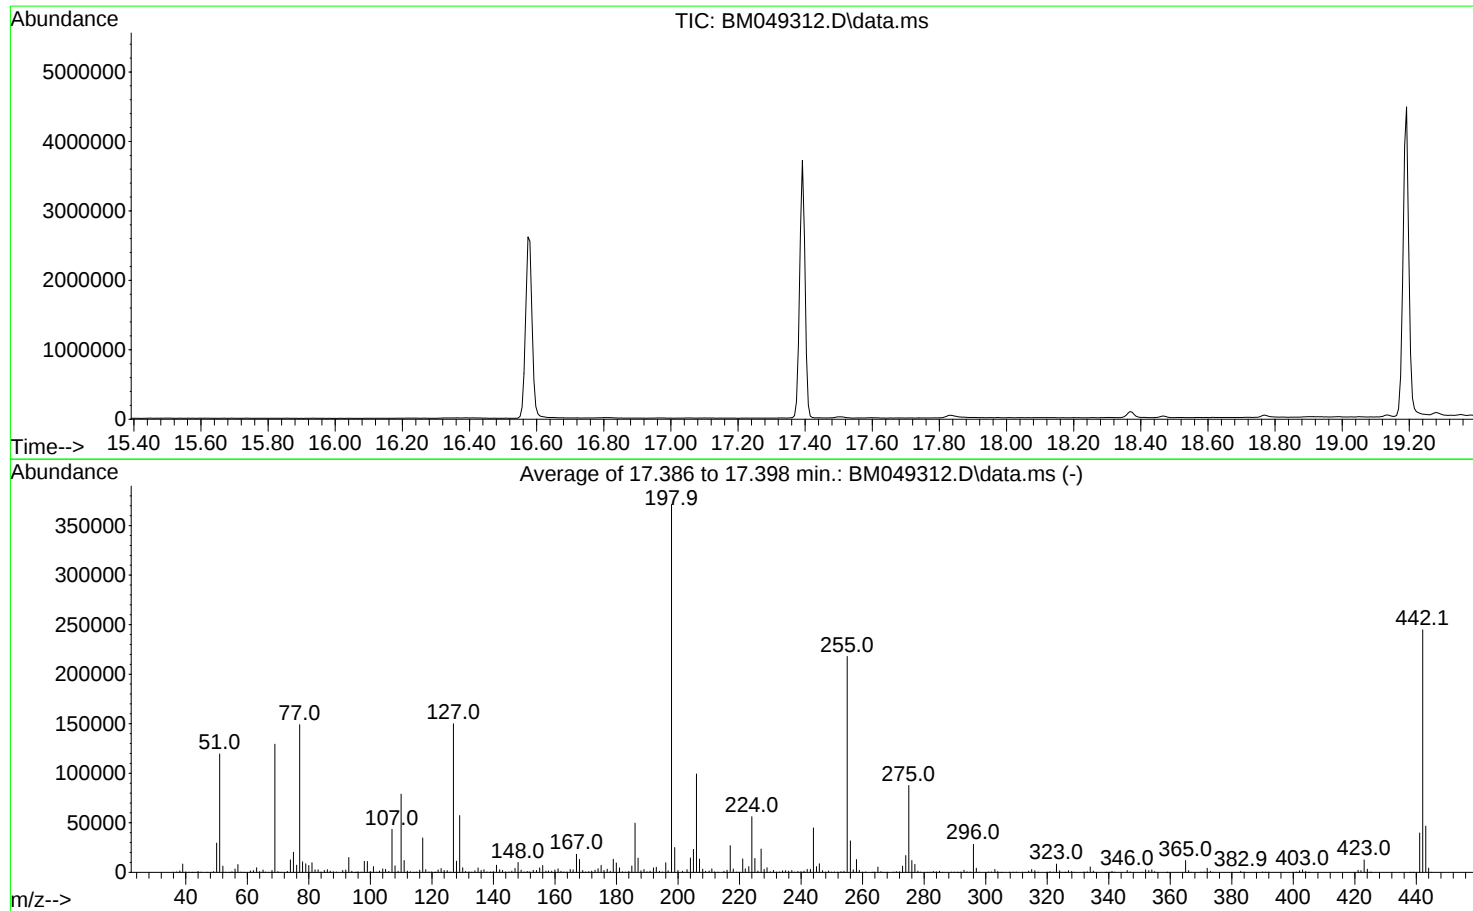

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	119518	PASS
68	69	0.00	2	1.5	1985	PASS
69	198	0.00	100	34.8	129308	PASS
70	69	0.00	2	0.6	812	PASS
127	198	10	80	40.4	150051	PASS
197	198	0.00	2	0.4	1564	PASS
198	198	100	100	100.0	371285	PASS
199	198	5	9	6.7	25061	PASS
275	198	10	60	23.6	87747	PASS
365	198	1	100	3.2	11911	PASS
441	198	0.01	100	10.7	39733	PASS
442	442	50	100	100.0	244885	PASS
443	442	15	24	19.0	46616	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/2/2025	BNA_M	<u>BM049312.D</u>
Compound Name	Response	Retention Time
DDT	1225308	20.439
DDD	2450	20.045
DDE	1049	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3499	1228807	0.28

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049312.D
Acq On : 02 Jan 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 02 11:23:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 02 11:23:13 2025
Response via : Initial Calibration

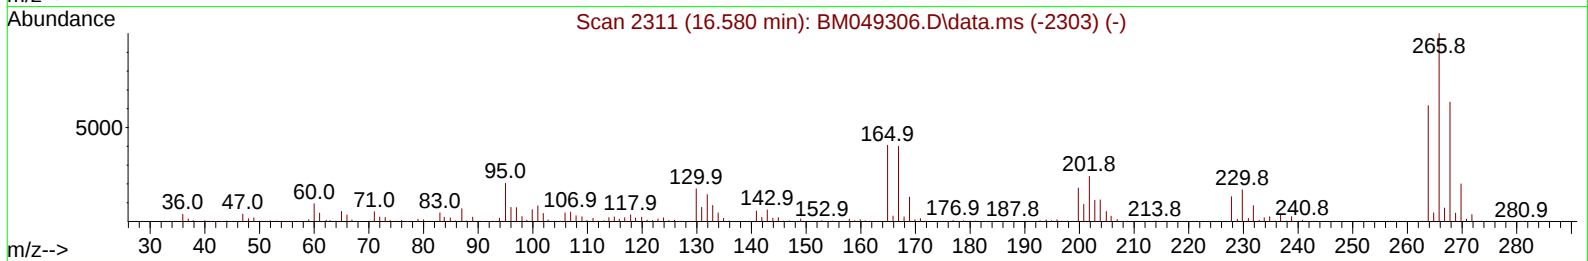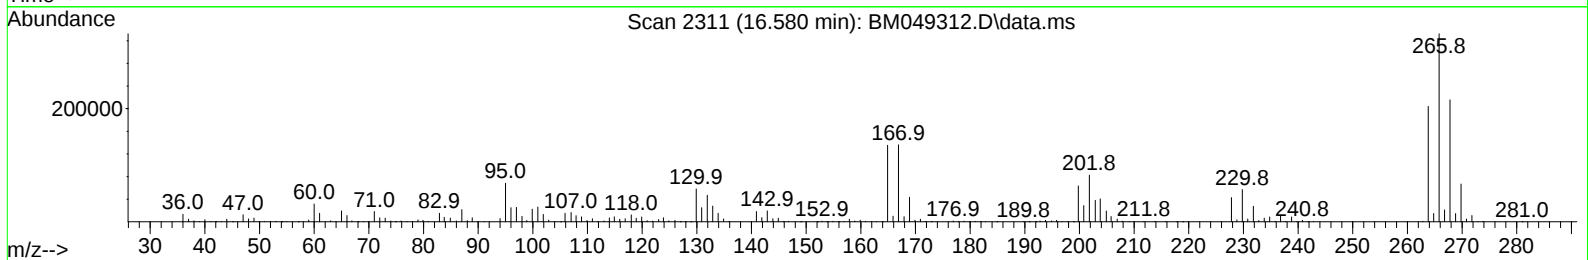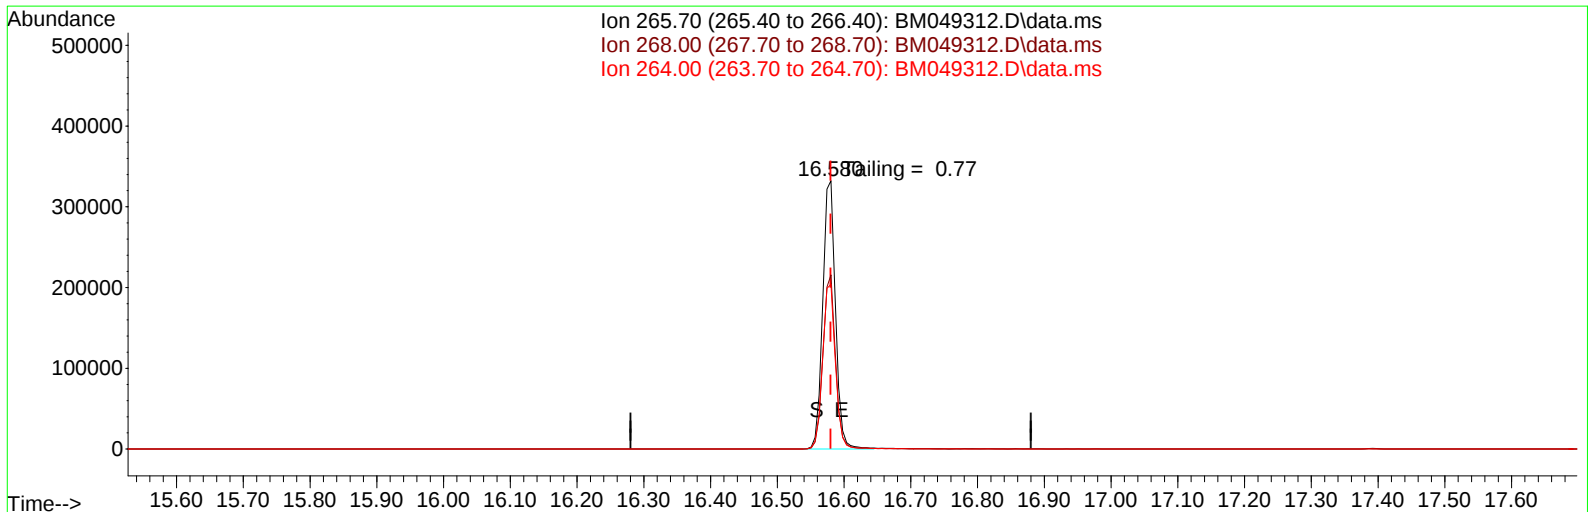

TIC: BM049312.D\data.ms

(70) Pentachlorophenol (C)

16.580min (+ 0.000) 46790.76 ng




response 442387

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.86
264.00	61.60	61.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010225\
Data File : BM049312.D
Acq On : 02 Jan 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 02 11:23:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 02 11:23:13 2025
Response via : Initial Calibration

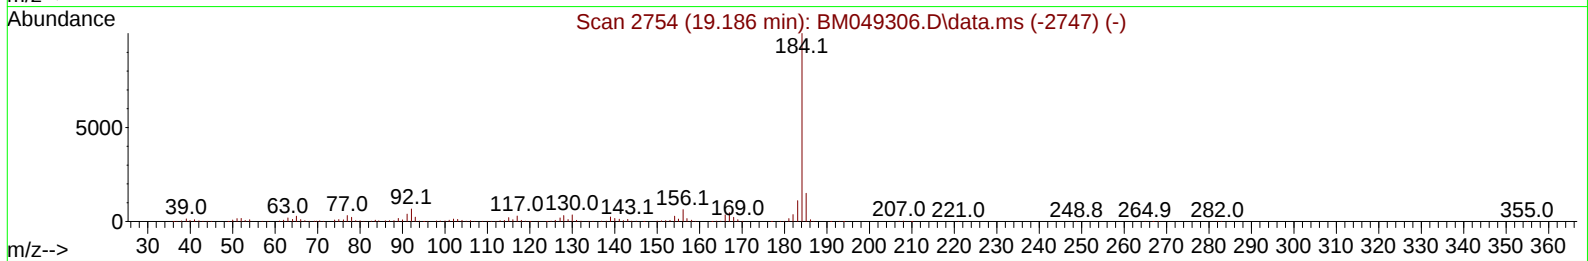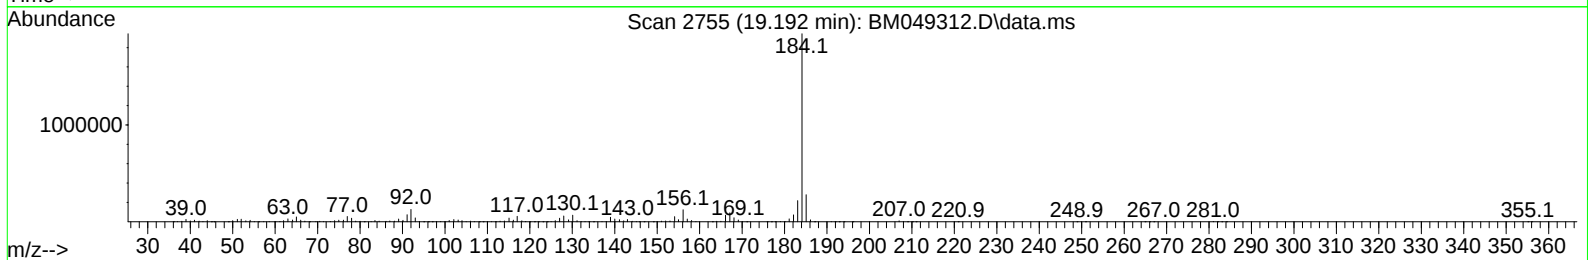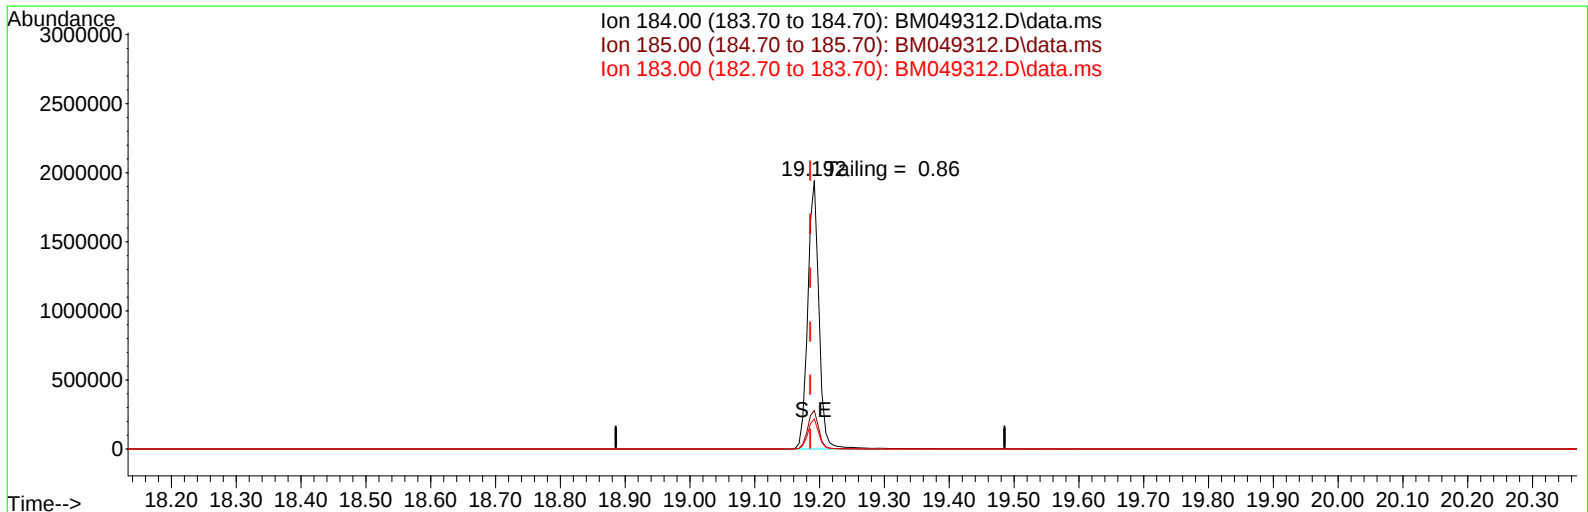

TIC: BM049312.D\data.ms

(77) Benzidine

19.192min (+ 0.006) 13166.69 ng

response 2334817

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.40
183.00	11.10	11.25
0.00	0.00	0.00