
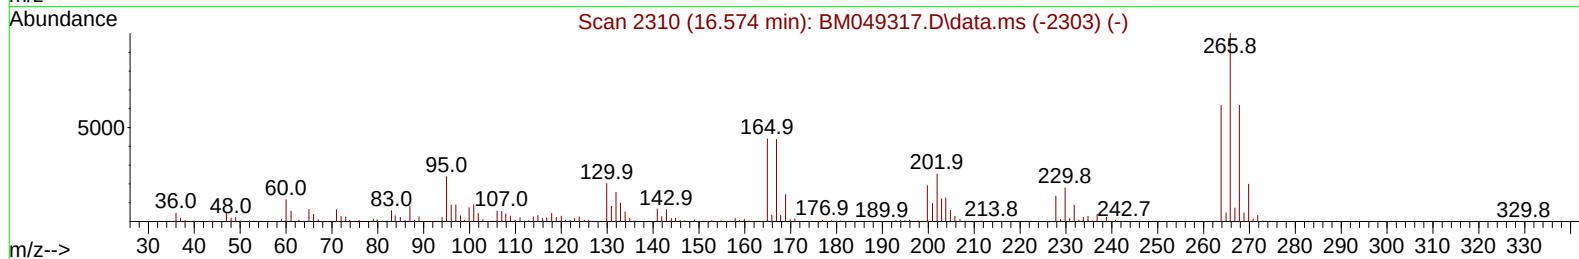
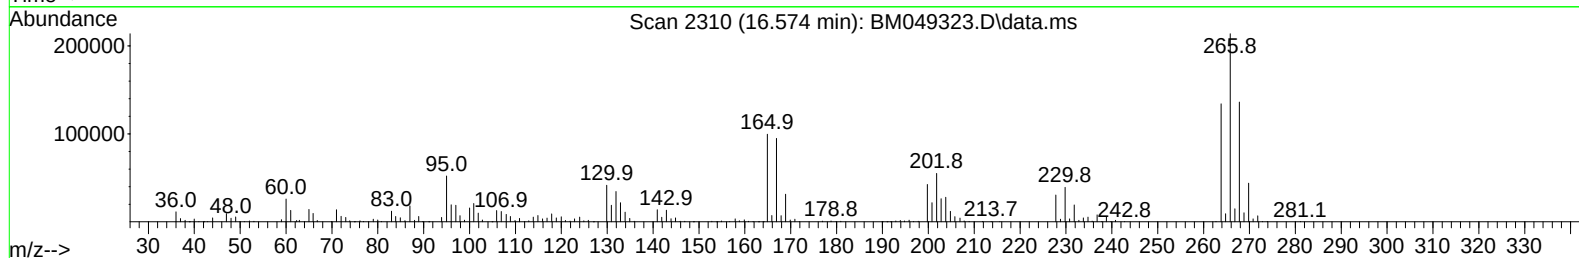


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010325\
Data File : BM049323.D
Acq On : 03 Jan 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 13:09:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 13:09:35 2025
Response via : Initial Calibration

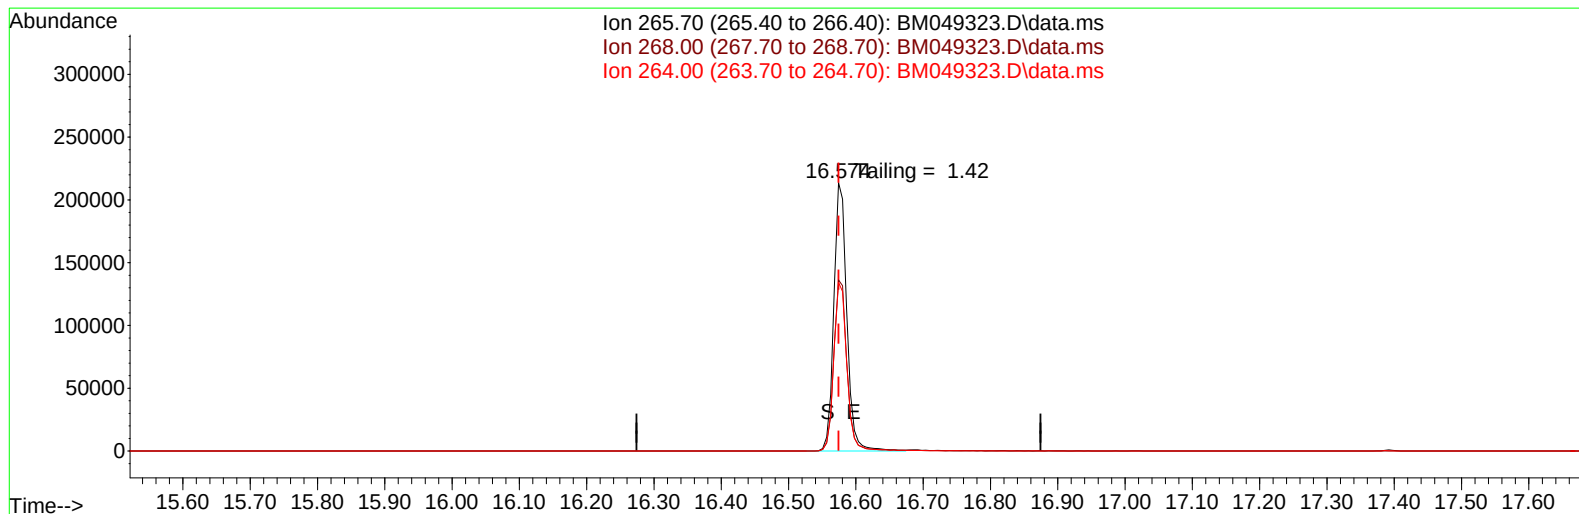

TIC: BM049323.D\data.ms

(70) Pentachlorophenol (C)




16.574min (0.000) 50264.59 ng

response 286754

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.80	63.71
264.00	61.70	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010325\
Data File : BM049323.D
Acq On : 03 Jan 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 13:09:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 13:09:35 2025
Response via : Initial Calibration

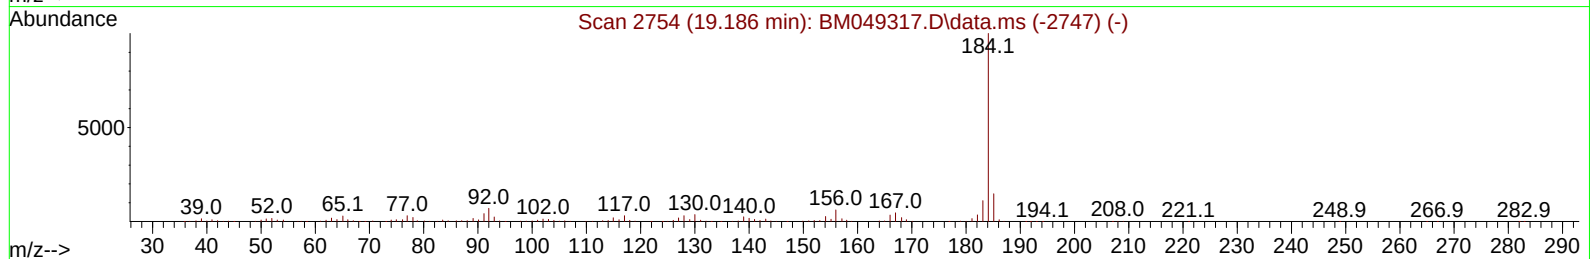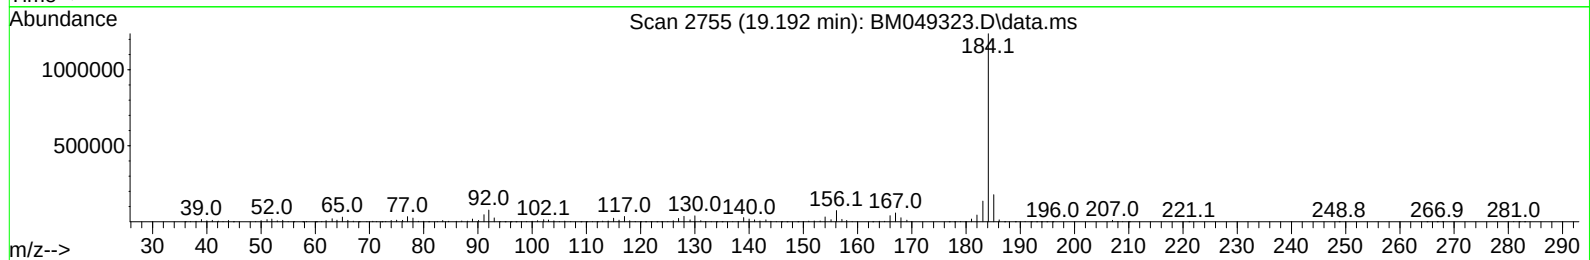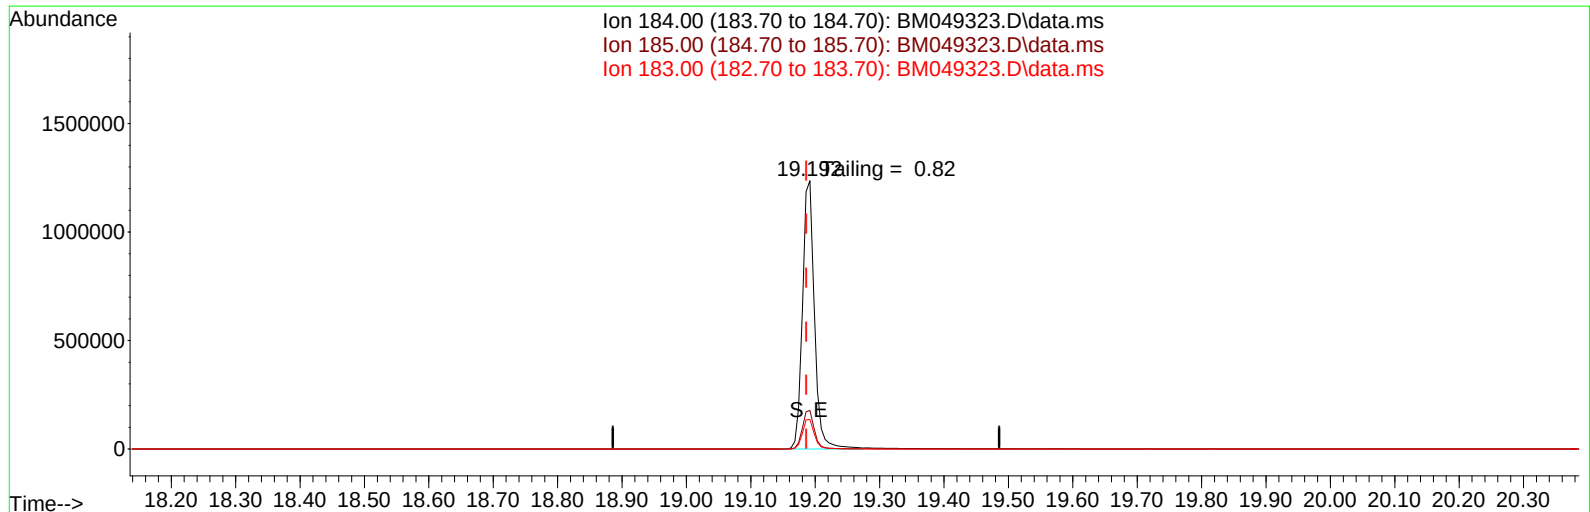

TIC: BM049323.D\data.ms

(77) Benzidine**19.192min (+ 0.006) 18290.10 ng****response 1618757**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.41
183.00	11.10	11.03
0.00	0.00	0.00