
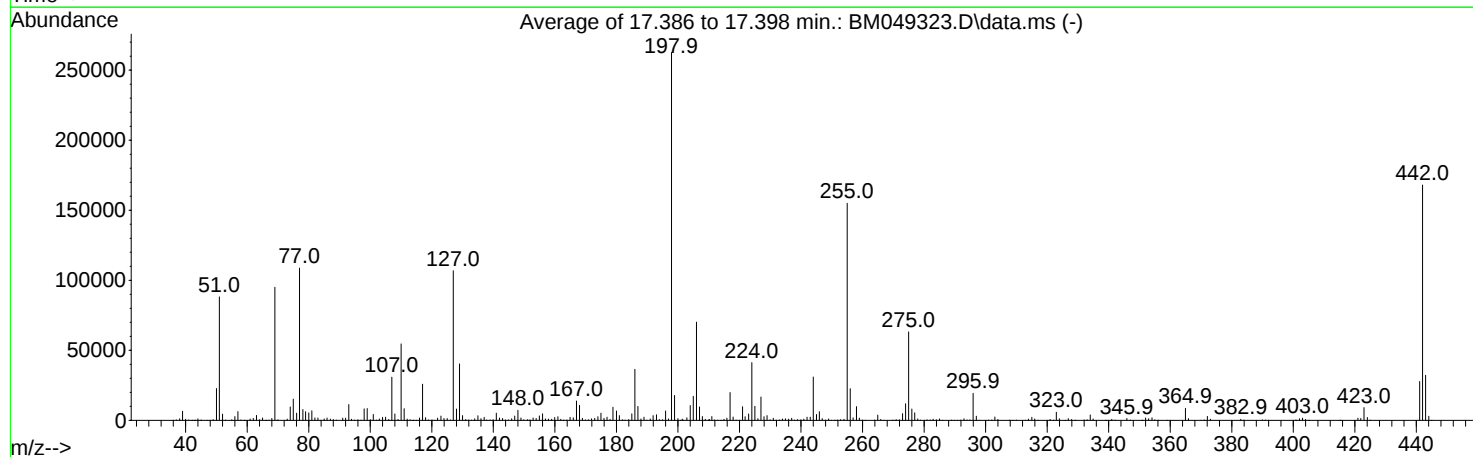


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010325\
Data File : BM049323.D
Acq On : 03 Jan 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 03 17:24:13 2025

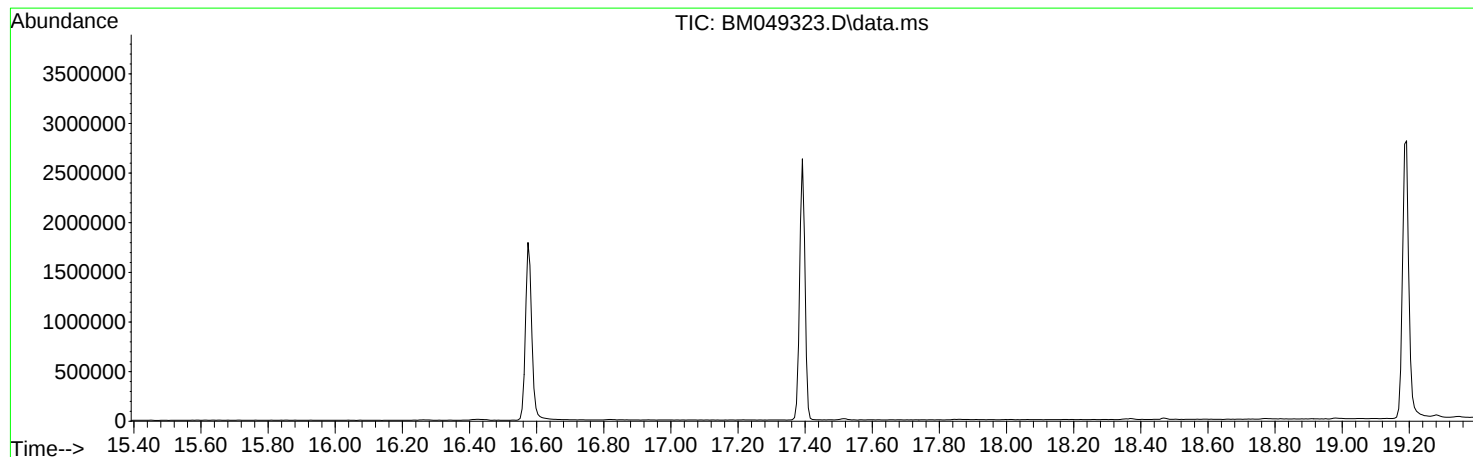

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	88173	PASS
68	69	0.00	2	1.4	1332	PASS
69	198	0.00	100	36.2	95005	PASS
70	69	0.00	2	0.5	489	PASS
127	198	10	80	40.7	106787	PASS
197	198	0.00	2	0.4	1018	PASS
198	198	100	100	100.0	262613	PASS
199	198	5	9	6.8	17797	PASS
275	198	10	60	24.0	63120	PASS
365	198	1	100	3.3	8578	PASS
441	198	0.01	100	10.6	27728	PASS
442	442	50	100	100.0	168045	PASS
443	442	15	24	19.2	32227	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/3/2025	BNA_M	<u>BM049323.D</u>
Compound Name	Response	Retention Time
DDT	827173	20.439
DDD	11188	19.992
DDE	1322	19.486
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12510	839683	1.49

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010325\
Data File : BM049323.D
Acq On : 03 Jan 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 03 13:09:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 13:09:35 2025
Response via : Initial Calibration

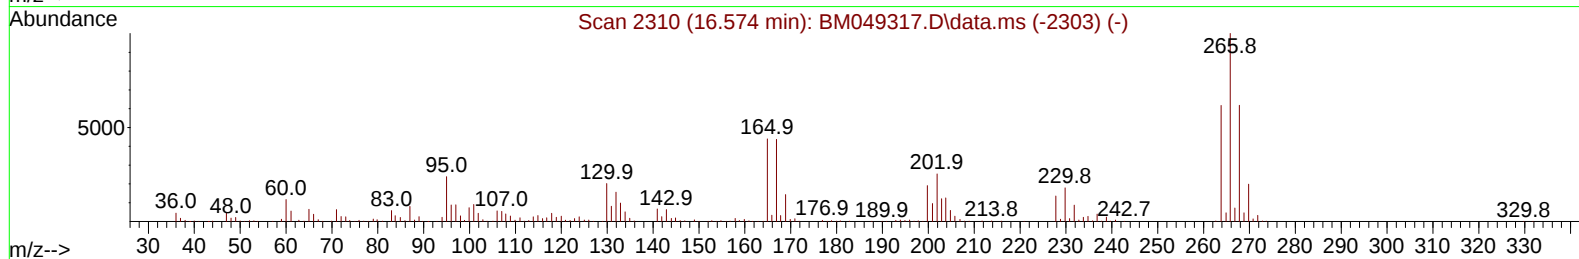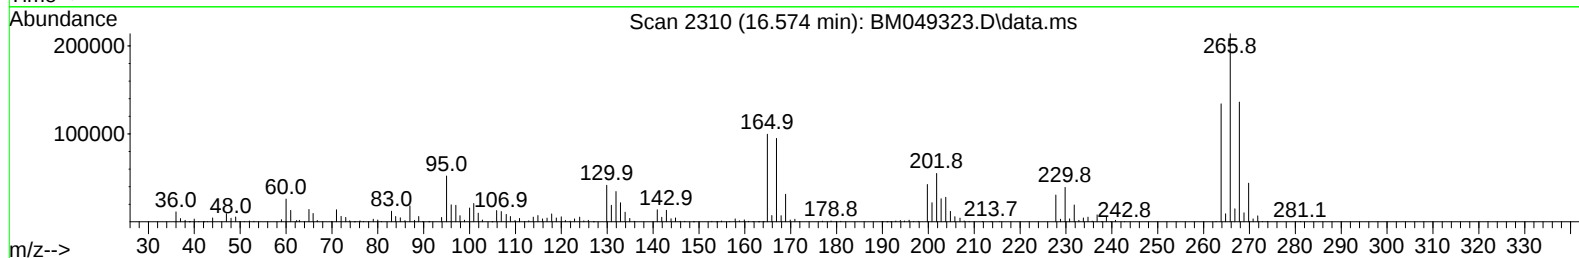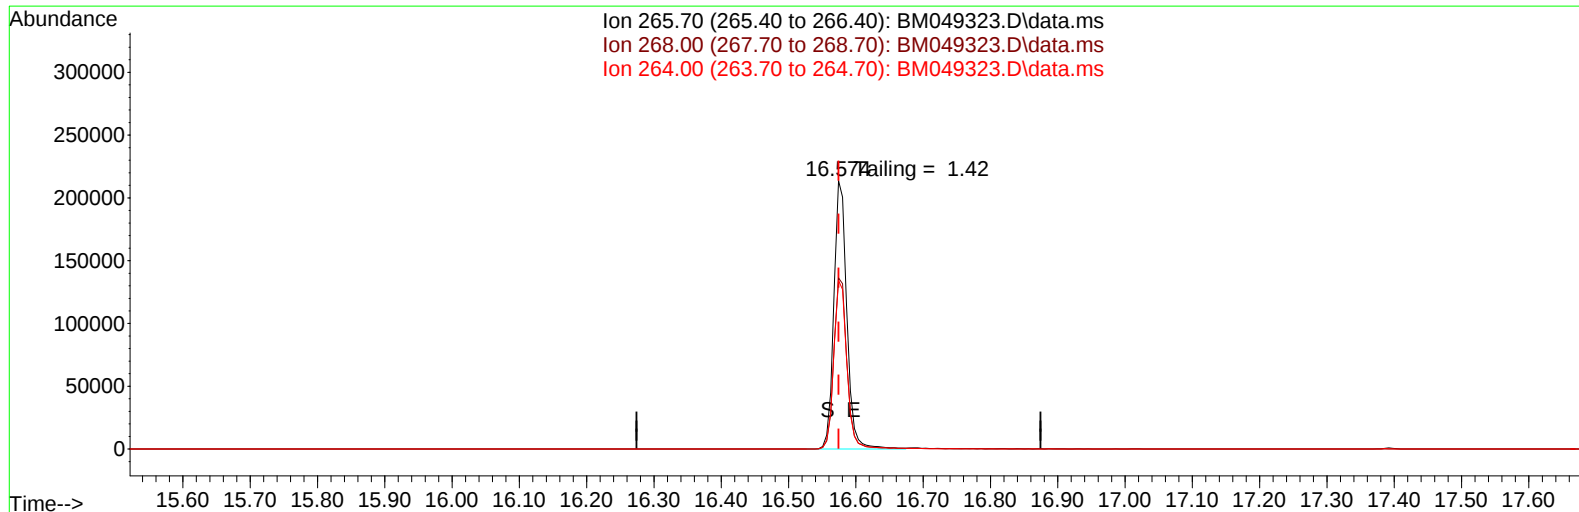

TIC: BM049323.D\data.ms

(70) Pentachlorophenol (C)

16.574min (0.000) 50264.59 ng




response 286754

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.80	63.71
264.00	61.70	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010325\
Data File : BM049323.D
Acq On : 03 Jan 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 03 13:09:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 13:09:35 2025
Response via : Initial Calibration

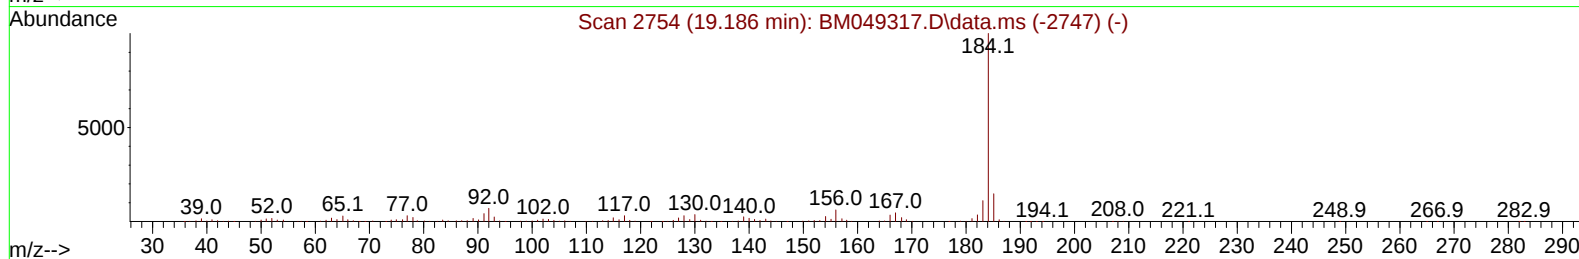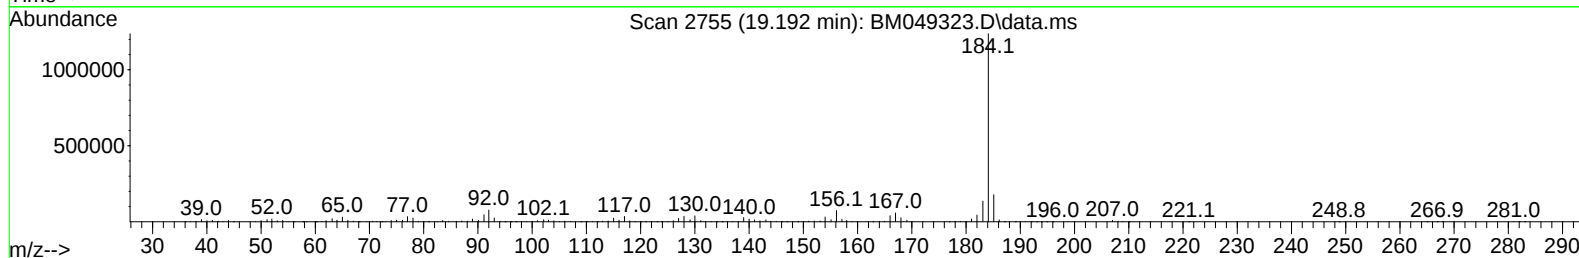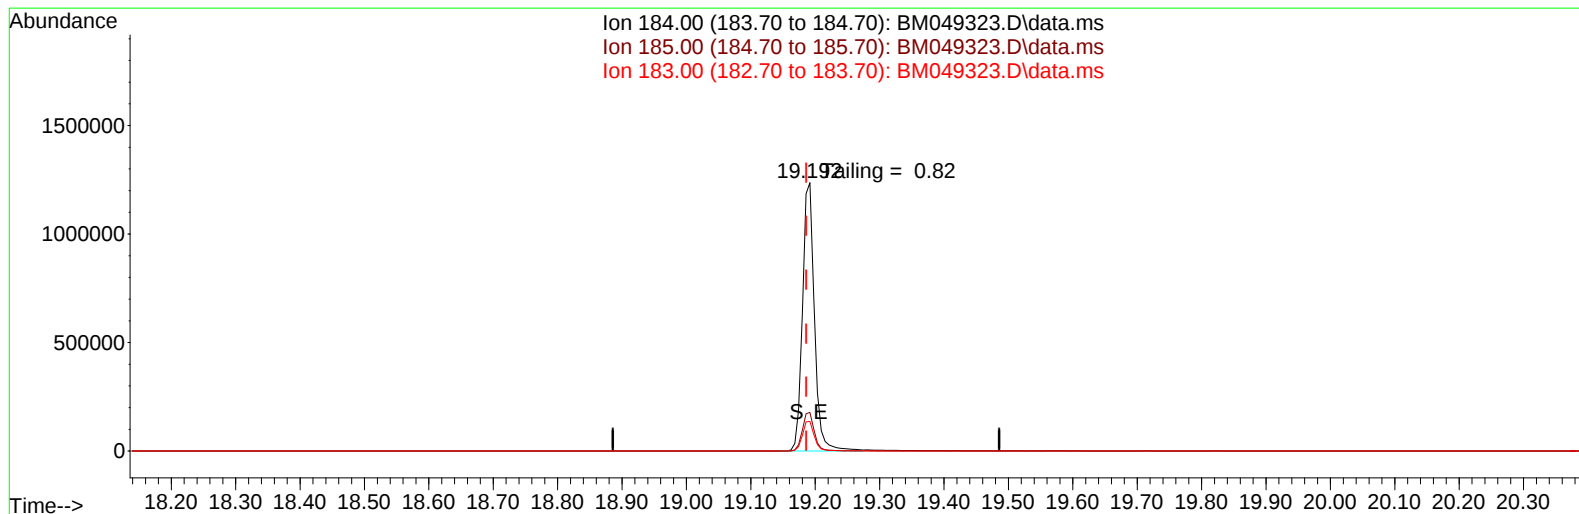

TIC: BM049323.D\data.ms

(77) Benzidine

19.192min (+ 0.006) 18290.10 ng

response 1618757

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.41
183.00	11.10	11.03
0.00	0.00	0.00