

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010522\
 Data File : BM033648.D
 Acq On : 05 Jan 2022 18:13
 Operator : CG/JU
 Sample : PB141851BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB141851BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.531	382	390	399	rBV	4379721	6474470	69.48%	12.602%
2	7.143	656	664	674	rBV	4092975	6656159	71.43%	12.956%
3	7.984	800	807	817	rBV	820794	1266414	13.59%	2.465%
4	9.148	997	1005	1014	rBV	2738849	4497814	48.27%	8.755%
5	10.801	1278	1286	1294	rBV	1076025	1768584	18.98%	3.442%
6	13.254	1696	1703	1713	rVB	6316226	9317987	100.00%	18.137%
7	14.624	1926	1936	1943	rBV	1431428	2109467	22.64%	4.106%
8	16.101	2180	2187	2202	rVB	3589742	4930389	52.91%	9.597%
9	17.360	2394	2401	2407	rBV	1382580	1949414	20.92%	3.794%
10	19.971	2839	2845	2850	rBV	6956332	8389759	90.04%	16.330%
11	21.518	3103	3108	3118	rVB	1544699	1966534	21.10%	3.828%
12	23.953	3515	3522	3530	rVB2	993508	2049603	22.00%	3.989%


Sum of corrected areas: 51376594

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010522\
Data File : BM033648.D
Acq On : 05 Jan 2022 18:13
Operator : CG/JU
Sample : PB141851BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141851BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

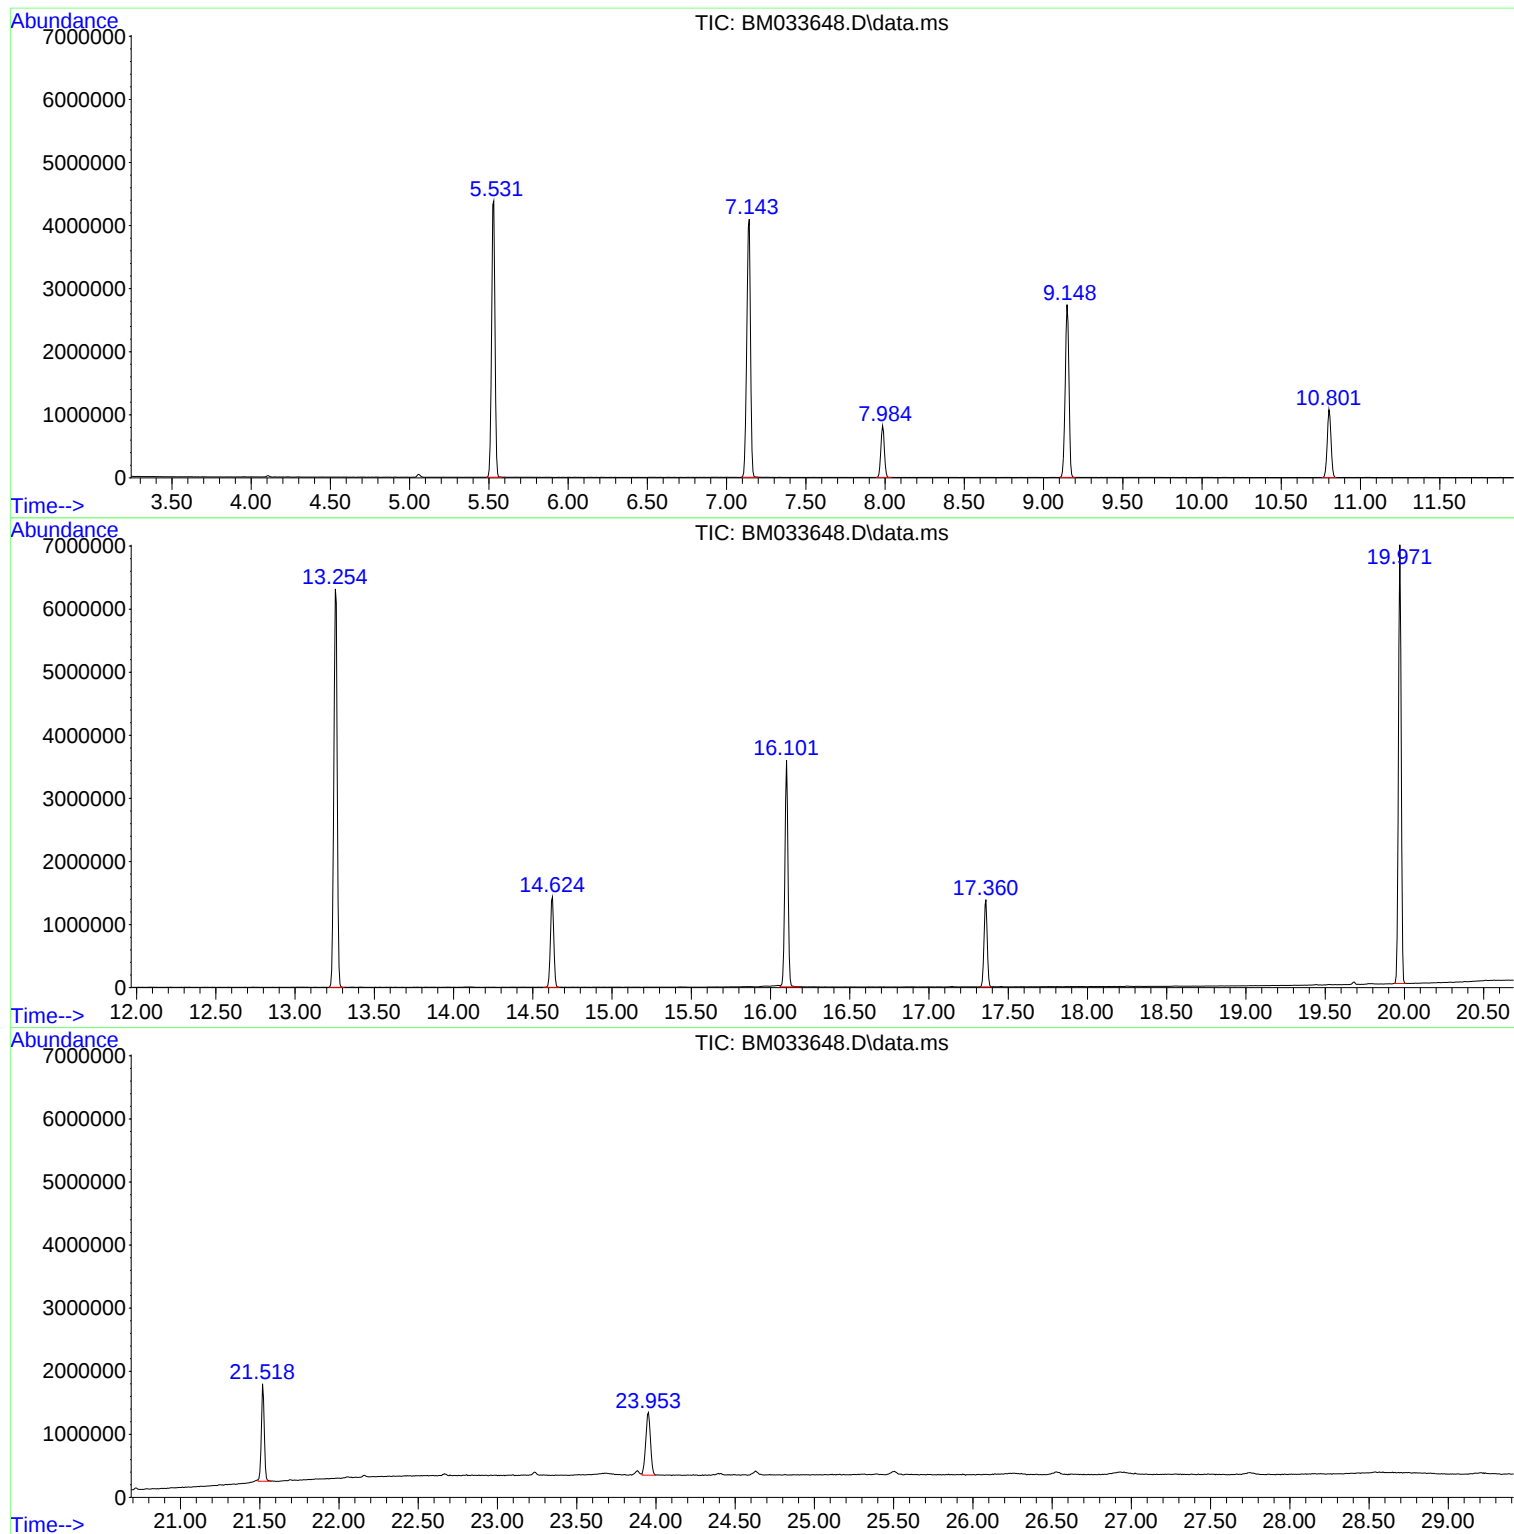

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010522\
Data File : BM033648.D
Acq On : 05 Jan 2022 18:13
Operator : CG/JU
Sample : PB141851BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141851BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010522\
Data File : BM033648.D
Acq On : 05 Jan 2022 18:13
Operator : CG/JU
Sample : PB141851BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141851BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------