


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010522\
 Data File : BM033639.D
 Acq On : 05 Jan 2022 11:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 05 17:07:26 2022

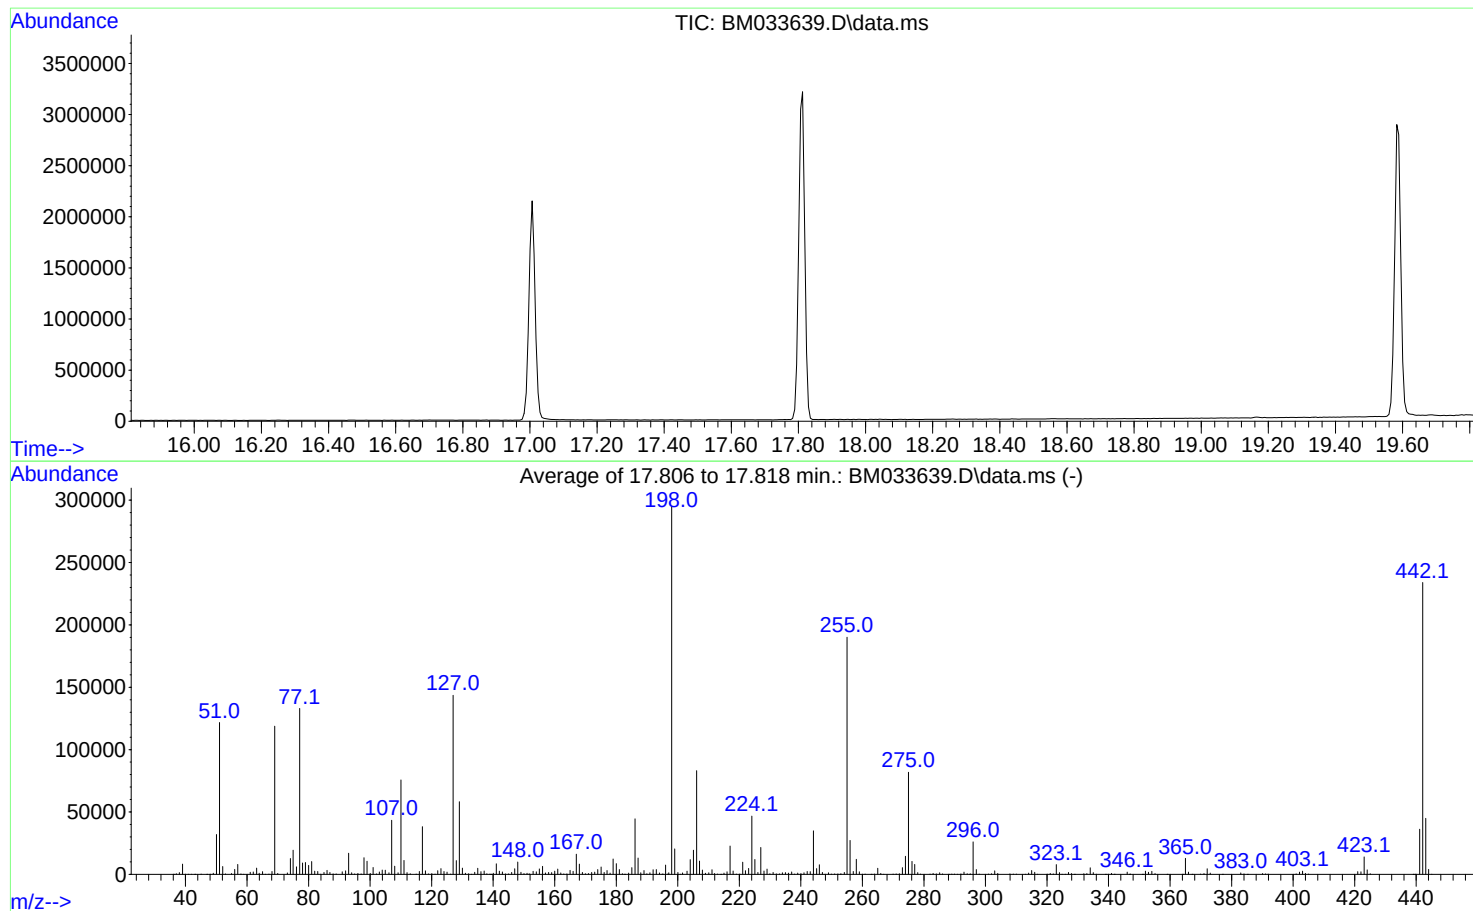




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	121801	PASS
68	69	0.00	2	1.9	2303	PASS
69	198	0.00	100	40.3	118792	PASS
70	69	0.00	2	0.6	731	PASS
127	198	10	80	48.7	143573	PASS
197	198	0.00	2	0.4	1316	PASS
198	198	100	100	100.0	294933	PASS
199	198	5	9	6.9	20415	PASS
275	198	10	60	27.7	81803	PASS
365	198	1	100	4.3	12828	PASS
441	198	0.01	100	12.3	36187	PASS
442	442	50	100	100.0	234005	PASS
443	442	15	24	19.2	44971	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010522\
 Data File : BM033639.D
 Acq On : 05 Jan 2022 11:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 05 18:01:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 05 17:07:26 2022
 Response via : Initial Calibration

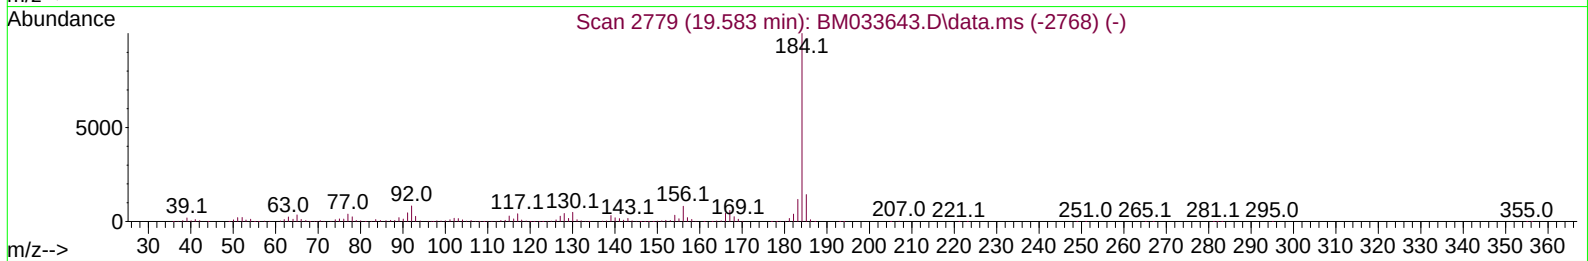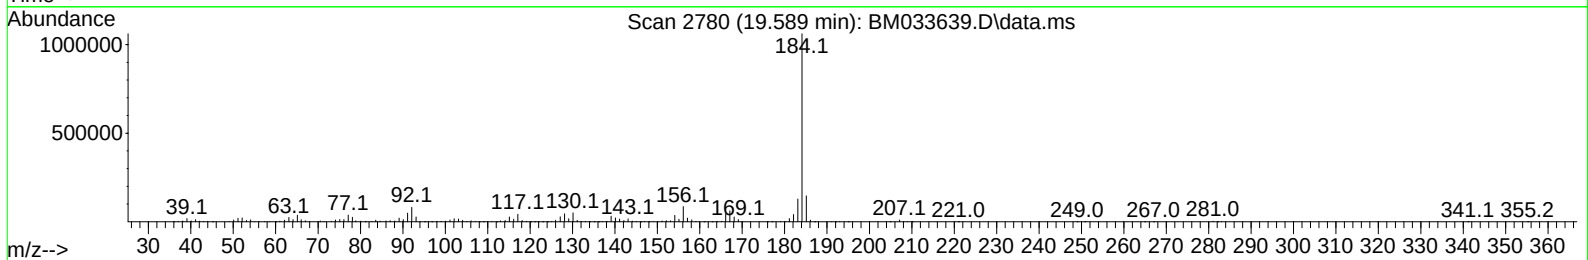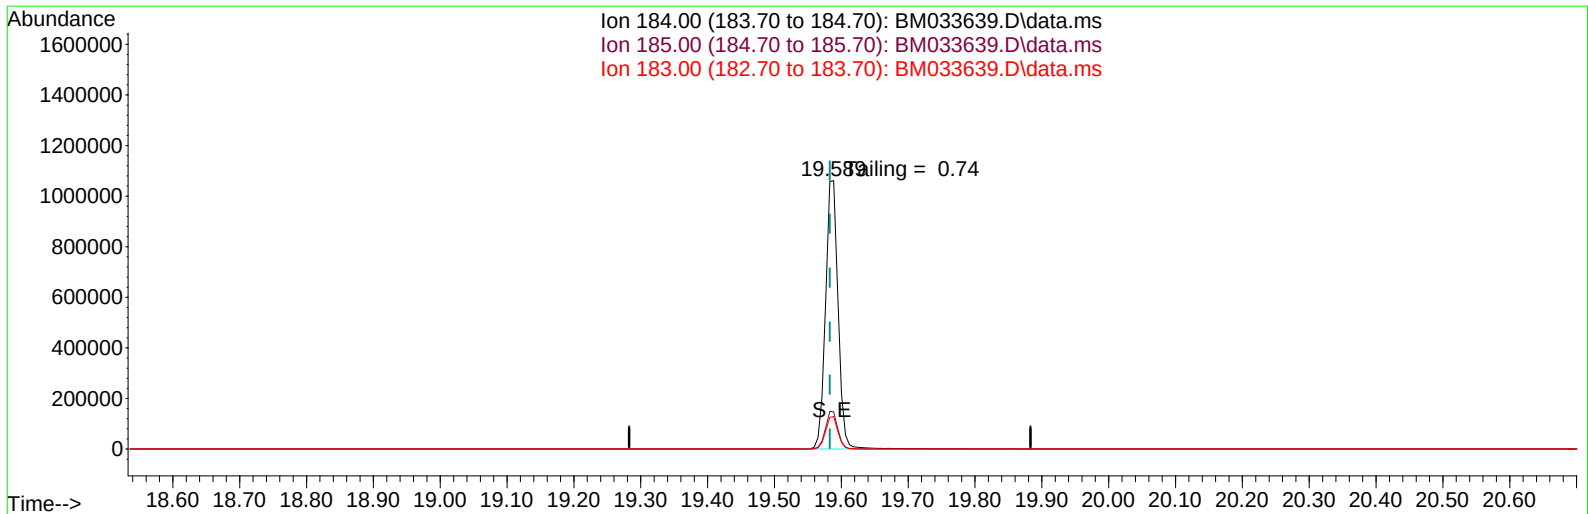

TIC: BM033639.D\data.ms

(77) Benzidine

19.589min (+ 0.006) 0.00 ng


response 1391722

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.84
183.00	12.10	12.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010522\
 Data File : BM033639.D
 Acq On : 05 Jan 2022 11:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 05 18:01:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 05 17:07:26 2022
 Response via : Initial Calibration

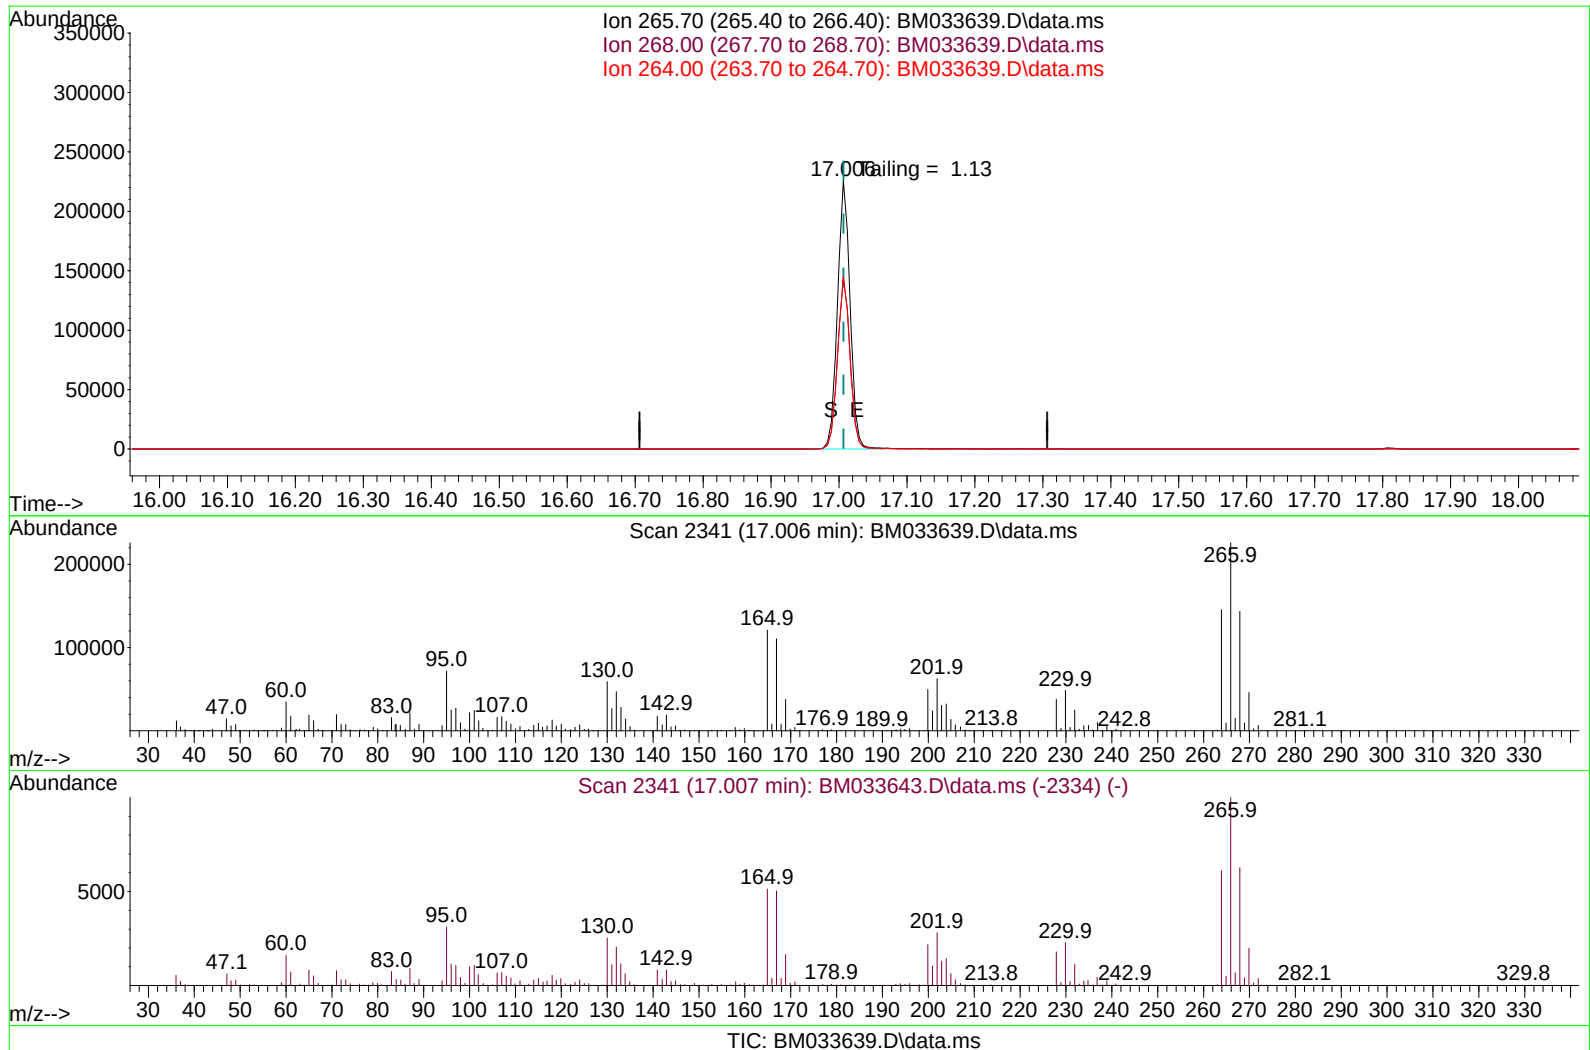

TIC: BM033639.D\data.ms

(70) Pentachlorophenol (C)

17.006min (-0.000) 0.00 ng

response 291514

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.56
264.00	61.40	64.41
0.00	0.00	0.00

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/5/2022	BNA_M	<u>BM033639.D</u>
Compound Name	Response	Retention Time
DDT	724949	20.82
DDD	12575	20.38
DDE	179	19.87
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12754	737703	1.73