

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010523\
 Data File : BM038375.D
 Acq On : 05 Jan 2023 12:22
 Operator : CG/JU
 Sample : PB149946BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK946

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038375.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	27	30	36	rVB	28273	32370	2.03%	0.193%
2	3.563	62	64	65	rBV2	2813	1608	0.10%	0.010%
3	3.799	100	104	121	rBV	296835	484666	30.41%	2.894%
4	4.122	156	159	166	rVB2	7960	13301	0.83%	0.079%
5	4.593	236	239	241	rBV3	1621	1764	0.11%	0.011%
6	5.010	309	310	314	rBV3	2058	2416	0.15%	0.014%
7	5.040	314	315	319	rVV3	1746	1997	0.13%	0.012%
8	5.175	336	338	342	rVB3	1659	1666	0.10%	0.010%
9	6.228	512	517	519	rVB3	1455	1830	0.11%	0.011%
10	7.157	669	675	689	rBV	327439	513200	32.20%	3.064%
11	7.328	697	704	712	rBV	245056	377107	23.66%	2.252%
12	7.528	731	738	749	rBV	317500	505678	31.72%	3.019%
13	7.681	760	764	766	rVB4	1224	1664	0.10%	0.010%
14	7.998	811	818	826	rBV	310212	481632	30.22%	2.876%
15	8.710	933	939	955	rBV	343806	552125	34.64%	3.297%
16	9.169	1009	1017	1027	rBV	281551	465969	29.23%	2.782%
17	9.892	1133	1140	1155	rBV	238208	392670	24.63%	2.344%
18	10.433	1222	1232	1246	rBV	325979	549684	34.49%	3.282%
19	10.810	1289	1296	1305	rBV	377387	615330	38.60%	3.674%
20	10.957	1314	1321	1339	rBV	290403	531718	33.36%	3.175%
21	12.398	1561	1566	1574	rVB4	2398	5624	0.35%	0.034%
22	12.786	1626	1632	1635	rBV2	767	1811	0.11%	0.011%
23	14.039	1839	1845	1855	rBV	529529	708152	44.43%	4.228%
24	14.327	1888	1894	1905	rBV	577387	814191	51.08%	4.861%
25	14.633	1940	1946	1956	rVB	525327	756315	47.45%	4.516%
26	14.833	1974	1980	2007	rBV	195731	337872	21.20%	2.017%
27	15.557	2100	2103	2107	rBV2	885	1704	0.11%	0.010%
28	15.621	2108	2114	2122	rBV	757219	1008785	63.29%	6.023%
29	15.745	2130	2135	2147	rBV	255730	352618	22.12%	2.105%
30	15.862	2152	2155	2160	rVB5	2484	3486	0.22%	0.021%
31	16.633	2282	2286	2290	rBV4	1133	1953	0.12%	0.012%
32	16.809	2313	2316	2321	rVB2	1804	2630	0.16%	0.016%
33	17.374	2406	2412	2422	rBV	639345	891302	55.92%	5.322%
34	17.474	2422	2429	2439	rVV	766654	1067091	66.95%	6.371%
35	17.739	2471	2474	2475	rBV2	1695	1860	0.12%	0.011%
36	17.880	2495	2498	2503	rVB3	3262	5049	0.32%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010523\
 Data File : BM038375.D
 Acq On : 05 Jan 2023 12:22
 Operator : CG/JU
 Sample : PB149946BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK946

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
 Title : SVOA CALIBRATION

37	17.956	2508	2511	2514	rBV4	1206	1675	0.11%	0.010%
38	18.333	2569	2575	2580	rVB6	1567	3204	0.20%	0.019%
39	18.821	2653	2658	2663	rBV6	4054	6662	0.42%	0.040%
40	19.039	2694	2695	2699	rBV4	2486	2930	0.18%	0.017%
41	19.321	2741	2743	2750	rVB4	7539	10450	0.66%	0.062%
42	19.392	2753	2755	2760	rVV2	5891	8016	0.50%	0.048%
43	19.615	2791	2793	2797	rBV3	4305	5001	0.31%	0.030%
44	19.668	2800	2802	2804	rVB3	5305	4218	0.26%	0.025%
45	19.756	2812	2817	2825	rBV	998154	1262289	79.19%	7.537%
46	20.733	2979	2983	2988	rVB	117321	126267	7.92%	0.754%
47	21.544	3116	3121	3129	rBV	775252	1028410	64.52%	6.140%
48	23.821	3501	3508	3516	rBV	836018	1593968	100.00%	9.517%
49	23.980	3528	3535	3543	rBV2	612974	1206690	75.70%	7.205%




Sum of corrected areas: 16748618

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010523\
Data File : BM038375.D
Acq On : 05 Jan 2023 12:22
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK946

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

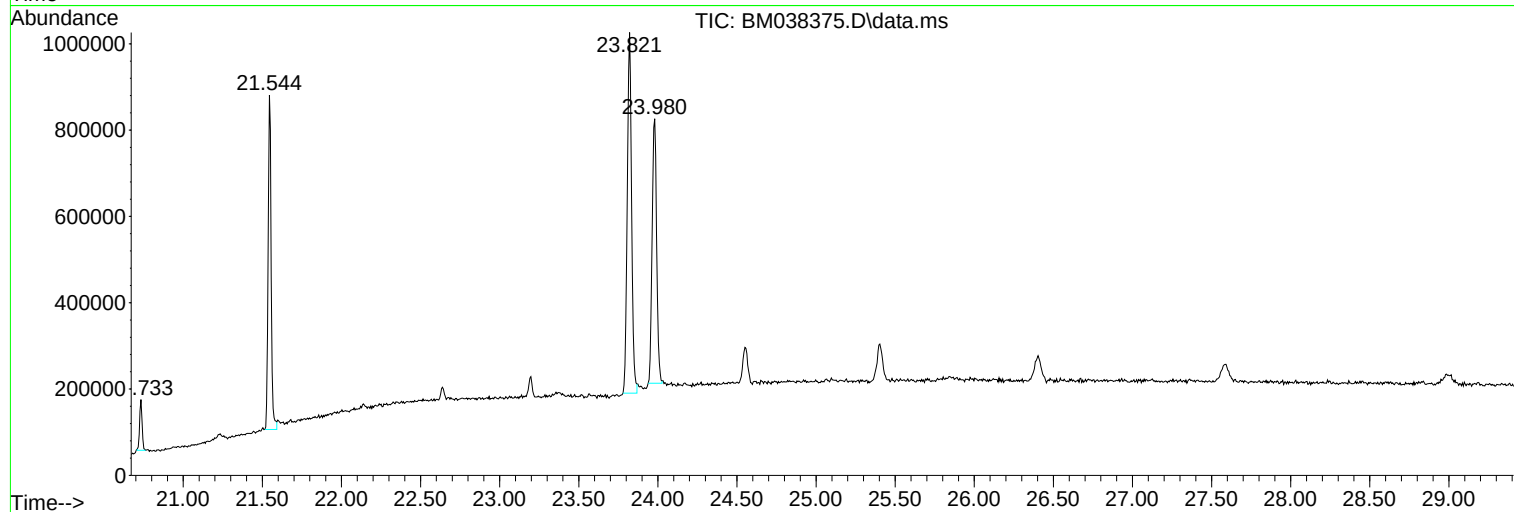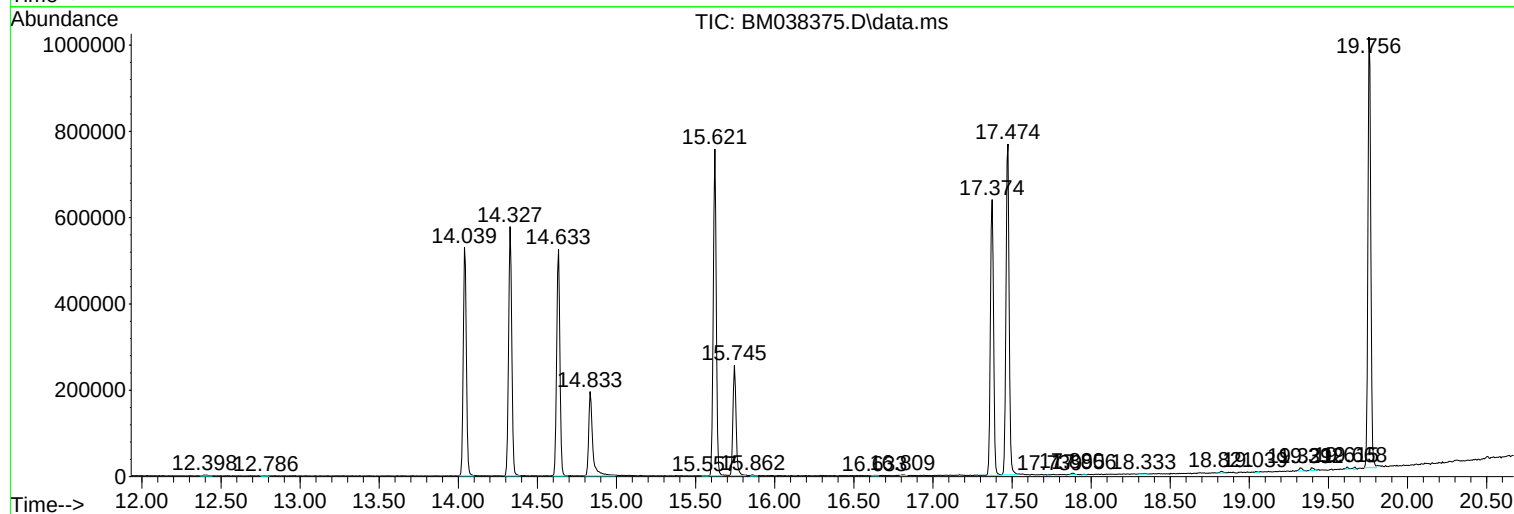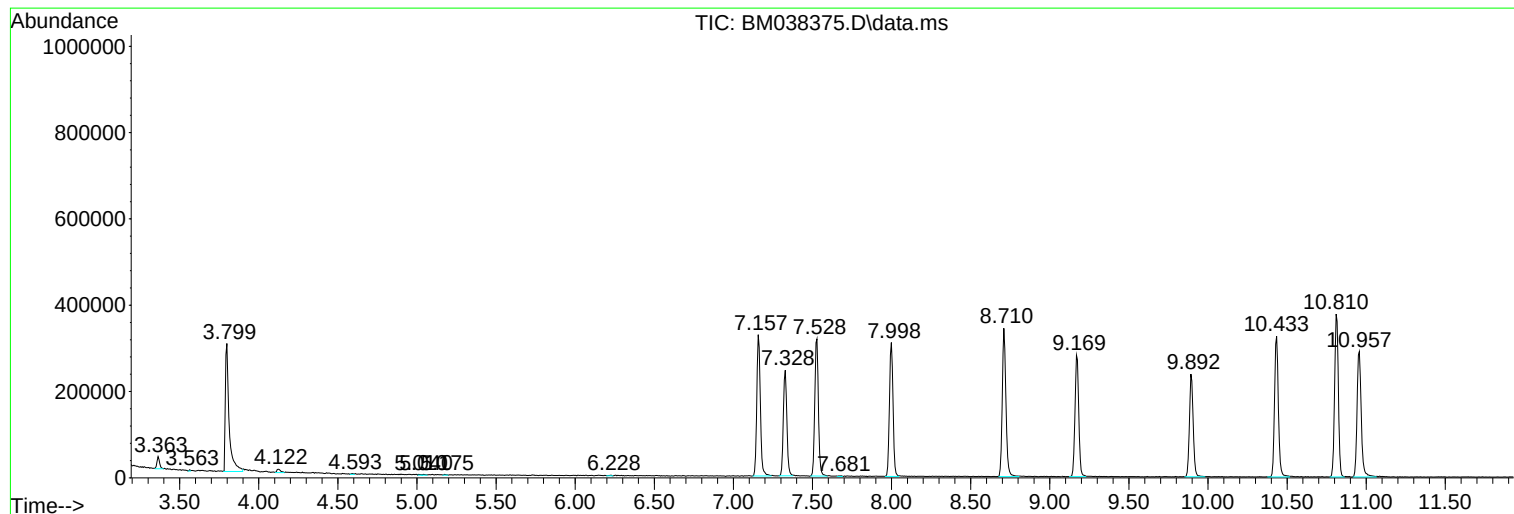

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010523\
Data File : BM038375.D
Acq On : 05 Jan 2023 12:22
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
SBLK946

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
20.733	2.46 ng/ul	126267	Chrysene-d12	21.544	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	86
2	Adipic acid, 2-ethylhexyl octyl ...	370	C22H42O4	1000324-48-6	83
3	Diisooctyl adipate	370	C22H42O4	001330-86-5	80
4	Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	80
5	Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	72

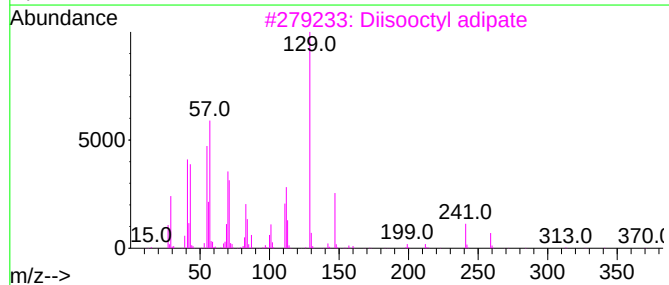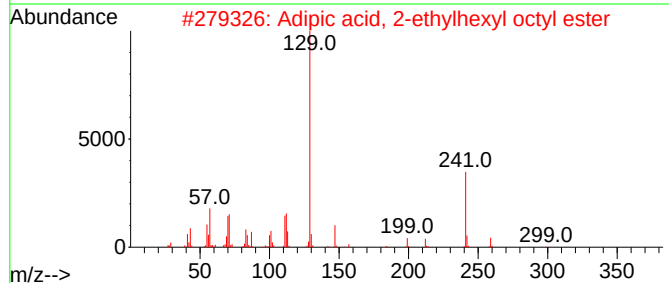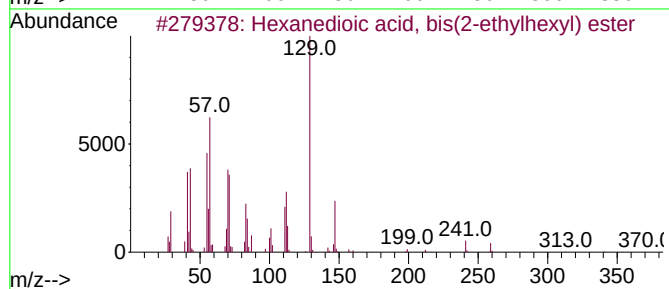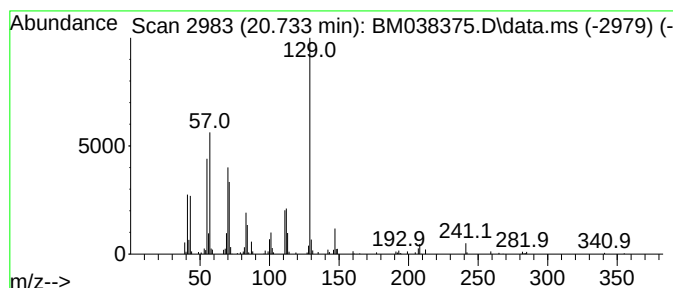

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010523\
Data File : BM038375.D
Acq On : 05 Jan 2023 12:22
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK946

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.733	2.5	ng/u1	126267	5	21.544	1028410	20.0