

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010715\
 Data File : BM000125.D
 Acq On : 07 Jan 2015 12:54
 Operator : TP/IZ
 Sample : SSTD3.219
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD3.219

Quant Time: Jan 08 01:42:02 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM010715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 08 01:34:24 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	3427	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	11826	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	7097	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	11684	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	10294	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	8645	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	49118	3.13	ng/ul	0.00
14) Fluoranthene-d10	19.25	212	79084	3.15	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.68	128	96095	3.03	ng/ul	98
5) 2-Methylnaphthalene	12.29	142	66279	3.16	ng/ul	100
7) Acenaphthylene	12.22	152	49118	3.08	ng/ul	96
8) Acenaphthene	14.54	153	68146	3.08	ng/ul	96
9) Fluorene	15.52	166	78963	3.11	ng/ul	95
11) Pentachlorophenol	16.87	266	8122	4.45	ng/ul	95
12) Phenanthrene	17.26	178	115383	3.19	ng/ul	98
13) Anthracene	17.35	178	111741	3.30	ng/ul	98
15) Fluoranthene	19.27	202	126066	3.18	ng/ul	96
17) Pyrene	19.63	202	126753	2.95	ng/ul	98
18) Benzo(a)anthracene	21.39	228	105799	3.12	ng/ul	96
19) Chrysene	21.44	228	108487	2.92	ng/ul	96
21) Benzo(b)fluoranthene	22.99	252	111937	3.29	ng/ul	93
22) Benzo(k)fluoranthene	23.04	252	99588	3.07	ng/ul	93
23) Benzo(a)pyrene	23.58	252	99473	3.23	ng/ul	93
24) Indeno(1,2,3-cd)pyrene	26.02	276	117742	3.35	ng/ul	100
25) Dibenzo(a,h)anthracene	26.03	278	96006	3.43	ng/ul	96
26) Benzo(g,h,i)perylene	26.73	276	100098	3.21	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010715\
Data File : BM000125.D
Acq On : 07 Jan 2015 12:54
Operator : TP/IZ
Sample : SSTD3.219
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD3.219

Quant Time: Jan 08 01:42:02 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM010715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 08 01:34:24 2015
Response via : Initial Calibration

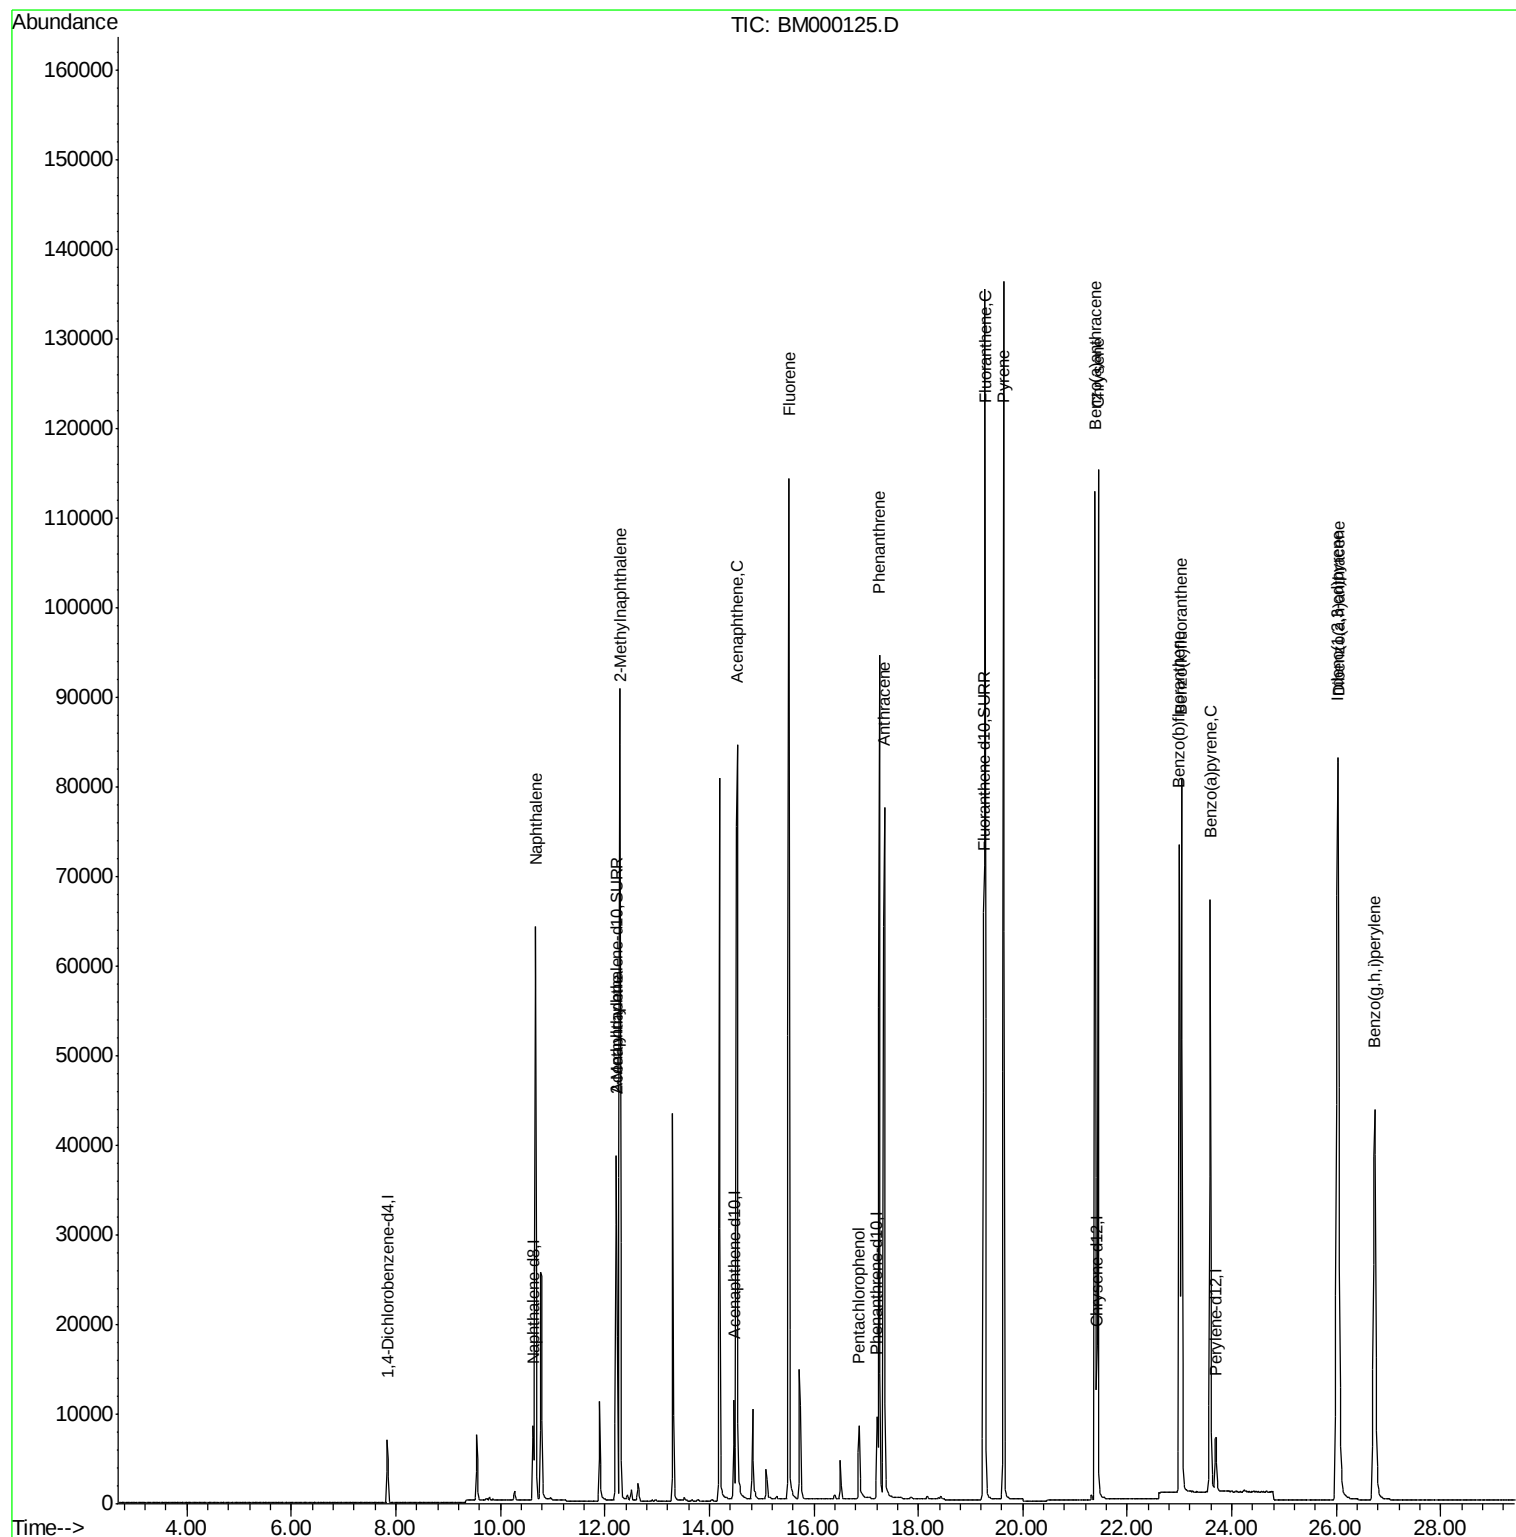



#3

Naphthalene

Concen: 3.03 ng/ul

RT: 10.68 min Scan# 1353

Delta R.T. -0.00 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54

Instrument :

BNA_M

ClientSampleId :

SSTD3.219


Tgt Ion:128 Resp: 96095

Ion Ratio Lower Upper

128 100

129 11.3 9.5 14.3




127 11.8 10.4 15.6

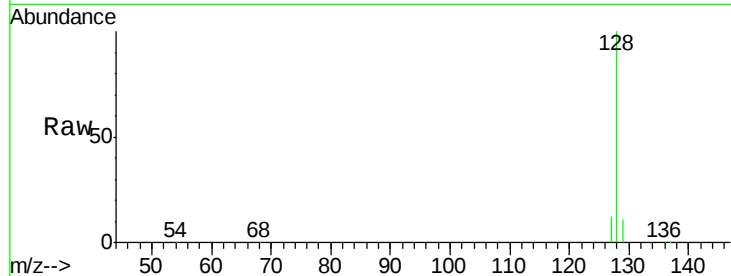

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

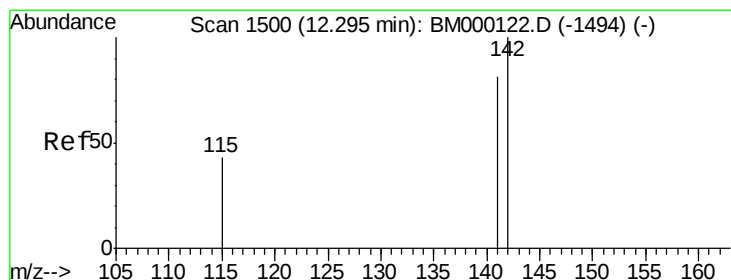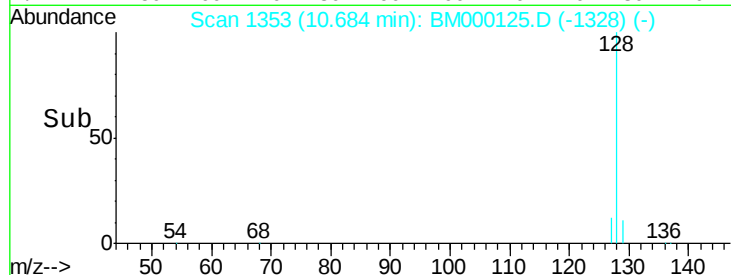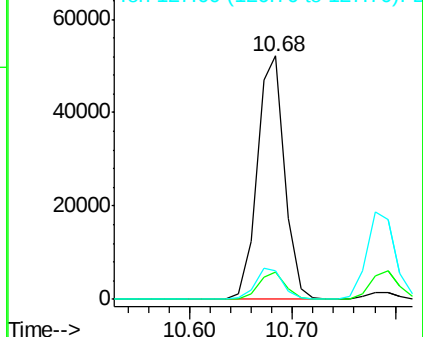

#5

2-Methylnaphthalene

Concen: 3.16 ng/ul

RT: 12.29 min Scan# 1500

Delta R.T. -0.00 min

Lab File: BM000125.D


Acq: 07 Jan 2015 12:54

Tgt Ion:142 Resp: 66279

Ion Ratio Lower Upper



142 100


141 86.2 68.9 103.3



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

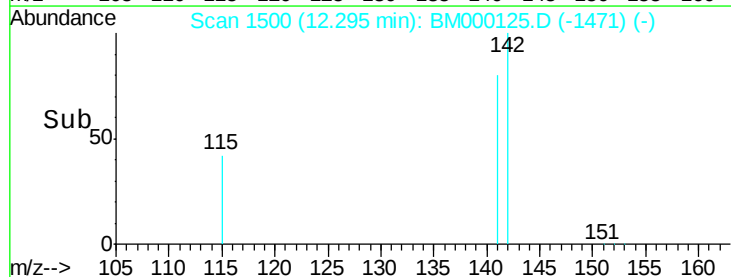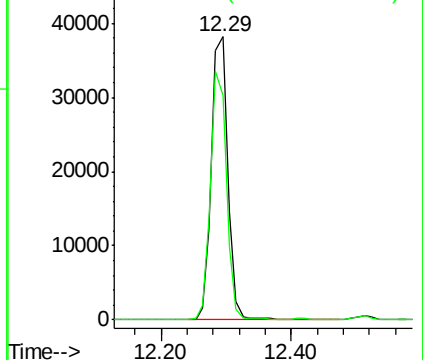

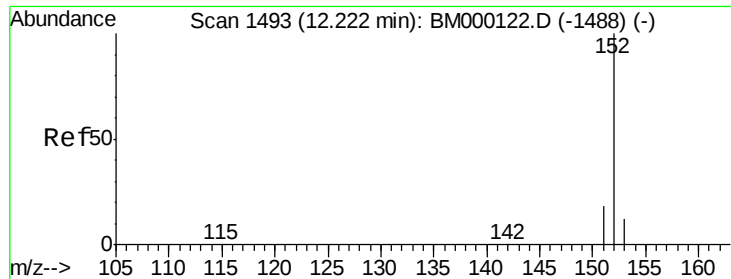

#7

Acenaphthylene

Concen: 3.08 ng/ul

RT: 12.22 min Scan# 1493

Delta R.T. -0.00 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54

Instrument :

BNA_M

ClientSampleId :

SSTD3.219


Tgt Ion:152 Resp: 49118

Ion Ratio Lower Upper

152 100

151 17.7 15.4 23.2




153 12.0 11.0 16.4



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

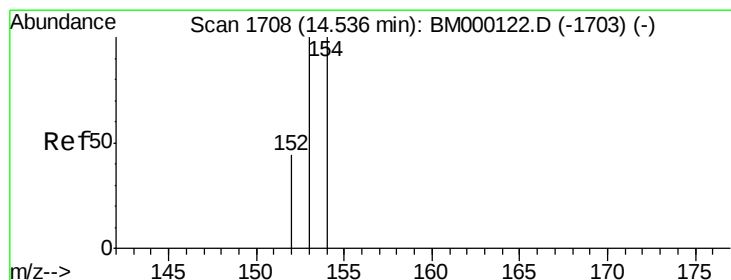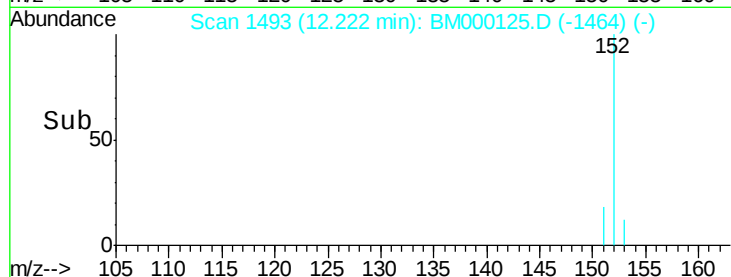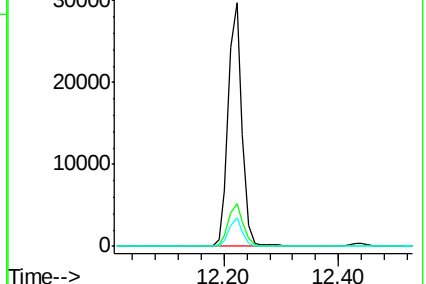

#8

Acenaphthene

Concen: 3.08 ng/ul

RT: 14.54 min Scan# 1708

Delta R.T. -0.00 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54


Tgt Ion:153 Resp: 68146

Ion Ratio Lower Upper

153 100

152 41.9 35.8 53.6



154 103.4 79.9 119.9

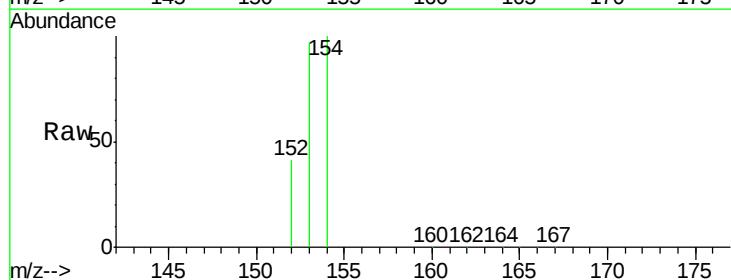

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

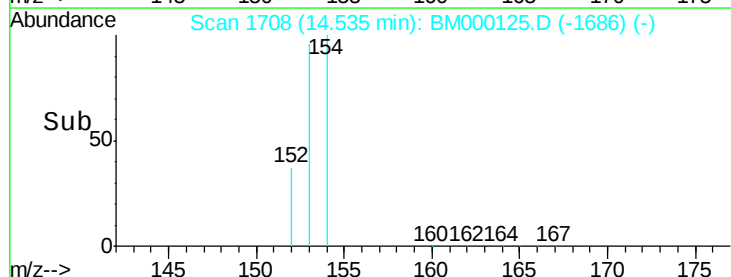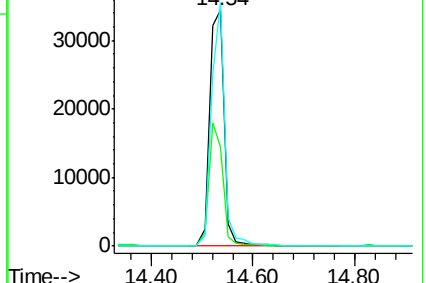



#9

Fluorene

Concen: 3.11 ng/ul

RT: 15.52 min Scan# 1772

Delta R.T. -0.00 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54

Instrument :

BNA_M

ClientSampleId :

SSTD3.219





Tgt Ion:166 Resp: 78963

Ion Ratio Lower Upper

166 100

165 90.4 77.0 115.4

167 13.9 11.0 16.6

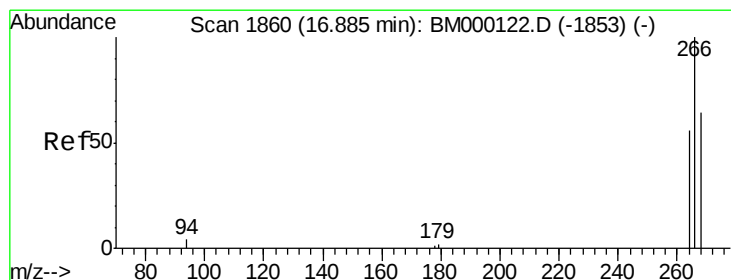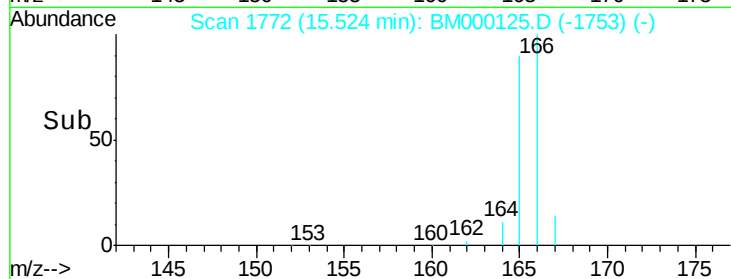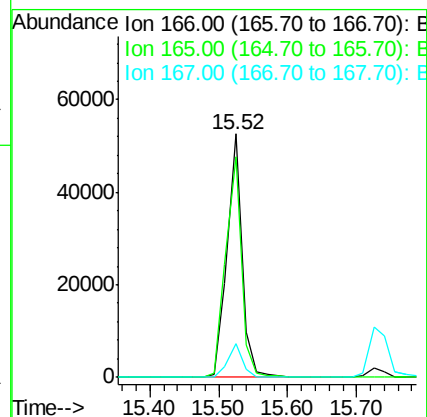

#11

Pentachlorophenol

Concen: 4.45 ng/ul

RT: 16.87 min Scan# 1859

Delta R.T. -0.02 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54




Tgt Ion:266 Resp: 8122


Ion Ratio Lower Upper

266 100

264 62.3 53.9 80.9

268 63.9 49.2 73.8

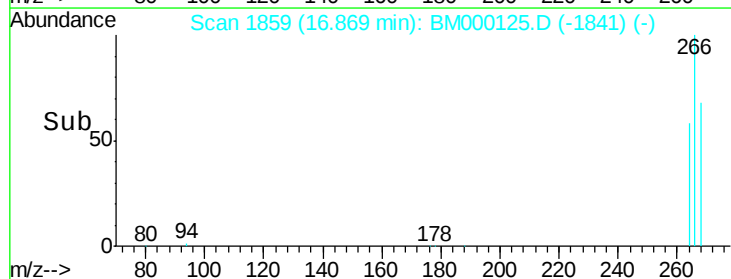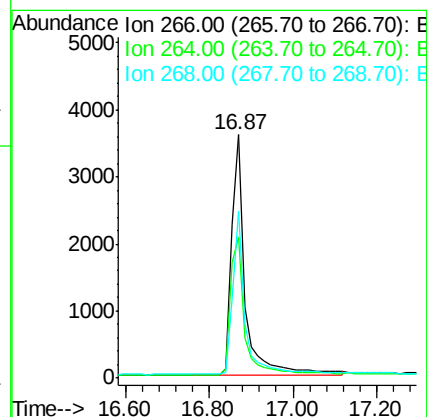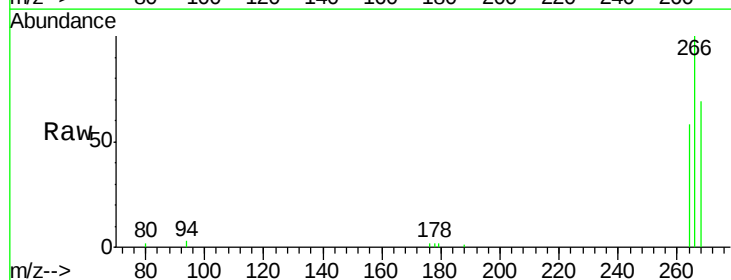

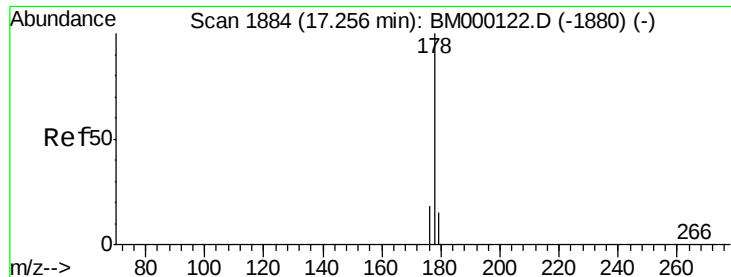

#12

Phenanthrene

Concen: 3.19 ng/ul

RT: 17.26 min Scan# 1884

Delta R.T. -0.00 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54

Instrument :

BNA_M

ClientSampleId :

SSTD3.219


Tgt Ion:178 Resp: 115383

Ion Ratio Lower Upper

178 100

176 17.0 15.1 22.7




179 16.2 13.0 19.4



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

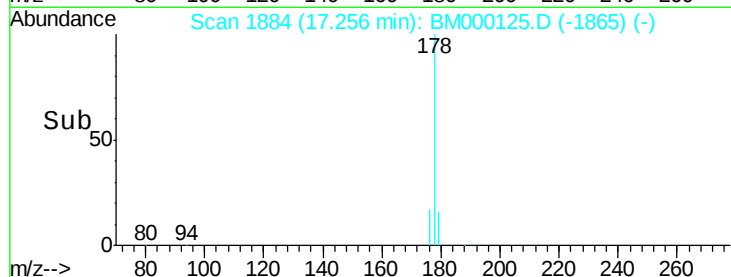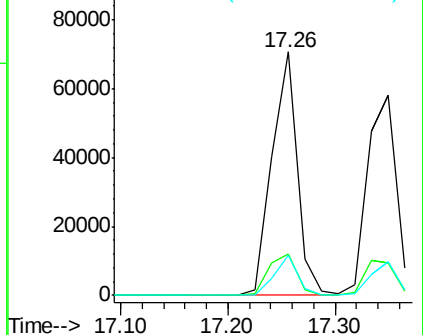

#13

Anthracene

Concen: 3.30 ng/ul

RT: 17.35 min Scan# 1890

Delta R.T. -0.00 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54


Tgt Ion:178 Resp: 111741

Ion Ratio Lower Upper

178 100

176 16.3 14.6 21.8



179 16.6 13.1 19.7




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

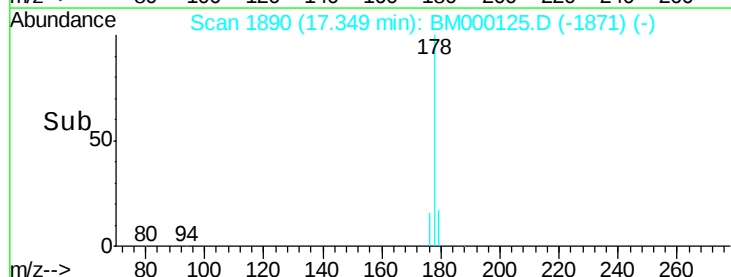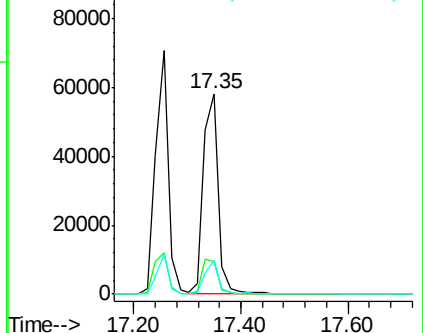

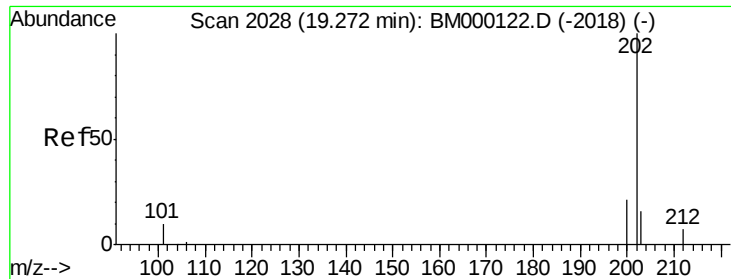

#15

Fluoranthene

Concen: 3.18 ng/u1

RT: 19.27 min Scan# 2028

Delta R.T. -0.00 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54

Instrument :

BNA_M

ClientSampleId :

SSTD3.219


Tgt Ion:202 Resp: 126066

Ion Ratio Lower Upper

202 100

101 7.4 0.0 30.5




203 16.9 0.0 36.6



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

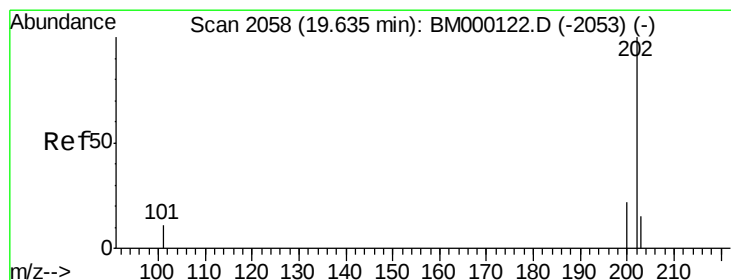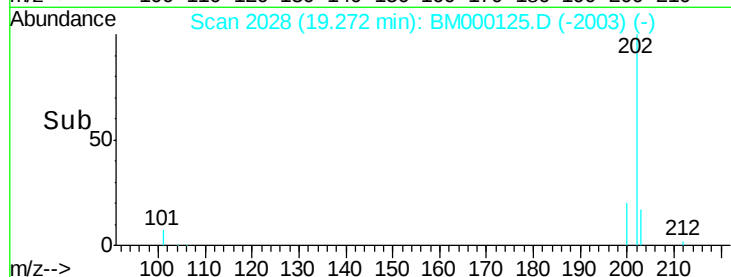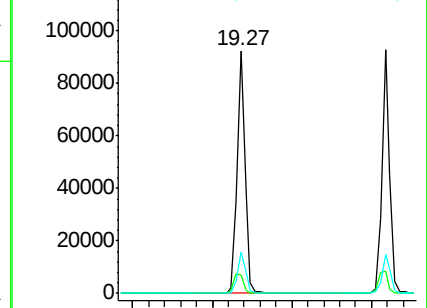

#17

Pyrene

Concen: 2.95 ng/u1

RT: 19.63 min Scan# 2058

Delta R.T. -0.00 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54


Tgt Ion:202 Resp: 126753

Ion Ratio Lower Upper

202 100

200 21.3 17.9 26.9



203 16.2 12.8 19.2

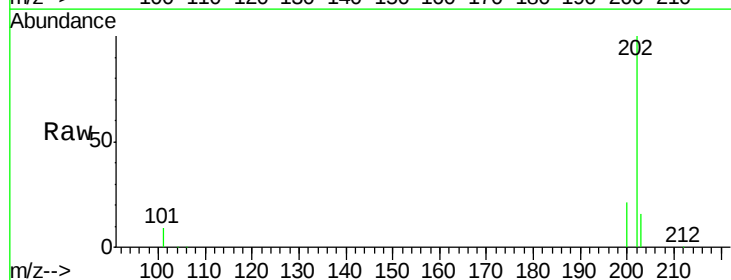


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

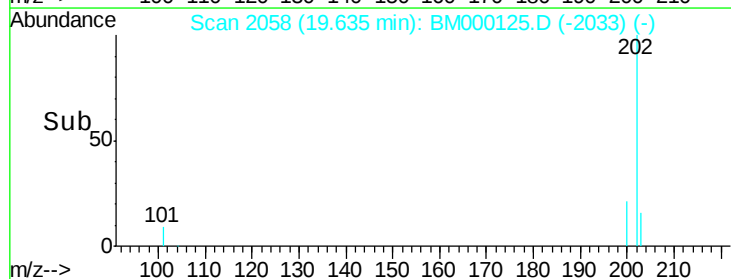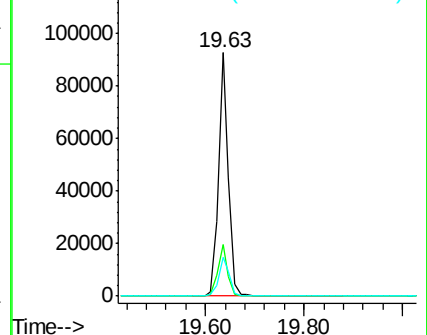

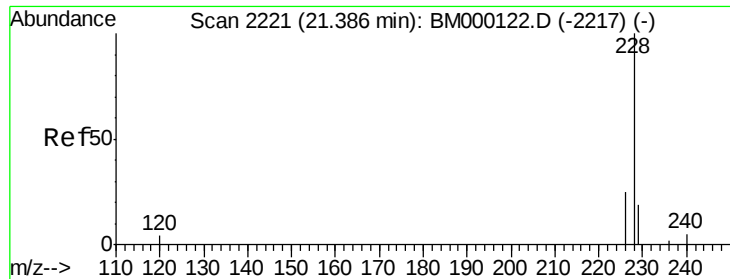

#18

Benzo(a)anthracene

Concen: 3.12 ng/ul

RT: 21.39 min Scan# 2221

Delta R.T. -0.00 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54

Instrument :

BNA_M

ClientSampleId :

SSTD3.219


Tgt Ion:228 Resp: 105799

Ion Ratio Lower Upper




228 100

226 23.7 20.8 31.2

229 21.0 15.5 23.3

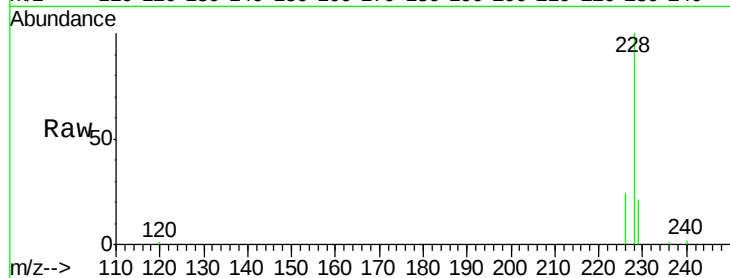

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

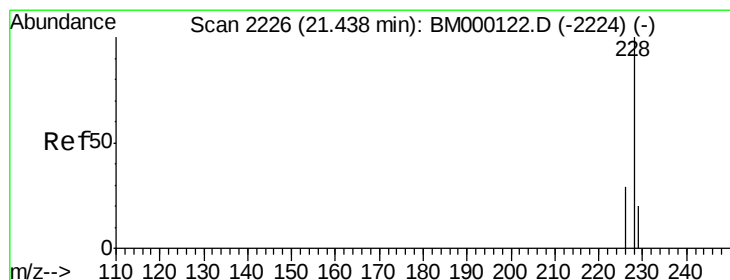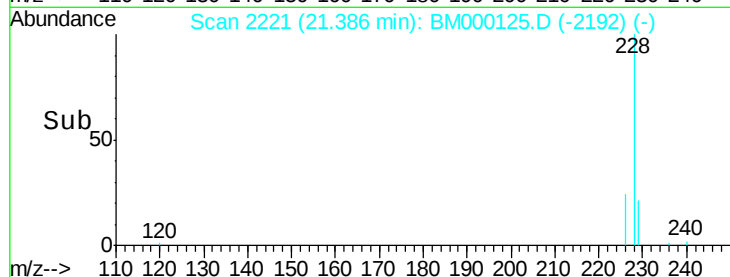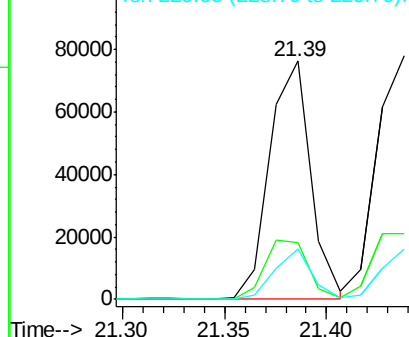

#19

Chrysene

Concen: 2.92 ng/ul

RT: 21.44 min Scan# 2226

Delta R.T. -0.00 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54


Tgt Ion:228 Resp: 108487

Ion Ratio Lower Upper



228 100


226 27.0 23.8 35.6

229 20.6 15.8 23.8

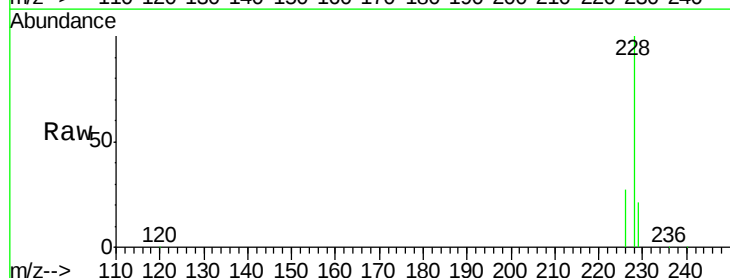

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

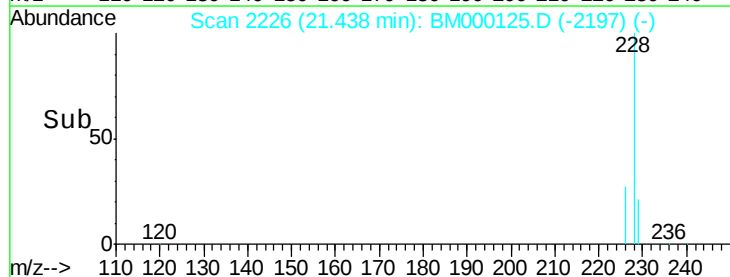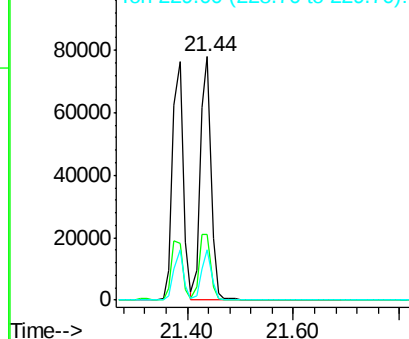

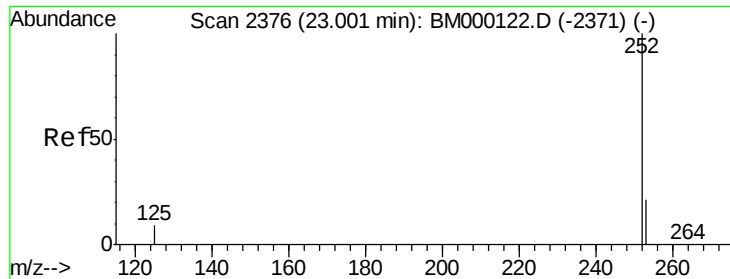

#21

Benzo(b)fluoranthene

Concen: 3.29 ng/u1

RT: 22.99 min Scan# 2375

Delta R.T. -0.01 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54

Instrument :

BNA_M

ClientSampleId :

SSTD3.219


Tgt Ion:252 Resp: 111937

Ion Ratio Lower Upper

252 100

253 20.3 0.0 48.2




125 9.4 0.0 21.6

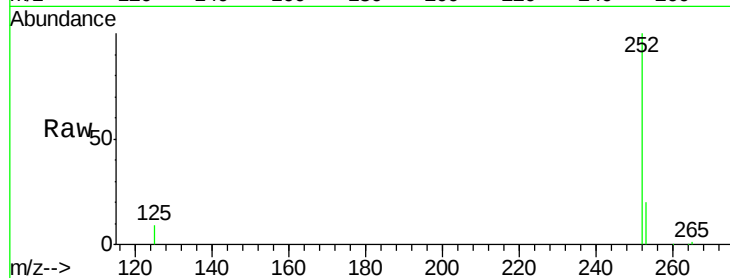

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

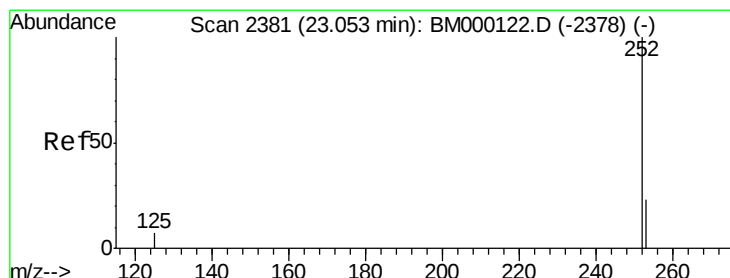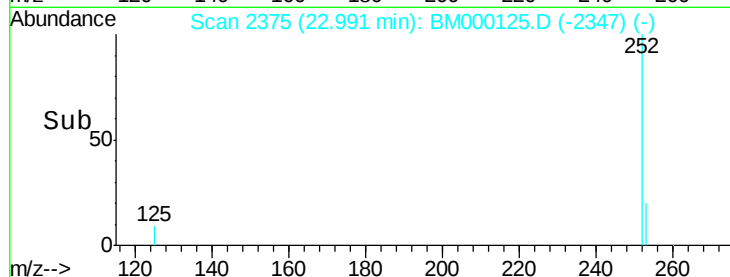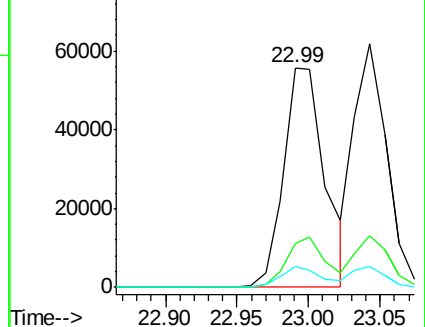

#22

Benzo(k)fluoranthene

Concen: 3.07 ng/u1

RT: 23.04 min Scan# 2380

Delta R.T. -0.01 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54


Tgt Ion:252 Resp: 99588

Ion Ratio Lower Upper

252 100

253 21.5 20.5 30.7



125 8.5 7.8 11.8

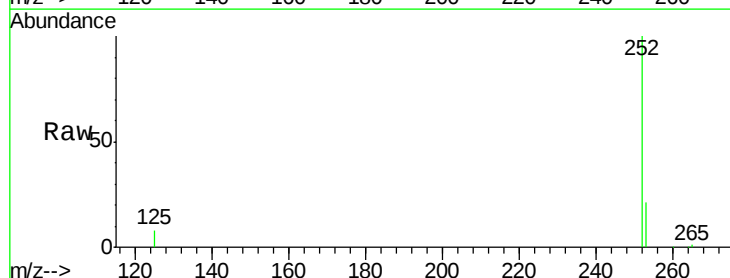


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

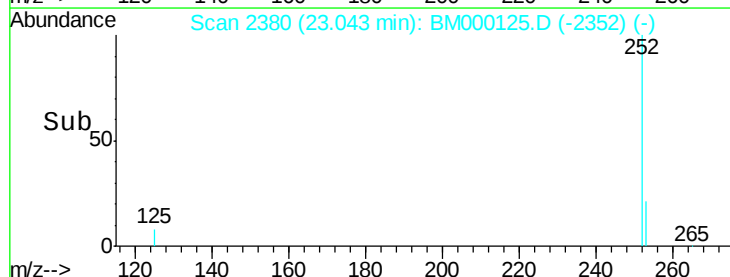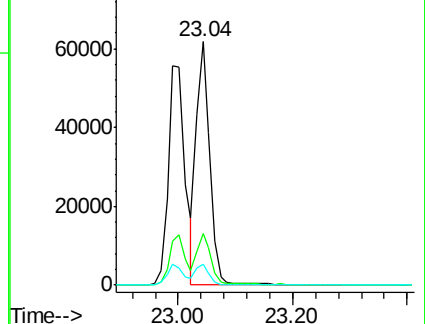

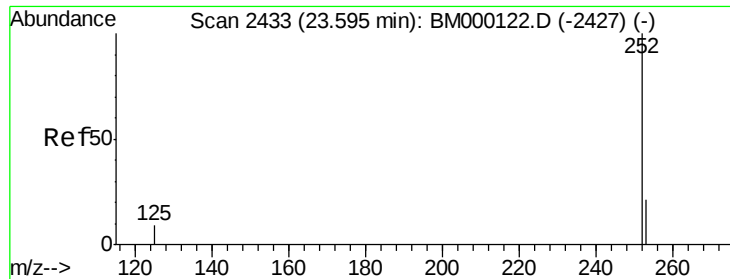

#23

Benzo(a)pyrene

Concen: 3.23 ng/ul

RT: 23.58 min Scan# 2432

Delta R.T. -0.01 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54

Instrument :

BNA_M

ClientSampleId :

SSTD3.219


Tgt Ion:252 Resp: 99473

Ion Ratio Lower Upper

252 100

253 20.7 19.8 29.6




125 10.2 9.2 13.8

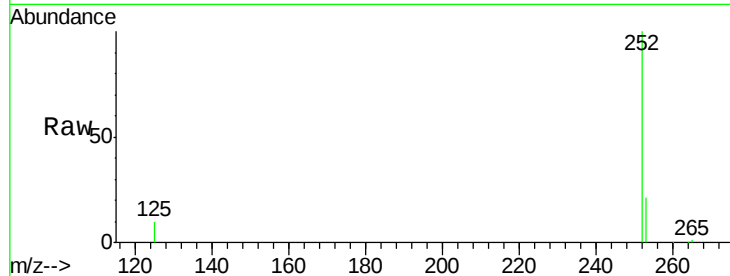

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

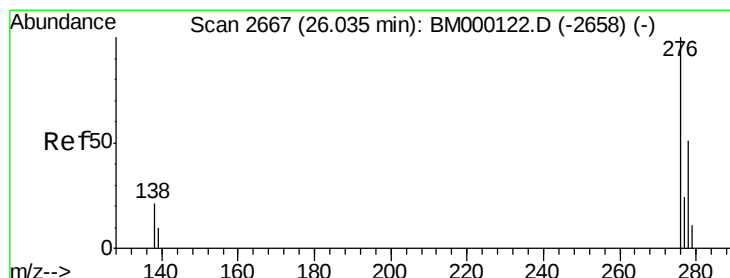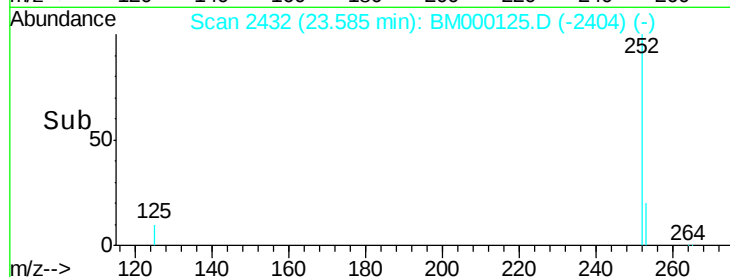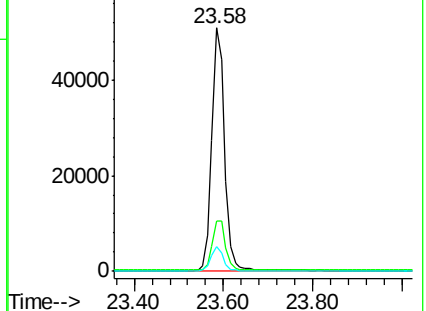

#24

Indeno(1,2,3-cd)pyrene

Concen: 3.35 ng/ul

RT: 26.02 min Scan# 2666

Delta R.T. -0.01 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54


Tgt Ion:276 Resp: 117742

Ion Ratio Lower Upper

276 100

138 21.8 17.6 26.4



277 24.6 19.9 29.9

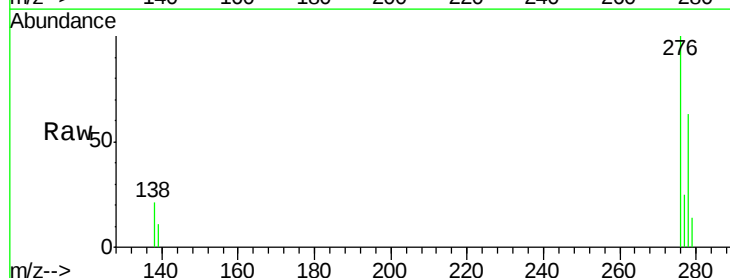


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

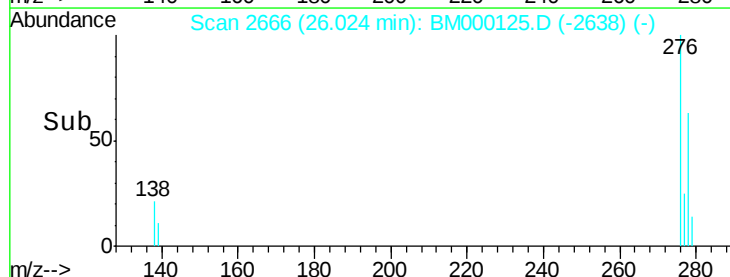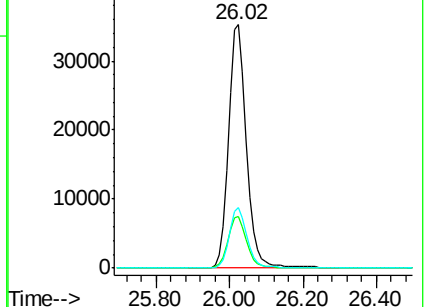

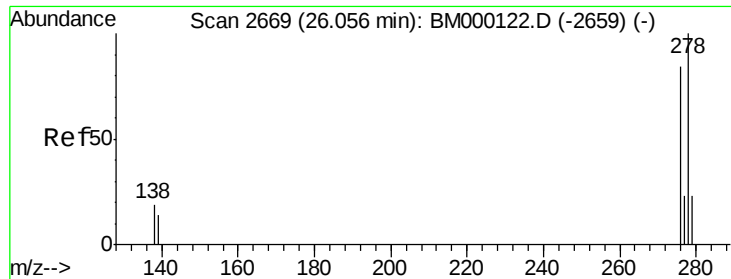

#25

Dibenzo(a,h)anthracene

Concen: 3.43 ng/ul

RT: 26.03 min Scan# 2667

Delta R.T. -0.02 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54

Instrument :

BNA_M

ClientSampleId :

SSTD3.219


Tgt Ion:278 Resp: 96006

Ion Ratio Lower Upper

278 100

139 15.2 12.6 18.8




279 22.9 20.6 30.8



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

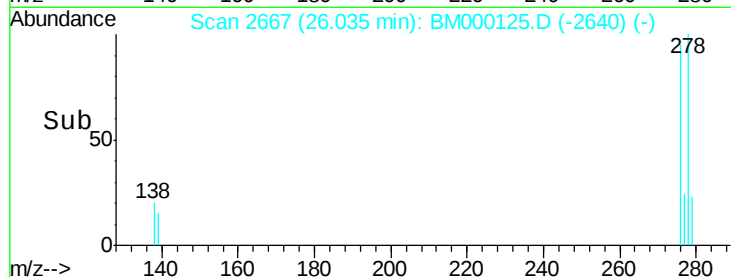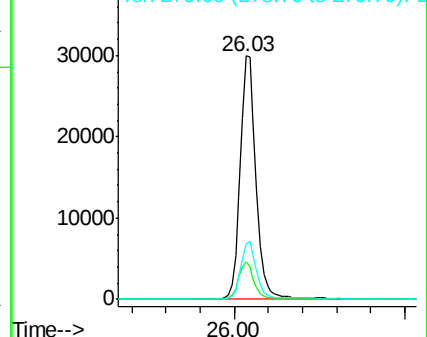

#26

Benzo(g,h,i)perylene

Concen: 3.21 ng/ul

RT: 26.73 min Scan# 2734

Delta R.T. -0.01 min

Lab File: BM000125.D

Acq: 07 Jan 2015 12:54


Tgt Ion:276 Resp: 100098

Ion Ratio Lower Upper

276 100

277 23.4 20.0 30.0

138 18.2 15.7 23.5



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

