
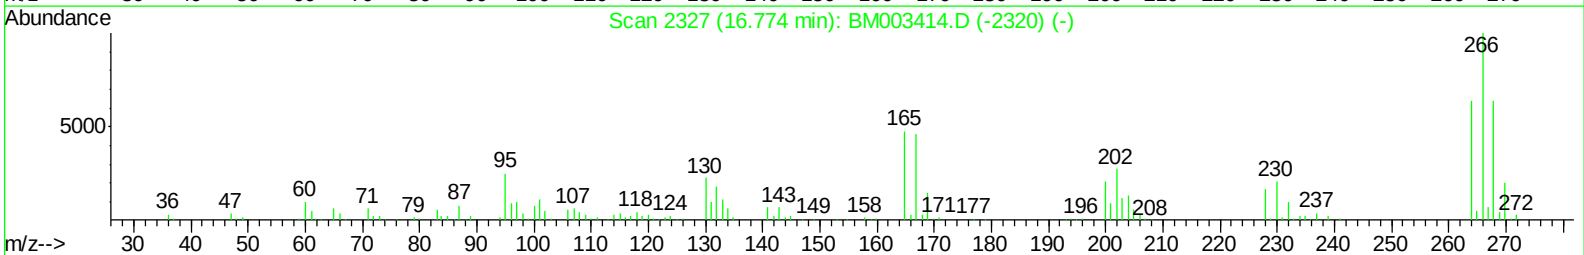
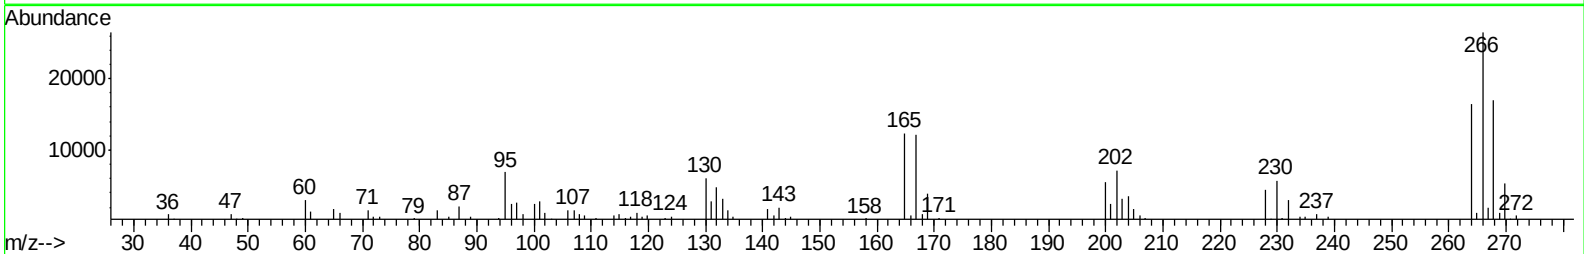


```
Data Path : Z:\HPCHEM1\BNA M\Data\BM010816\  
Data File : BM003923.D  
Acq On    : 08 Jan 2016  14:58  
Operator  : SJ/UM  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Jan 11 07:14:14 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

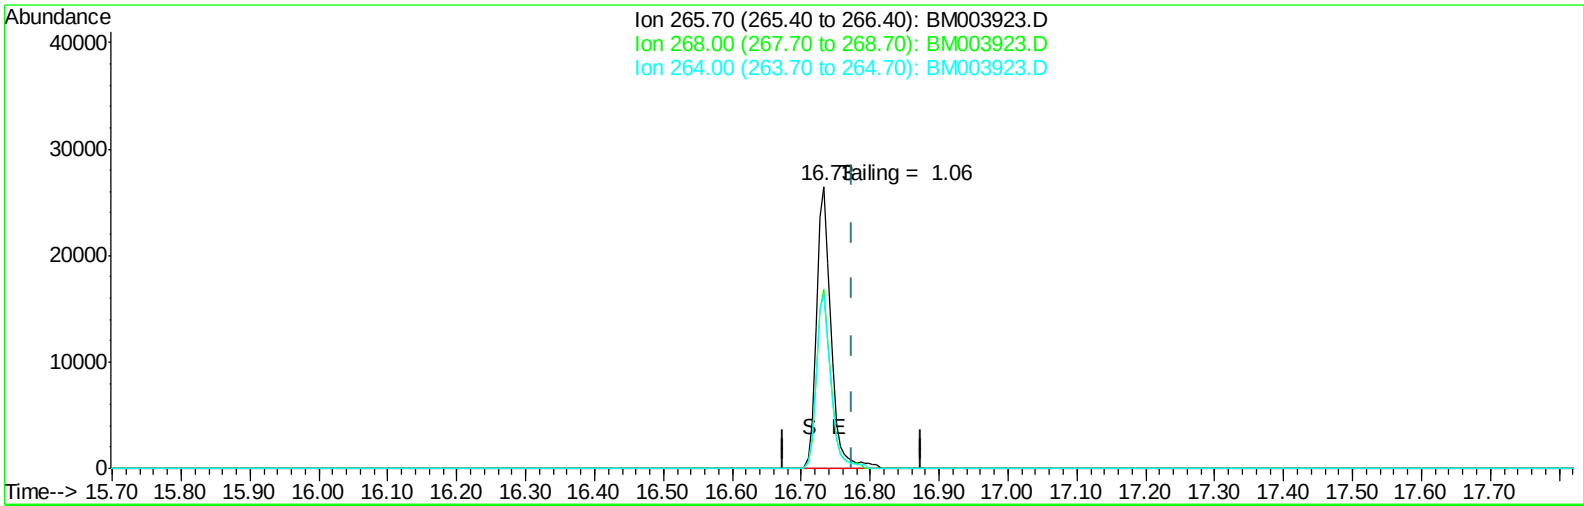

TIC: BM003923.D

(69) Pentachlorophenol (C)




16.733min (-0.041) 0.00ng

response 38846

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.86
264.00	61.20	61.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM010816\
Data File : BM003923.D
Acq On : 08 Jan 2016 14:58
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 07:14:14 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

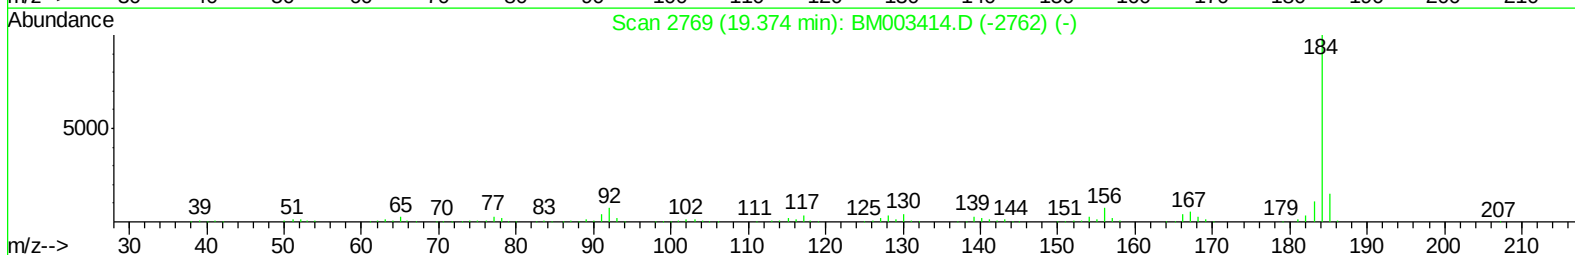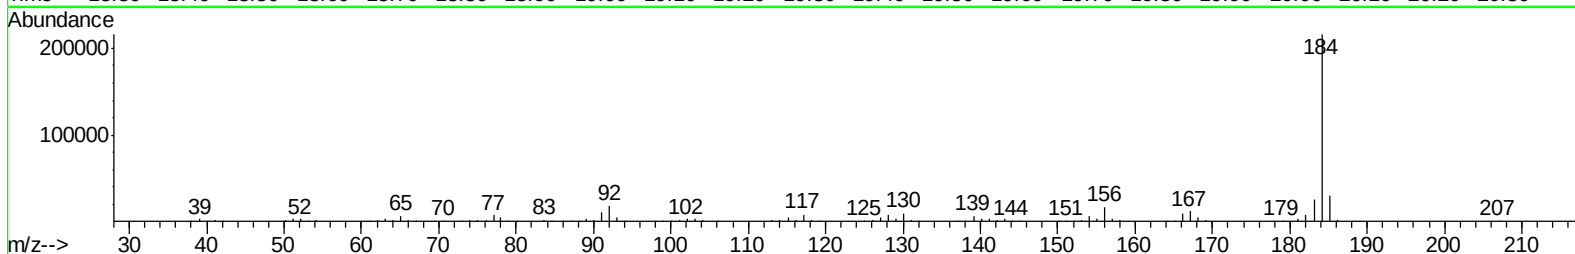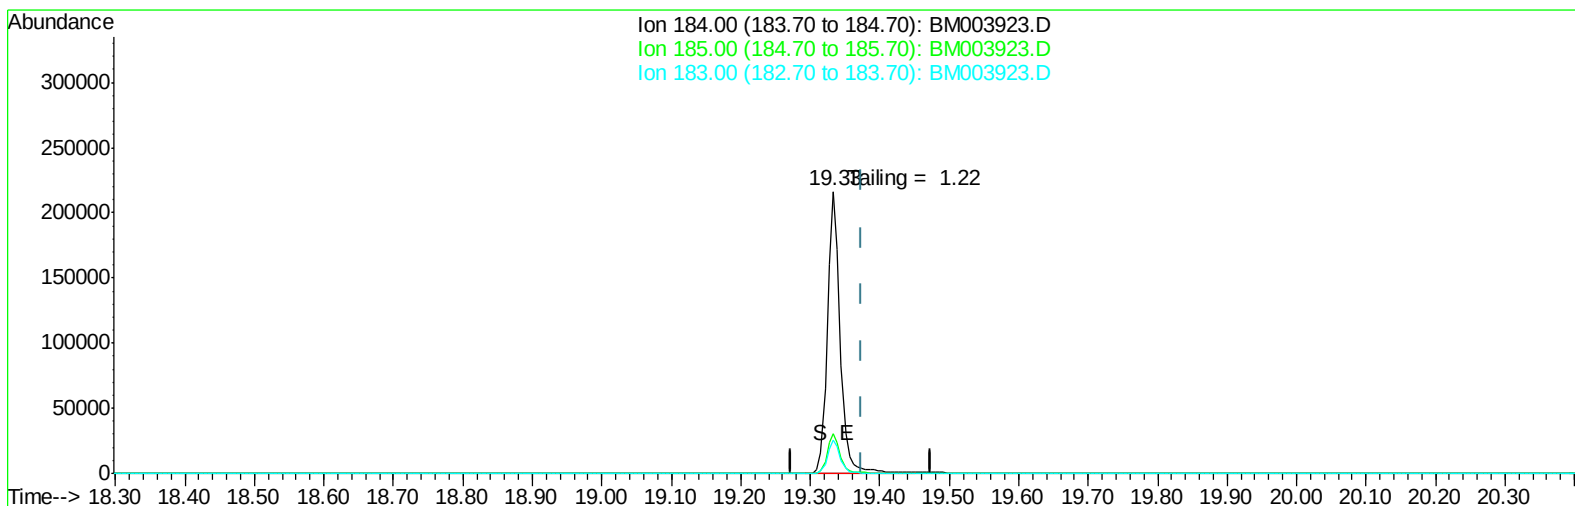

TIC: BM003923.D

(76) Benzidine

19.333min (-0.041) 3613.11ng

response 277568

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.05
183.00	11.10	11.64
0.00	0.00	0.00