


Data Path : Z:\HPCHEM1\BNA M\DATA\BM010816\  
 Data File : BM003923.D  
 Acq On : 08 Jan 2016 14:58  
 Operator : SJ/UM  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-SIM-BM010216.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jan 04 13:33:21 2016

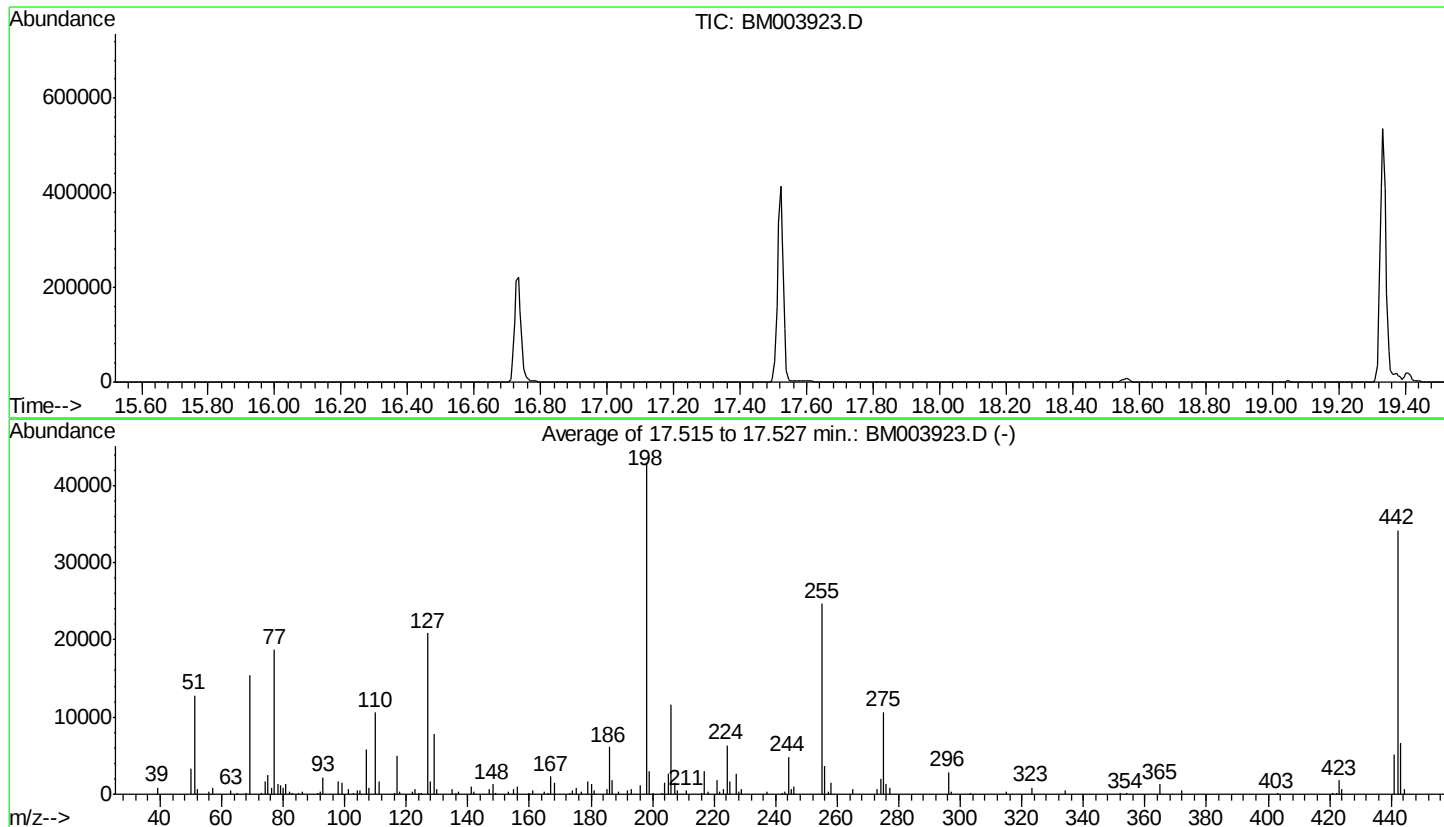

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 29.9      | 12821   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.3       | 205     | PASS             |
| 69          | 198          | 0.00         | 100          | 35.8      | 15387   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 48.5      | 20840   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 42928   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 2919    | PASS             |
| 275         | 198          | 10           | 60           | 24.9      | 10680   | PASS             |
| 365         | 198          | 1            | 100          | 3.0       | 1273    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.2      | 5201    | PASS             |
| 442         | 198          | 50           | 100          | 79.7      | 34202   | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 6702    | PASS             |