

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010915\
 Data File : BM000160.D
 Acq On : 09 Jan 2015 16:04
 Operator : TP/IZ
 Sample : MDL-05-S
 Misc : MDL-SOIL-0.15PPM-SIM
 ALS Vial : 38 Sample Multiplier: 1

Quant Time: Jan 09 22:11:26 2015

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM010715.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jan 08 10:41:47 2015

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	2870	0.40	ng/ul	0.00
2) Naphthalene-d8	10.62	136	9290	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.47	164	5734	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	10701	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	9450	0.40	ng/ul	-0.01
20) Perylene-d12	23.69	264	8748	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.21	152	3696	0.30	ng/ul	-0.01
14) Fluoranthene-d10	19.25	212	5960	0.26	ng/ul	0.00


Target Compounds

						Qvalue
3) Naphthalene	10.67	128	2253	0.09	ng/ul#	93
5) 2-Methylnaphthalene	12.28	142	1402	0.08	ng/ul	97
7) Acenaphthylene	14.20	152	2176	0.08	ng/ul#	93
8) Acenaphthene	14.52	153	1526	0.09	ng/ul#	85
9) Fluorene	15.52	166	1738	0.08	ng/ul#	97
11) Pentachlorophenol	16.89	266	220	0.13	ng/ul	96
12) Phenanthrene	17.26	178	2751	0.08	ng/ul	93
13) Anthracene	17.26	178	2751	0.09	ng/ul	93
15) Fluoranthene	19.27	202	3230	0.09	ng/ul	96
17) Pyrene	19.64	202	3303	0.08	ng/ul	97
18) Benzo(a)anthracene	21.39	228	2539	0.08	ng/ul	96
19) Chrysene	21.44	228	2901	0.09	ng/ul	97
21) Benzo(b)fluoranthene	23.00	252	2904	0.08	ng/ul	80
22) Benzo(k)fluoranthene	23.04	252	2641	0.08	ng/ul#	83
23) Benzo(a)pyrene	23.60	252	2526	0.08	ng/ul#	71
24) Indeno(1,2,3-cd)pyrene	26.03	276	2886	0.08	ng/ul	96
25) Dibenzo(a,h)anthracene	26.06	278	2254	0.08	ng/ul#	74
26) Benzo(g,h,i)perylene	26.73	276	2580	0.08	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010915\
Data File : BM000160.D
Acq On : 09 Jan 2015 16:04
Operator : TP/IZ
Sample : MDL-05-S
Misc : MDL-SOIL-0.15PPM-SIM
ALS Vial : 38 Sample Multiplier: 1

Quant Time: Jan 09 22:11:26 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM010715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 08 10:41:47 2015
Response via : Initial Calibration

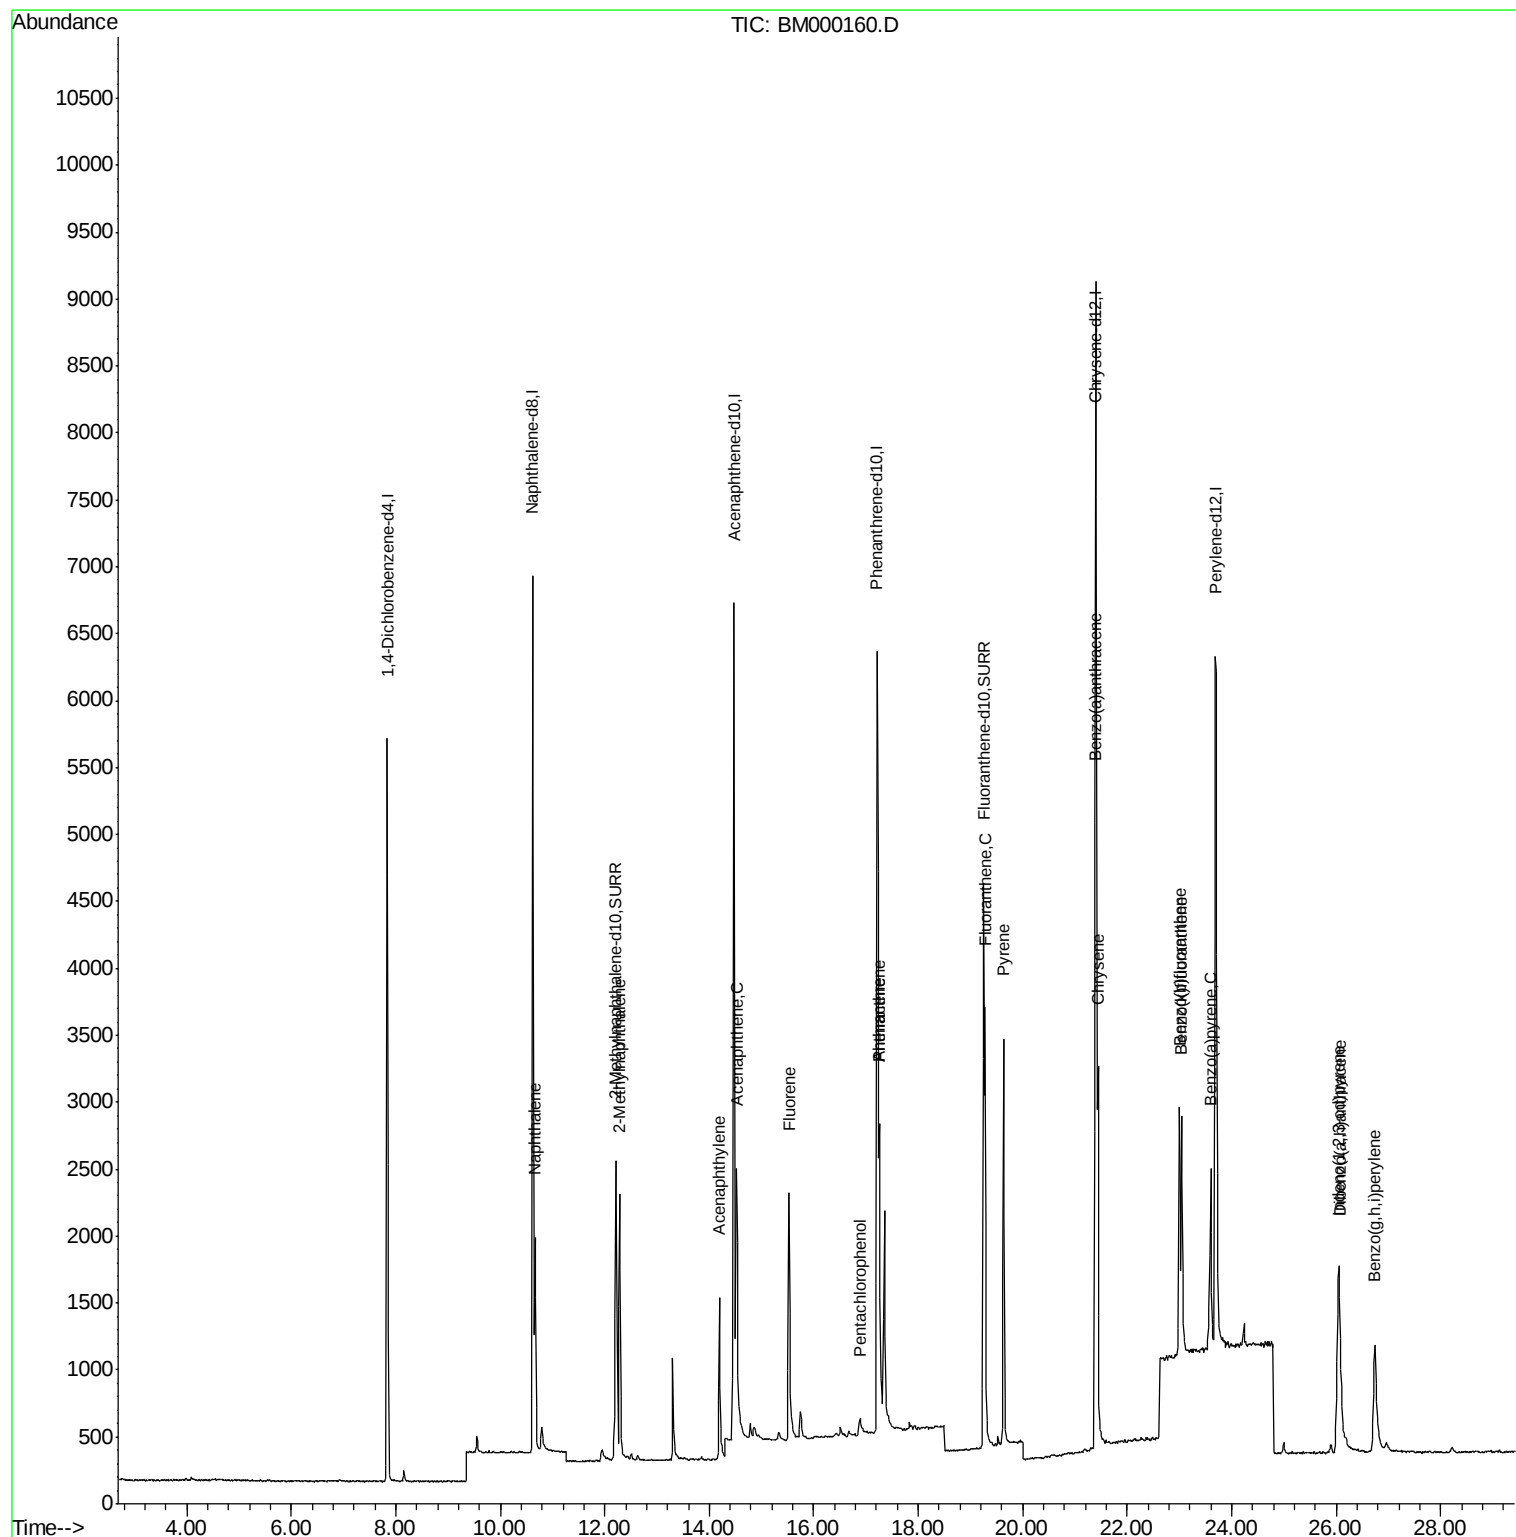



#3

Naphthalene

Concen: 0.09 ng/ul


RT: 10.67 min Scan# 1352

Delta R.T. -0.01 min




Lab File: BM000160.D

Acq: 09 Jan 2015 16:04

Tgt Ion:	128	Resp:	2253
Ion	Ratio	Lower	Upper
128	100		
129	13.6	9.5	14.3
127	16.5	10.4	15.6

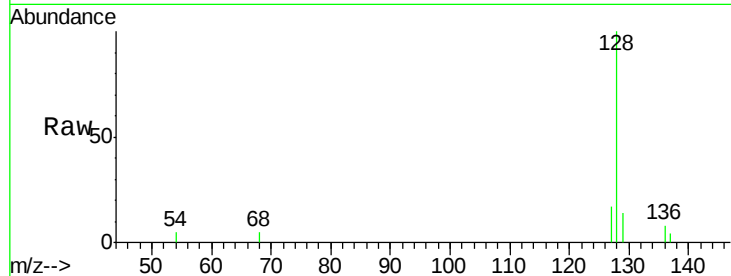

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

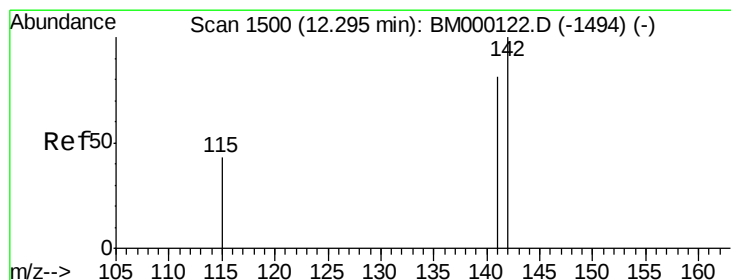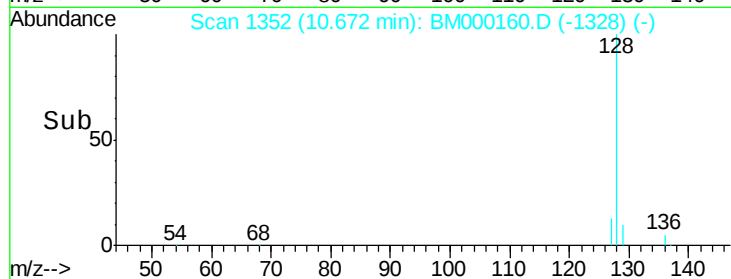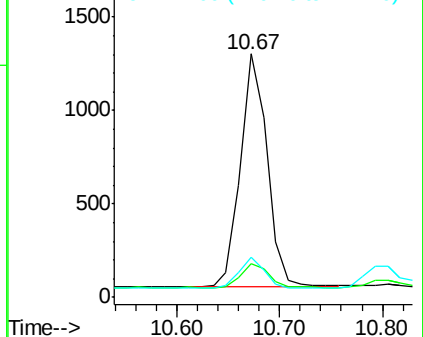

#5

2-Methylnaphthalene

Concen: 0.08 ng/ul


RT: 12.28 min Scan# 1499

Delta R.T. -0.01 min



Lab File: BM000160.D


Acq: 09 Jan 2015 16:04

Tgt Ion:	142	Resp:	1402
Ion	Ratio	Lower	Upper
142	100		
141	88.7	68.9	103.3



Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E

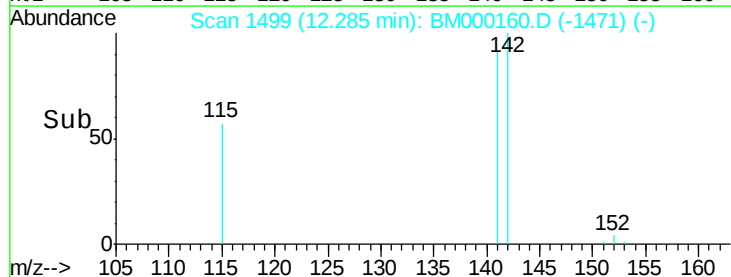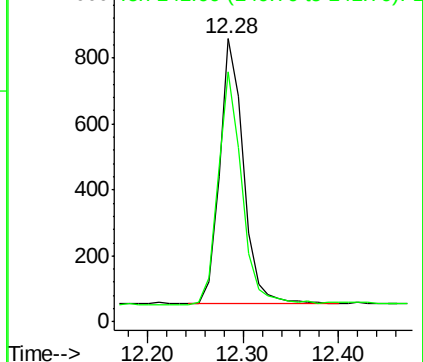

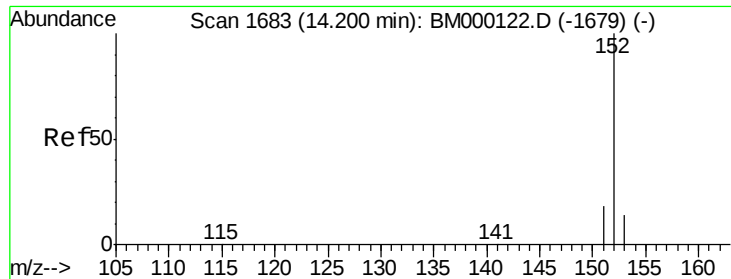

#7

Acenaphthylene

Concen: 0.08 ng/ul

RT: 14.20 min Scan# 1683

Delta R.T. 0.00 min

Lab File: BM000160.D

Acq: 09 Jan 2015 16:04


Tgt Ion:152 Resp: 2176

Ion Ratio Lower Upper

152 100

151 21.6 15.4 23.2




153 17.5 11.0 16.4#

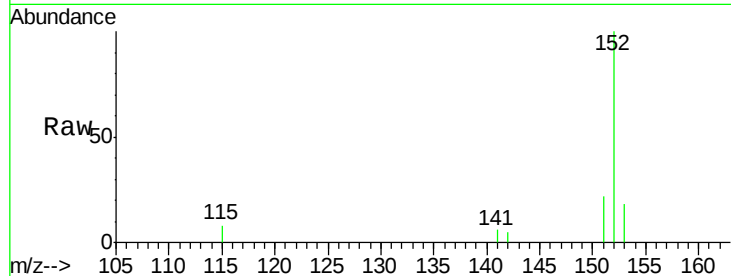

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

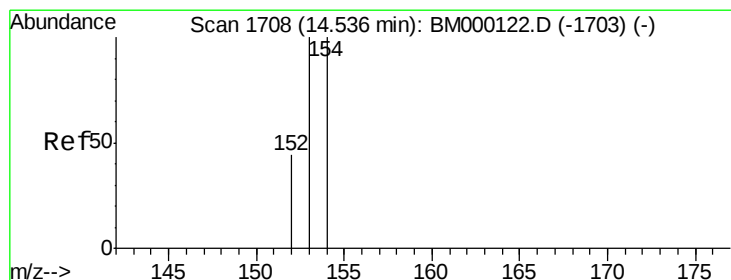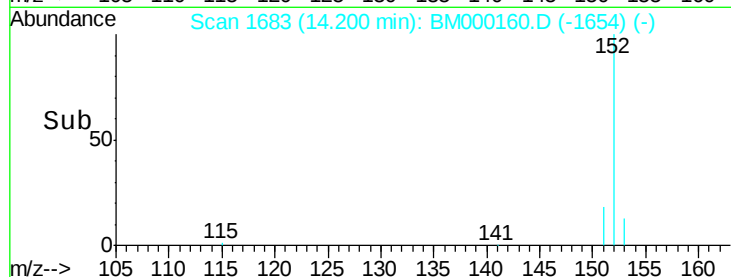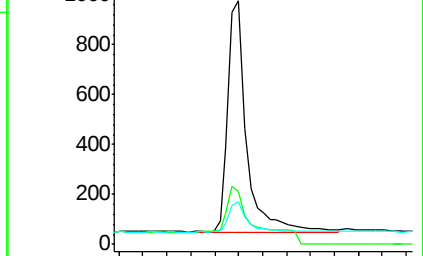

#8

Acenaphthene

Concen: 0.09 ng/ul

RT: 14.52 min Scan# 1707

Delta R.T. -0.02 min

Lab File: BM000160.D

Acq: 09 Jan 2015 16:04


Tgt Ion:153 Resp: 1526

Ion Ratio Lower Upper

153 100

152 56.6 35.8 53.6#



154 86.6 79.9 119.9



Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E





Ion 154.00 (153.70 to 154.70): E

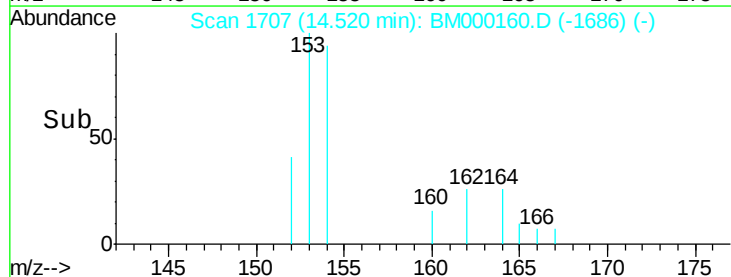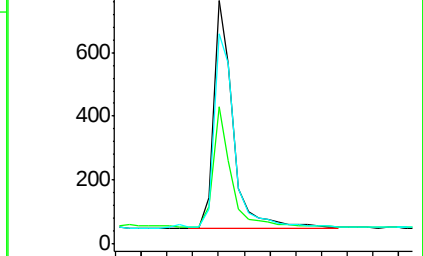






#9
Fluorene
 Concen: 0.08 ng/ul
 RT: 15.52 min Scan# 1772
 Delta R.T. 0.00 min
 Lab File: BM000160.D
 Acq: 09 Jan 2015 16:04


Tgt Ion:166 Resp: 1738
 Ion Ratio Lower Upper
 166 100
 165 97.6 77.0 115.4
 167 18.1 11.0 16.6#

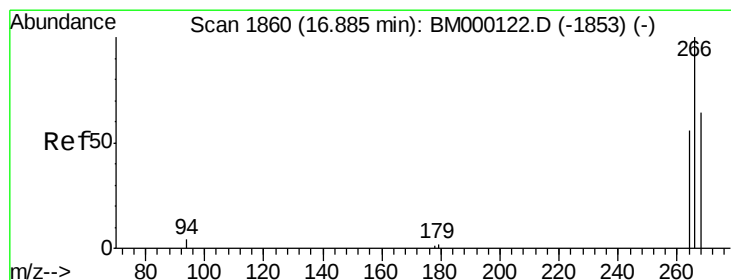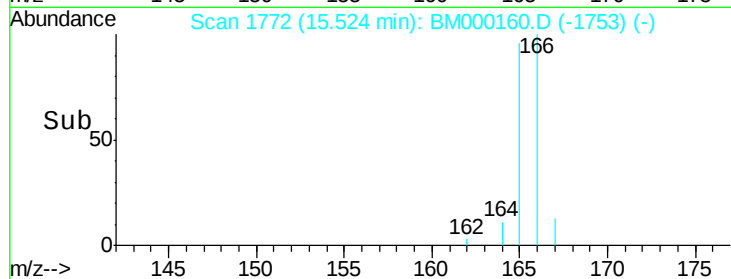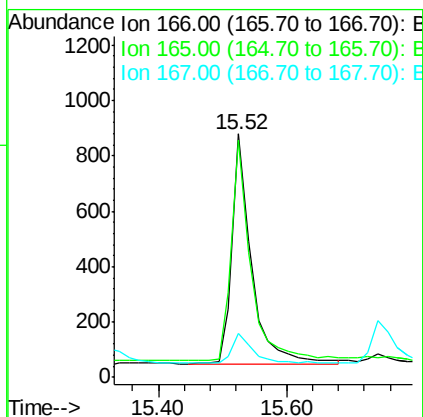

#11
Pentachlorophenol
 Concen: 0.13 ng/ul
 RT: 16.89 min Scan# 1860
 Delta R.T. 0.00 min
 Lab File: BM000160.D
 Acq: 09 Jan 2015 16:04

Tgt Ion:266 Resp: 220
 Ion Ratio Lower Upper
 266 100
 264 67.7 53.9 80.9
 268 67.3 49.2 73.8

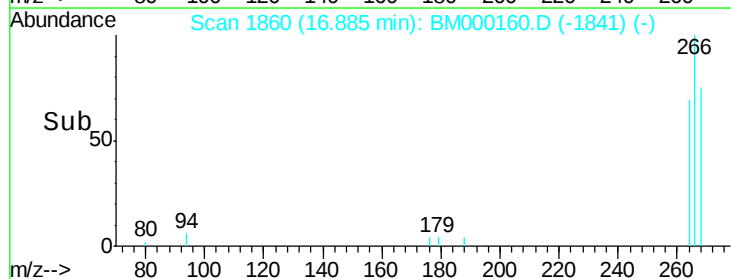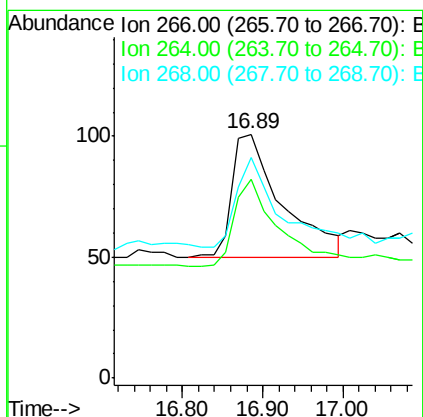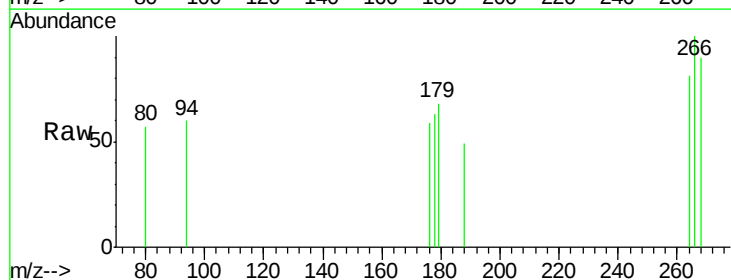

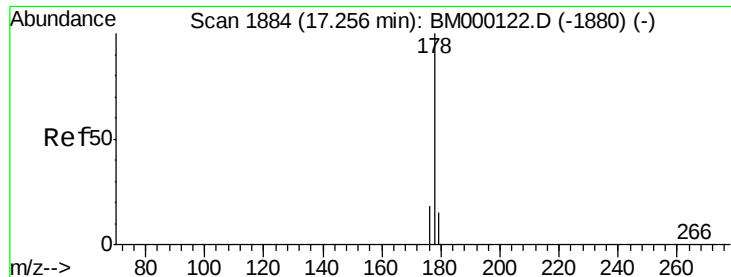

#12

Phenanthrene

Concen: 0.08 ng/ul

RT: 17.26 min Scan# 1884

Delta R.T. 0.00 min

Lab File: BM000160.D

Acq: 09 Jan 2015 16:04


Tgt Ion:178 Resp: 2751

Ion Ratio Lower Upper

178 100

176 21.7 15.1 22.7




179 19.3 13.0 19.4

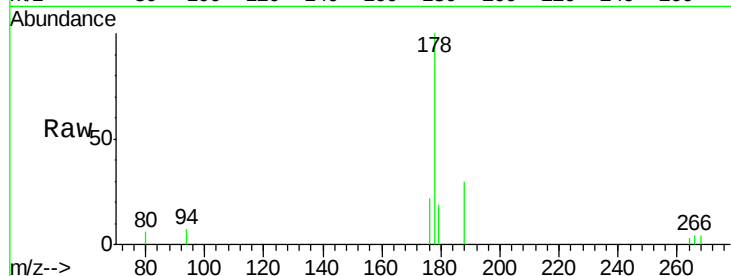

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

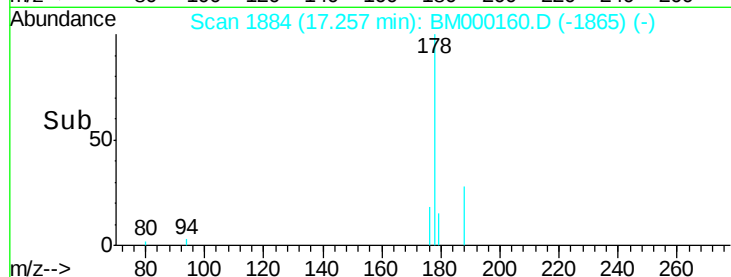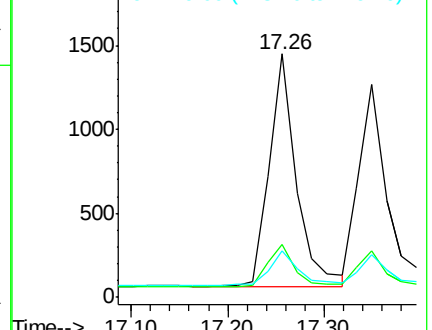

#13

Anthracene

Concen: 0.09 ng/ul

RT: 17.26 min Scan# 1884

Delta R.T. -0.09 min

Lab File: BM000160.D

Acq: 09 Jan 2015 16:04


Tgt Ion:178 Resp: 2751

Ion Ratio Lower Upper

178 100

176 21.7 14.6 21.8



179 19.3 13.1 19.7




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E





Ion 179.00 (178.70 to 179.70): E

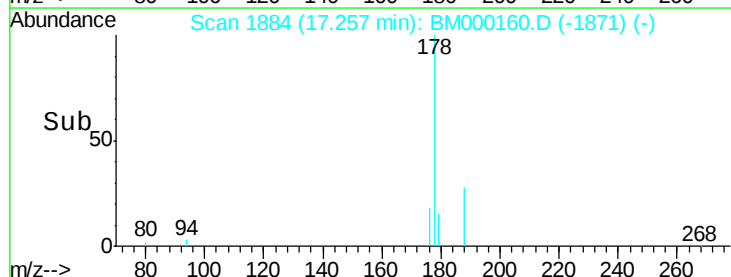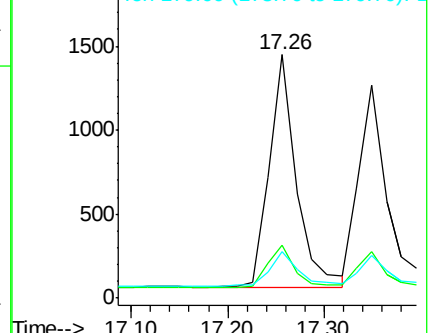

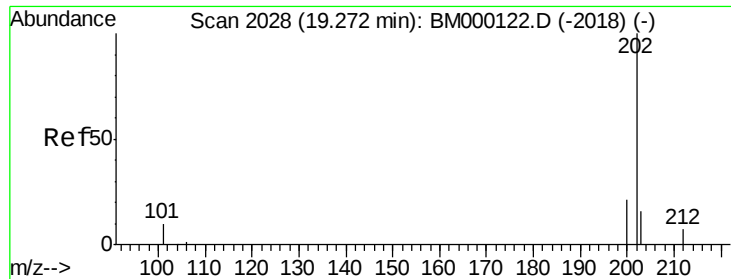




#15
 Fluoranthene
 Concen: 0.09 ng/u1
 RT: 19.27 min Scan# 2028
 Delta R.T. 0.00 min
 Lab File: BM000160.D
 Acq: 09 Jan 2015 16:04


Tgt Ion:202 Resp: 3230
 Ion Ratio Lower Upper
 202 100
 101 9.9 0.0 30.5
 203 18.8 0.0 36.6

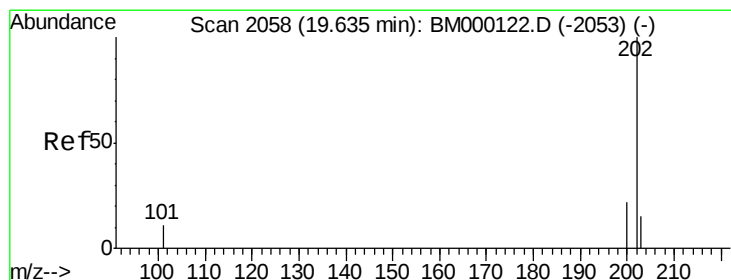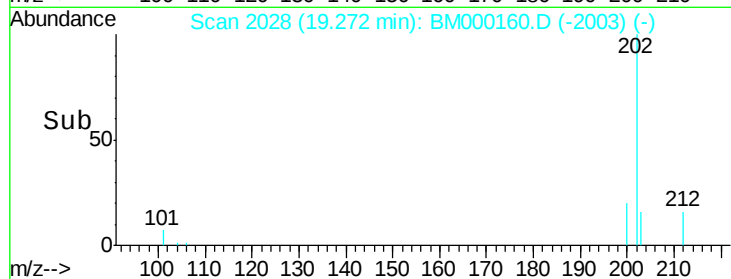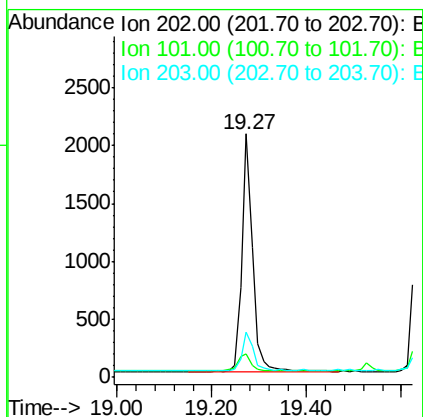

#17
 Pyrene
 Concen: 0.08 ng/u1
 RT: 19.64 min Scan# 2058
 Delta R.T. 0.00 min
 Lab File: BM000160.D
 Acq: 09 Jan 2015 16:04


Tgt Ion:202 Resp: 3303
 Ion Ratio Lower Upper
 202 100
 200 22.3 17.9 26.9
 203 19.1 12.8 19.2

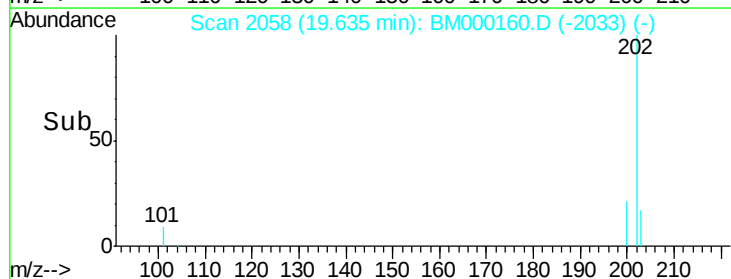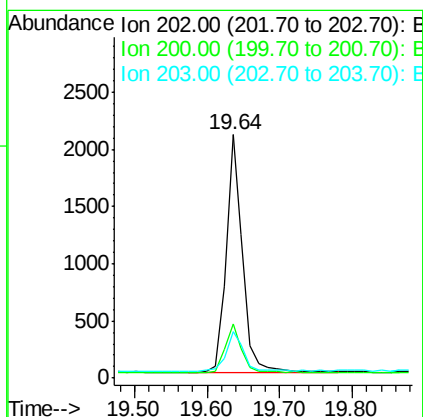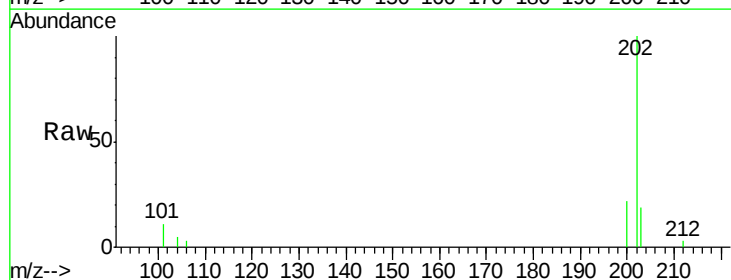



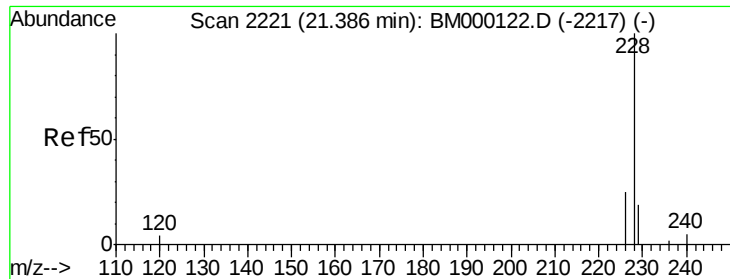


#18
Benzo(a)anthracene
Concen: 0.08 ng/ul
RT: 21.39 min Scan# 2221
Delta R.T. 0.00 min
Lab File: BM000160.D
Acq: 09 Jan 2015 16:04

Tgt Ion:228 Resp: 2539
Ion Ratio Lower Upper
228 100
226 25.6 20.8 31.2
229 23.3 15.5 23.3

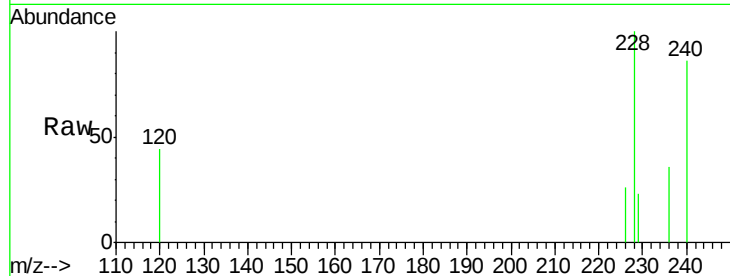


Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

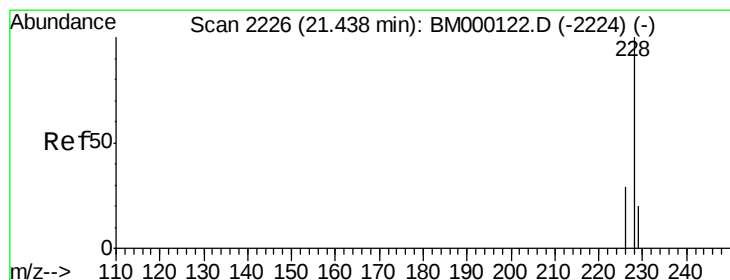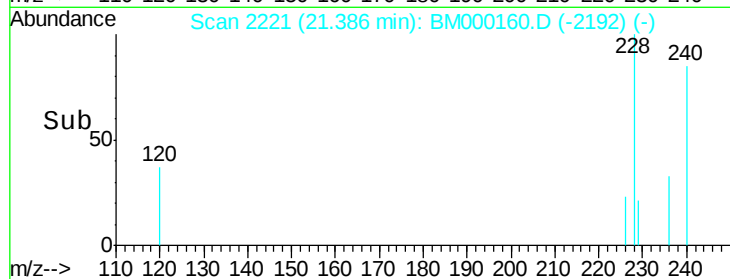
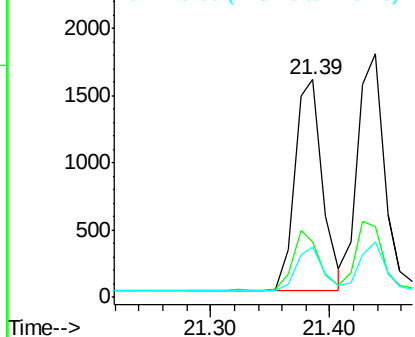


#19
Chrysene
Concen: 0.09 ng/ul
RT: 21.44 min Scan# 2226
Delta R.T. 0.00 min
Lab File: BM000160.D
Acq: 09 Jan 2015 16:04

Tgt Ion:228 Resp: 2901
Ion Ratio Lower Upper
228 100
226 28.9 23.8 35.6
229 22.6 15.8 23.8

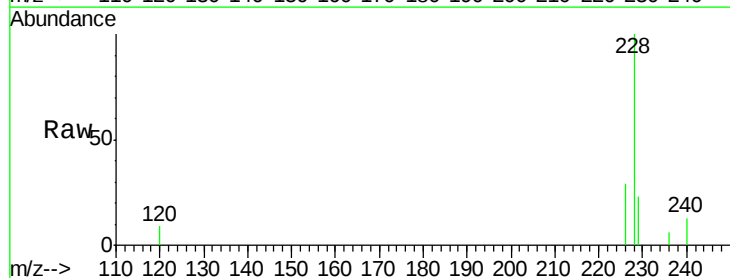

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

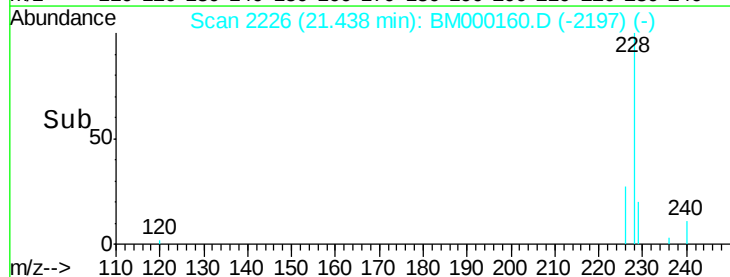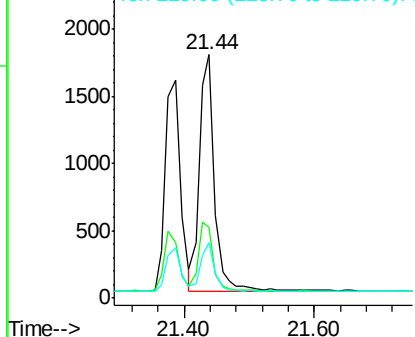



#21

Benzo(b)fluoranthene

Concen: 0.08 ng/ul

RT: 23.00 min Scan# 2376

Delta R.T. 0.00 min

Lab File: BM000160.D

Acq: 09 Jan 2015 16:04


Tgt Ion:252 Resp: 2904

Ion Ratio Lower Upper




252 100

253 36.6 0.0 48.2

125 13.6 0.0 21.6

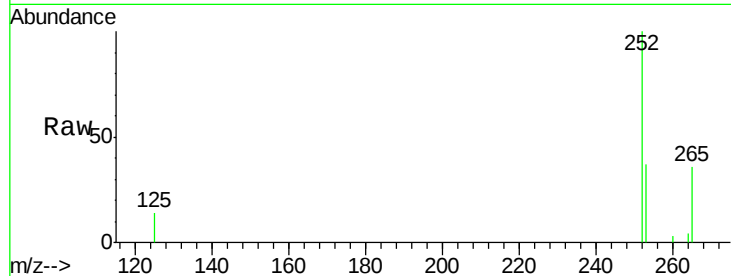

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

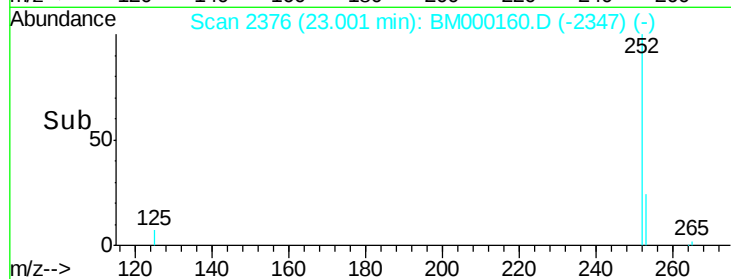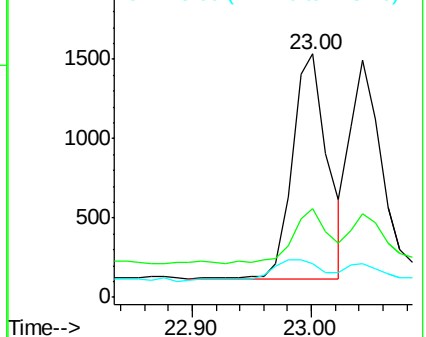

#22

Benzo(k)fluoranthene

Concen: 0.08 ng/ul

RT: 23.04 min Scan# 2380

Delta R.T. -0.01 min

Lab File: BM000160.D

Acq: 09 Jan 2015 16:04


Tgt Ion:252 Resp: 2641

Ion Ratio Lower Upper



252 100


253 35.0 20.5 30.7#

125 14.3 7.8 11.8#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

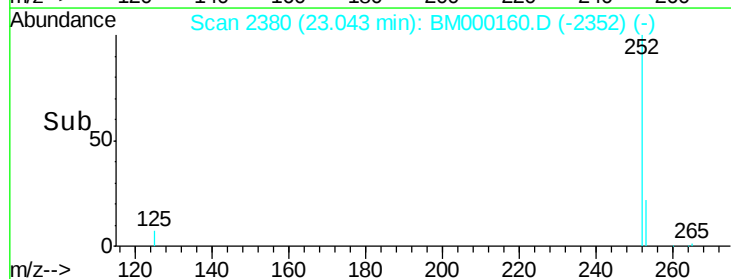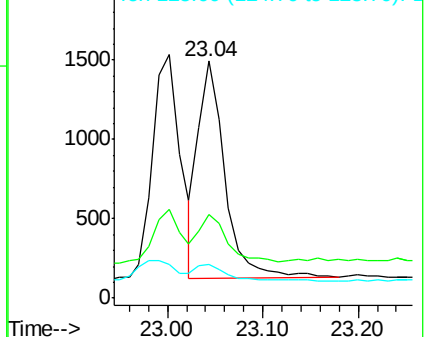

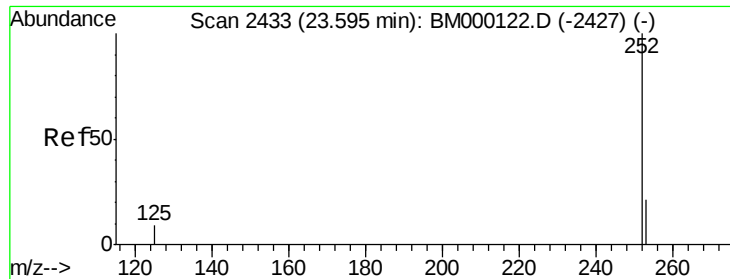

#23

Benzo(a)pyrene

Concen: 0.08 ng/ul

RT: 23.60 min Scan# 2433

Delta R.T. 0.00 min

Lab File: BM000160.D

Acq: 09 Jan 2015 16:04


Tgt Ion: 252 Resp: 2526

Ion Ratio Lower Upper




252 100

253 42.2 19.8 29.6#

125 17.4 9.2 13.8#

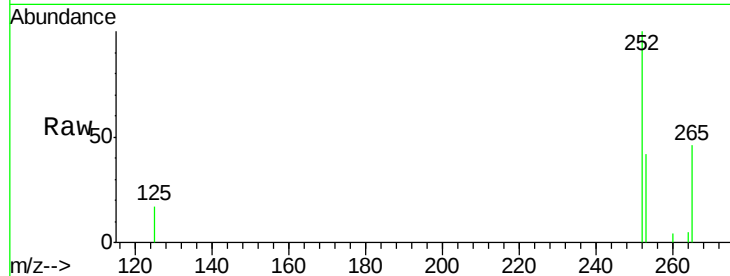

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

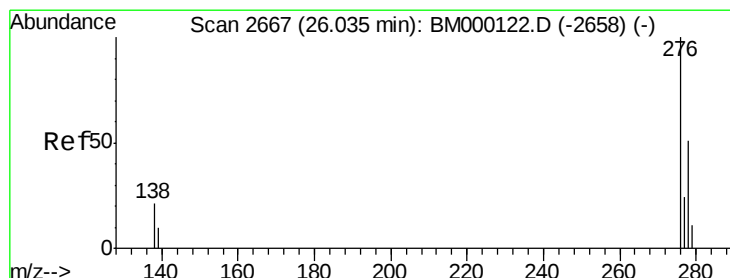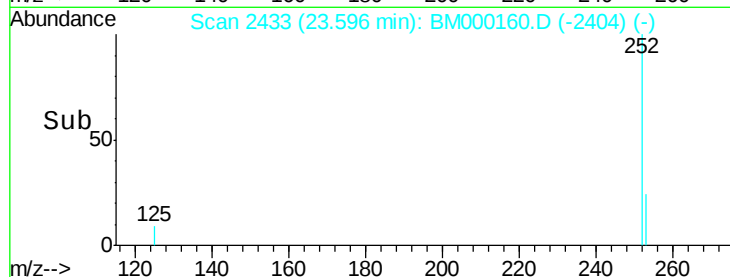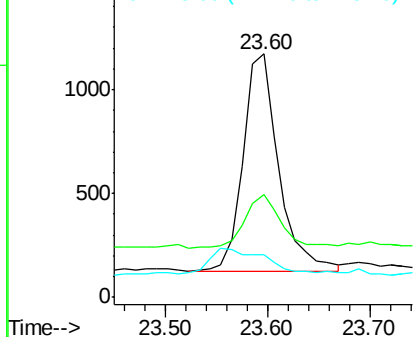

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.08 ng/ul

RT: 26.03 min Scan# 2667

Delta R.T. 0.00 min

Lab File: BM000160.D

Acq: 09 Jan 2015 16:04


Tgt Ion: 276 Resp: 2886

Ion Ratio Lower Upper



276 100


138 18.6 17.6 26.4

277 25.4 19.9 29.9

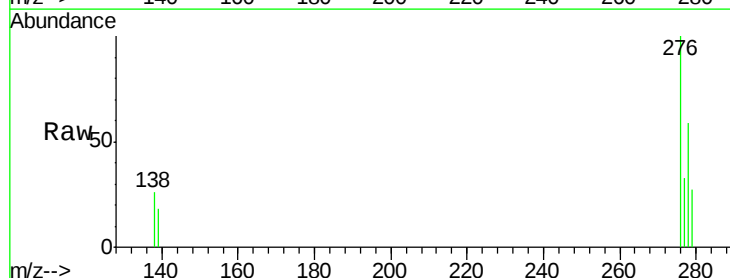

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

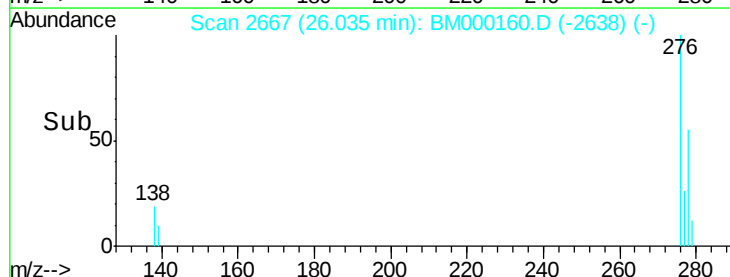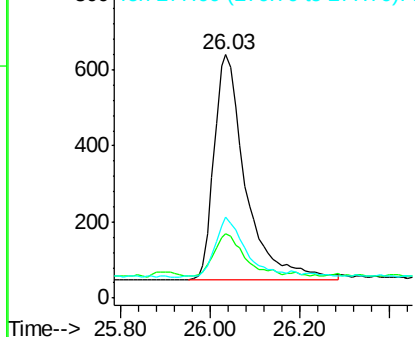

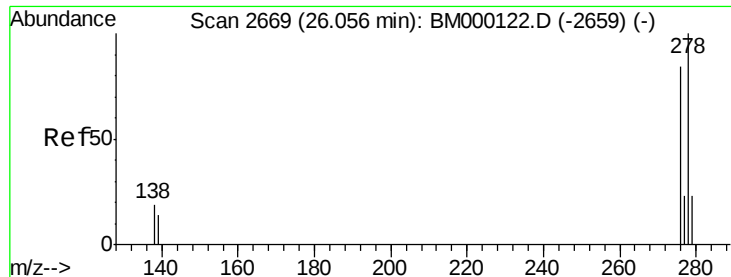

#25

Dibenzo(a,h)anthracene

Concen: 0.08 ng/ul

RT: 26.06 min Scan# 2669

Delta R.T. 0.00 min

Lab File: BM000160.D

Acq: 09 Jan 2015 16:04


Tgt Ion: 278 Resp: 2254

Ion Ratio Lower Upper

278 100

139 22.3 12.6 18.8#




279 42.3 20.6 30.8#



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

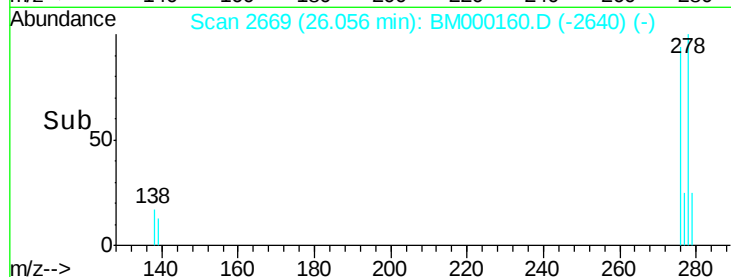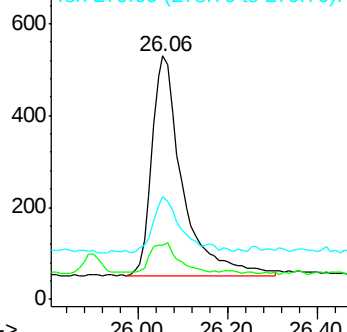

#26

Benzo(g,h,i)perylene

Concen: 0.08 ng/ul

RT: 26.73 min Scan# 2734

Delta R.T. -0.01 min

Lab File: BM000160.D

Acq: 09 Jan 2015 16:04


Tgt Ion: 276 Resp: 2580

Ion Ratio Lower Upper

276 100

277 30.8 20.0 30.0#

138 23.5 15.7 23.5



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

