


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM010915\
 Data File : BM000154.D
 Acq On : 09 Jan 2015 11:23
 Operator : TP/IZ
 Sample : DFTPP06
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM010715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 12 11:40:45 2015

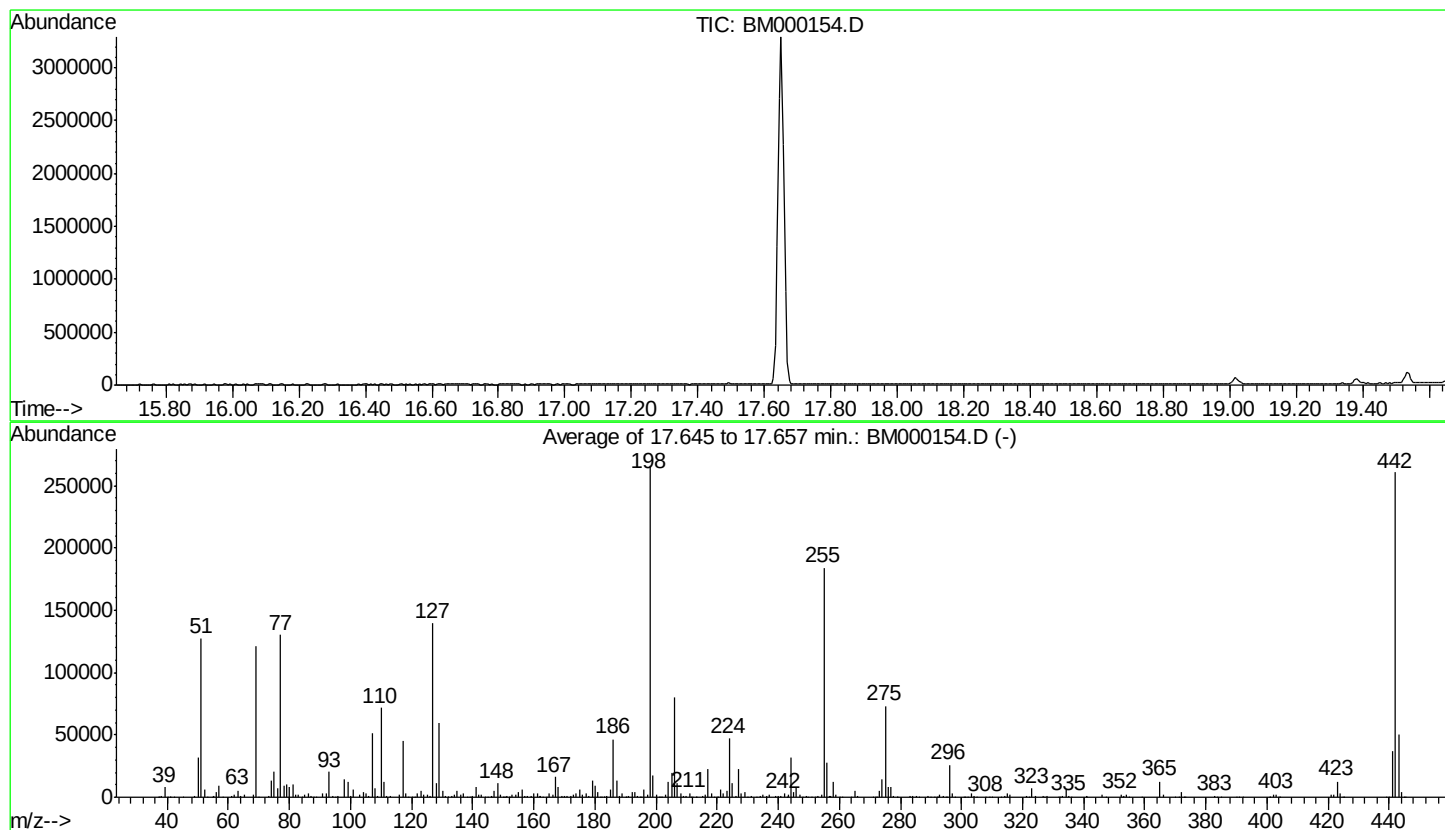

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.8	127274	PASS
68	69	0.00	2	1.7	2043	PASS
69	198	0.00	100	45.7	121637	PASS
70	69	0.00	2	0.4	477	PASS
127	198	10	80	52.3	139298	PASS
197	198	0.00	2	0.8	2041	PASS
198	198	100	100	100.0	266176	PASS
199	198	5	9	6.7	17710	PASS
275	198	10	60	27.5	73290	PASS
365	198	1	100	4.7	12482	PASS
441	443	0.01	100	74.3	37333	PASS
442	198	50	100	98.0	260970	PASS
443	442	15	24	19.3	50242	PASS