

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011017\
 Data File : BM008747.D
 Acq On : 09 Jan 2017 20:24
 Operator : UM/SJ
 Sample : I1061-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA963

Quant Time: Jan 10 01:06:10 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 10 00:37:03 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.96	152	97229	20.00	ng/ul	0.00
18) Naphthalene-d8	10.76	136	408831	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.59	164	298189	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.33	188	677806	20.00	ng/ul	0.00
75) Chrysene-d12	21.49	240	860811	20.00	ng/ul	0.00
83) Perylene-d12	23.86	264	869928	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	3171	1.51	ng/uL	0.00
5) Phenol-d5	7.10	99	64067	8.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.29	67	184472	34.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.49	132	158721	28.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.65	113	107837	17.41	ng/ul	0.00
19) Nitrobenzene-d5	9.12	128	90810	36.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.84	143	97979	35.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.37	165	194291	30.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.89	131	14112	2.02	ng/ul	0.00
43) Dimethylphthalate-d6	13.99	166	719891	36.59	ng/ul	0.00
46) Acenaphthylene-d8	14.28	160	840342	36.22	ng/ul	0.00
51) 4-Nitrophenol-d4	14.76	143	23210	7.21	ng/ul	0.00
57) Fluorene-d10	15.57	176	633735	34.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.69	200	121091	34.66	ng/ul	0.00
70) Anthracene-d10	17.43	188	1094816	37.49	ng/ul	0.00
76) Pyrene-d10	19.71	212	1316015	34.70	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.70	264	1311499	36.96	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.04	163	20918	1.06	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011017\
Data File : BM008747.D
Acq On : 09 Jan 2017 20:24
Operator : UM/SJ
Sample : I1061-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA963

Quant Time: Jan 10 01:06:10 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010617.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 10 00:37:03 2017
Response via : Initial Calibration

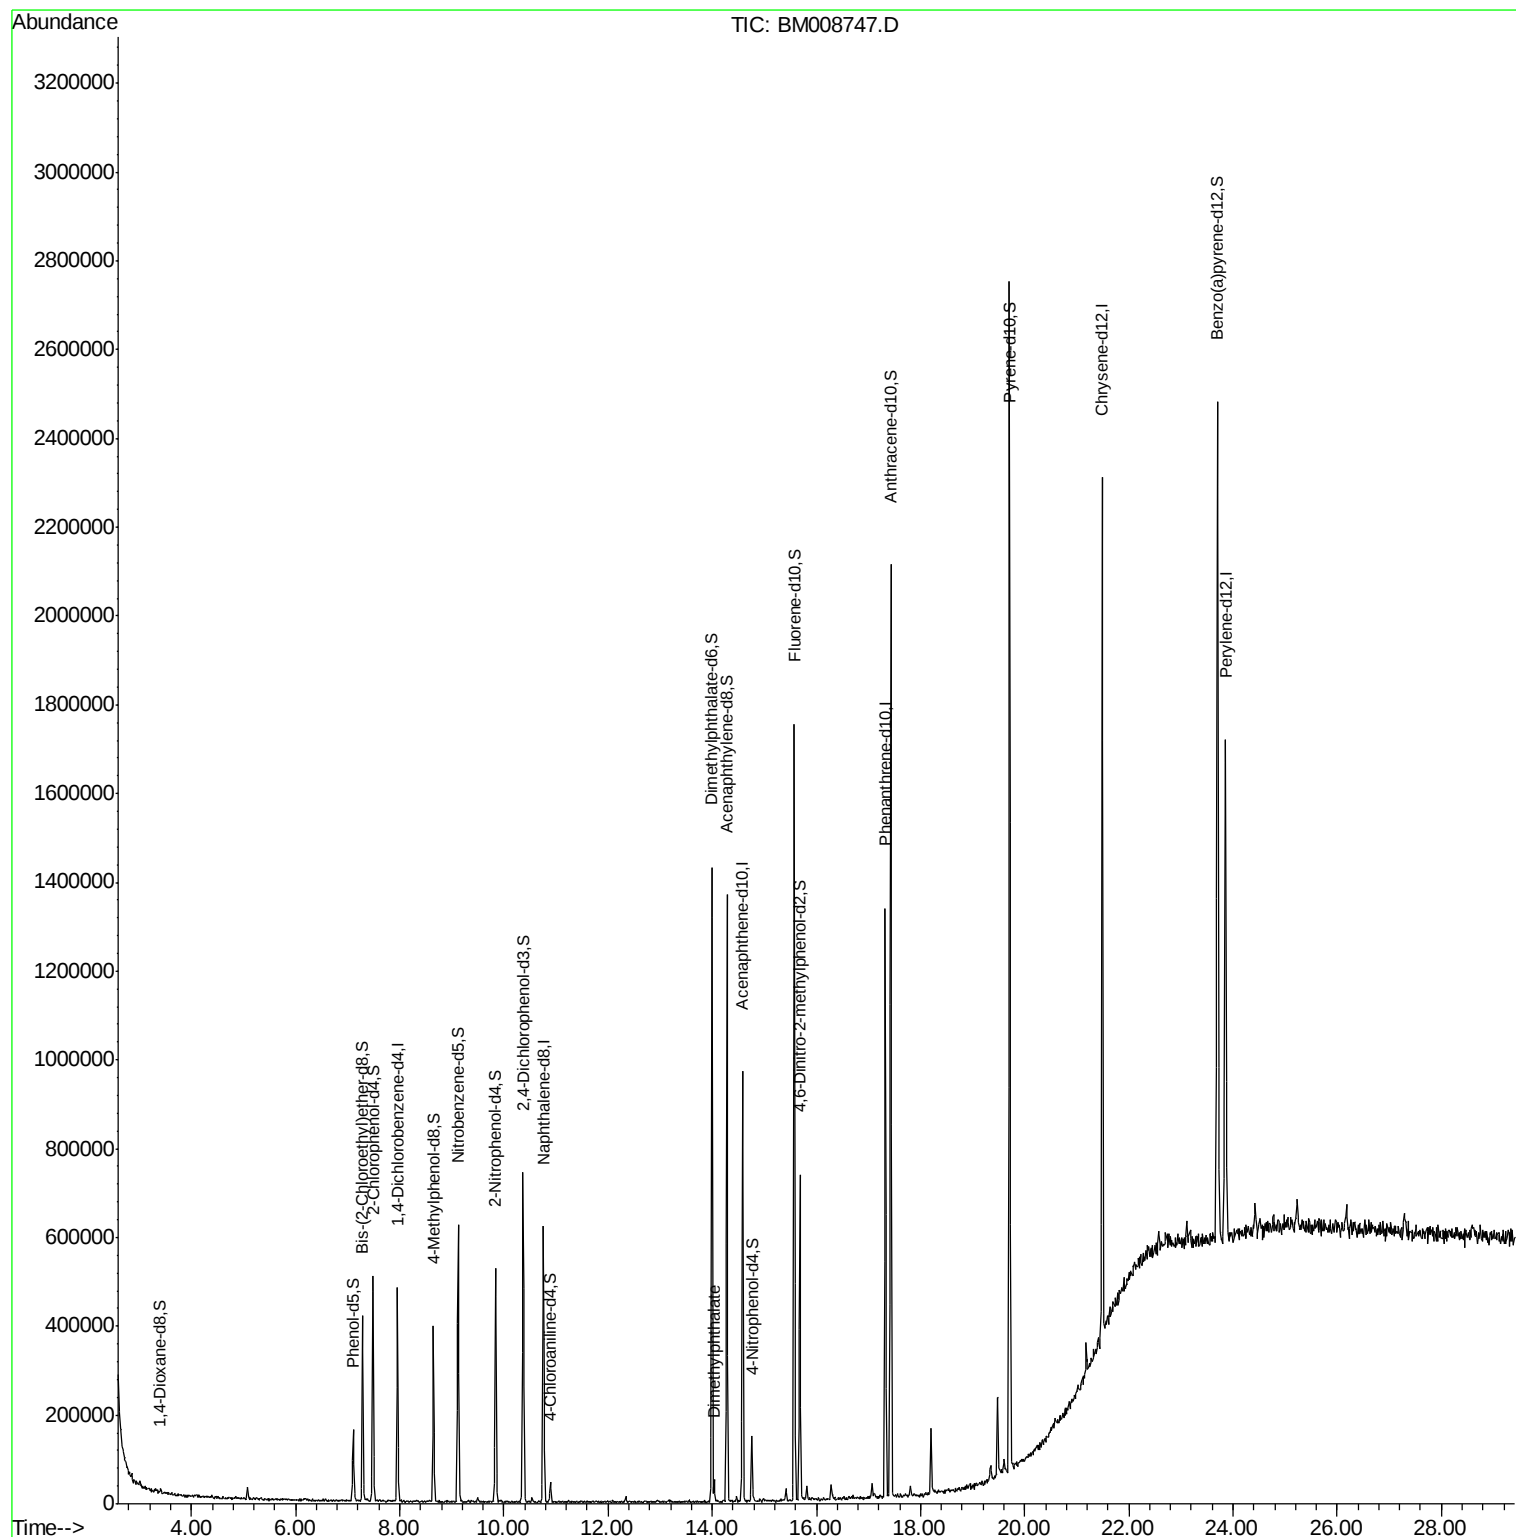

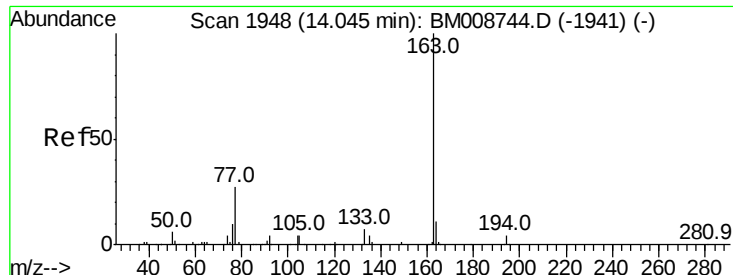

#44

Dimethylphthalate

Concen: 1.06 ng/ul

RT: 14.04 min Scan# 1947

Delta R.T. -0.01 min

Lab File: BM008747.D

Acq: 09 Jan 2017 20:24

Instrument :

BNA_M

ClientSampleId :

DA963


Tot Ion:163 Resp: 20918

Ion Ratio Lower Upper

163 100

194 6.5 3.4 5.0#

164 7.1 8.2 12.4#

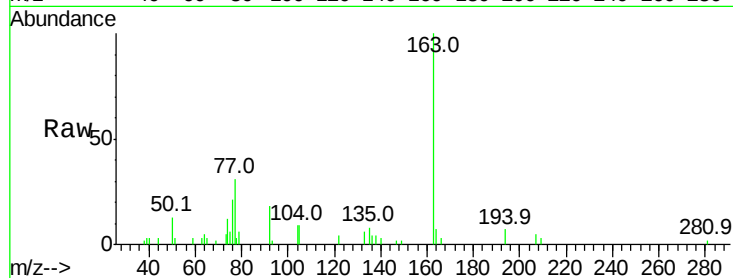

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

