
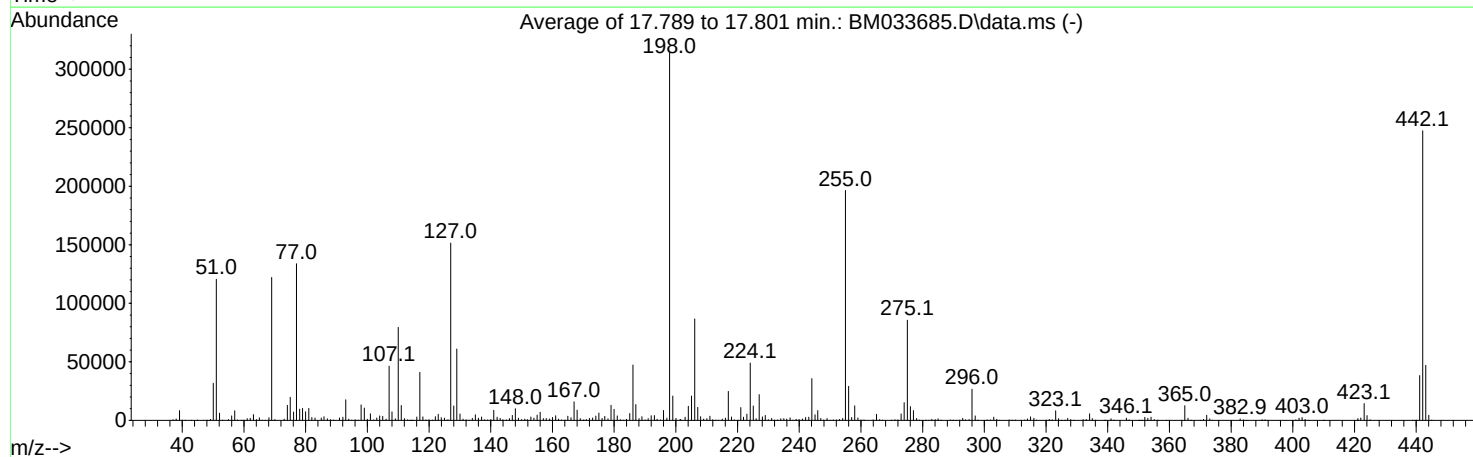


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011022\
 Data File : BM033685.D
 Acq On : 10 Jan 2022 14:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 05 17:07:26 2022

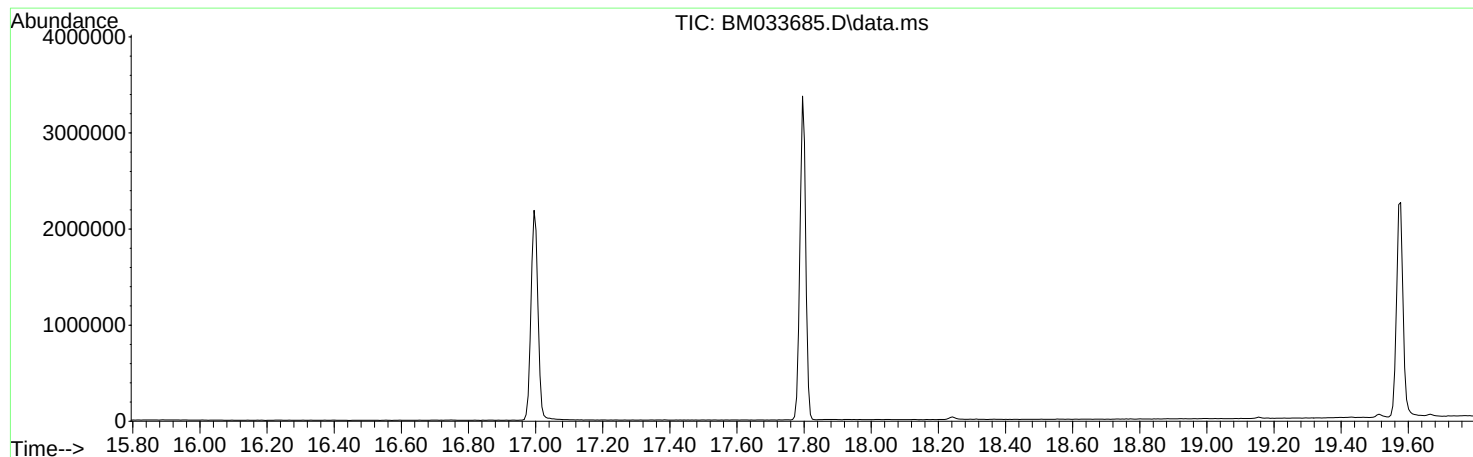

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	120513	PASS
68	69	0.00	2	1.9	2354	PASS
69	198	0.00	100	38.9	122139	PASS
70	69	0.00	2	0.6	694	PASS
127	198	10	80	48.2	151509	PASS
197	198	0.00	2	0.6	1928	PASS
198	198	100	100	100.0	314283	PASS
199	198	5	9	6.6	20795	PASS
275	198	10	60	27.2	85531	PASS
365	198	1	100	4.0	12628	PASS
441	198	0.01	100	12.2	38248	PASS
442	442	50	100	100.0	247360	PASS
443	442	15	24	19.0	47091	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/10/2022	BNA_M	<u>BM033685.D</u>
Compound Name	Response	Retention Time
DDT	808911	20.813
DDD	24067	20.371
DDE	792	19.871
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24859	833770	2.98

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011022\
 Data File : BM033685.D
 Acq On : 10 Jan 2022 14:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 11 03:03:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 05 17:07:26 2022
 Response via : Initial Calibration

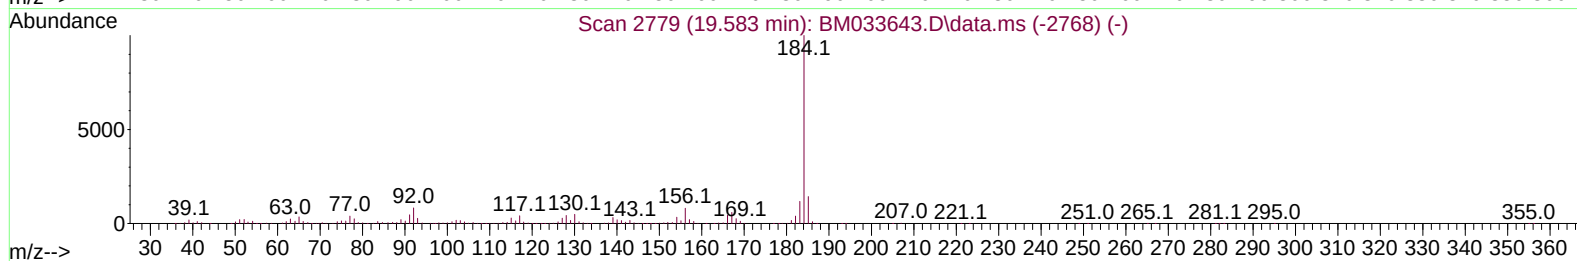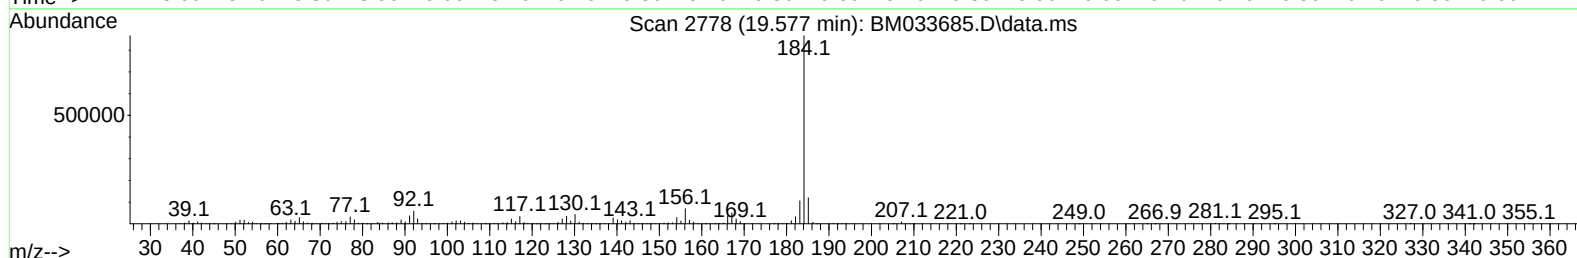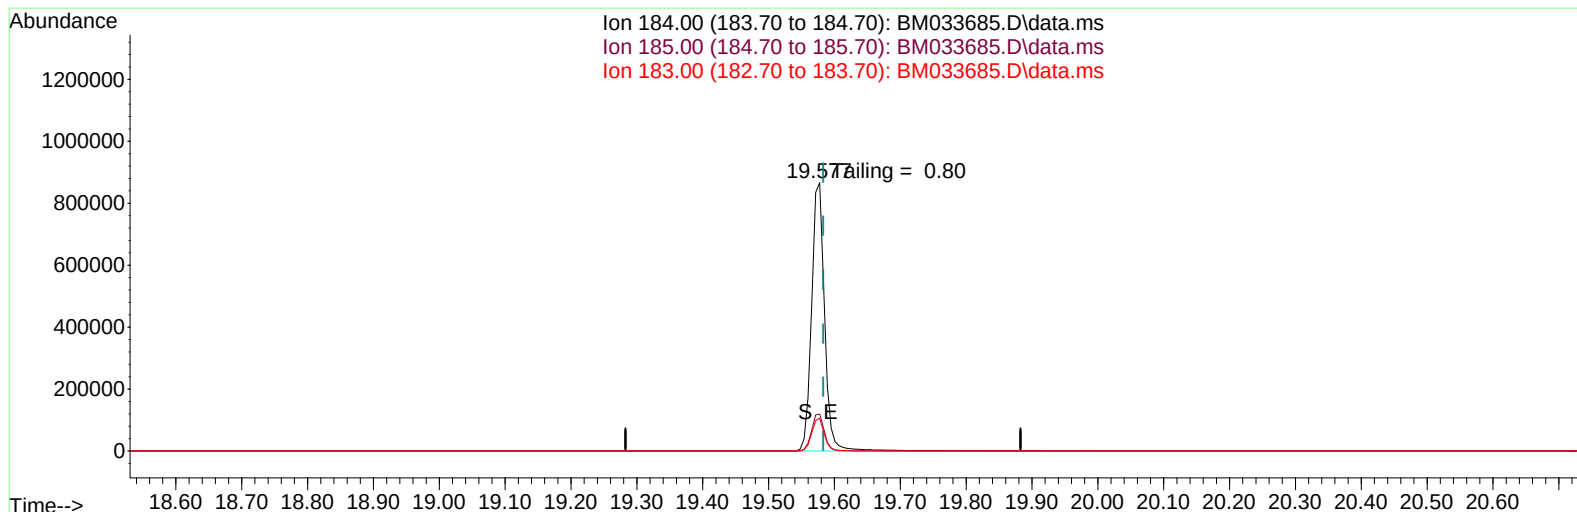

TIC: BM033685.D\data.ms

(77) Benzidine

19.577min (-0.006) 40159.95 ng




response 1184827

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.77
183.00	12.10	12.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011022\
Data File : BM033685.D
Acq On : 10 Jan 2022 14:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 11 03:03:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 17:07:26 2022
Response via : Initial Calibration

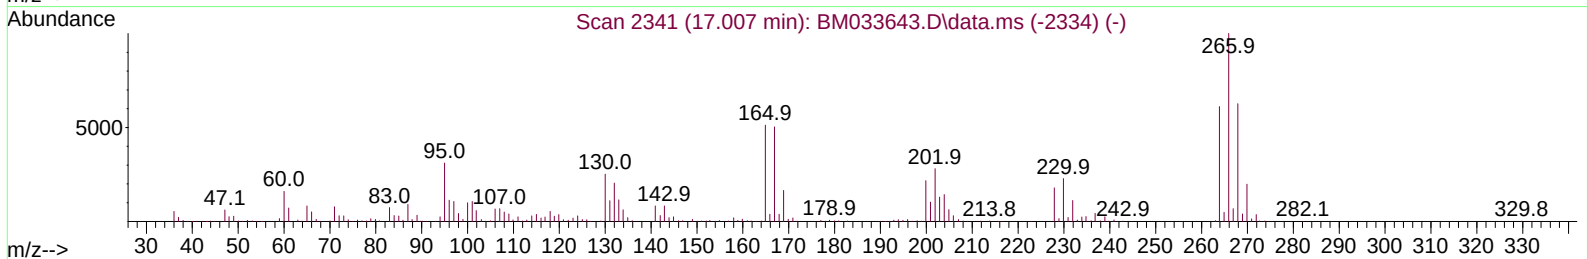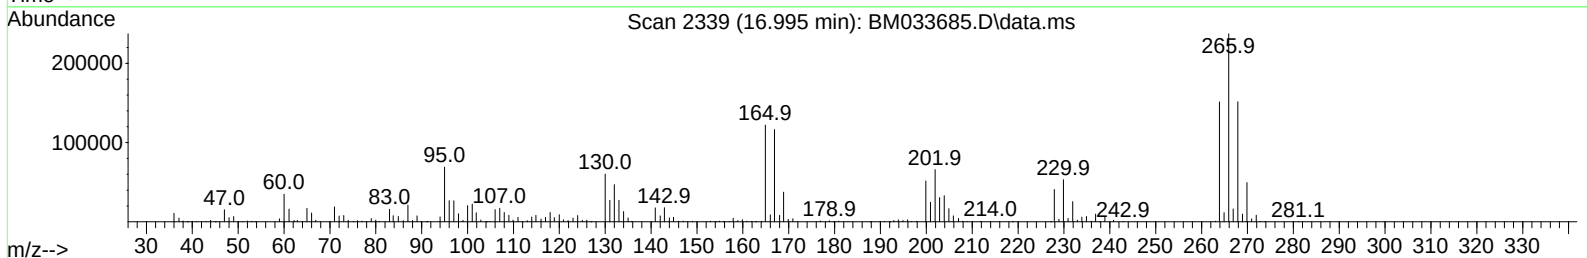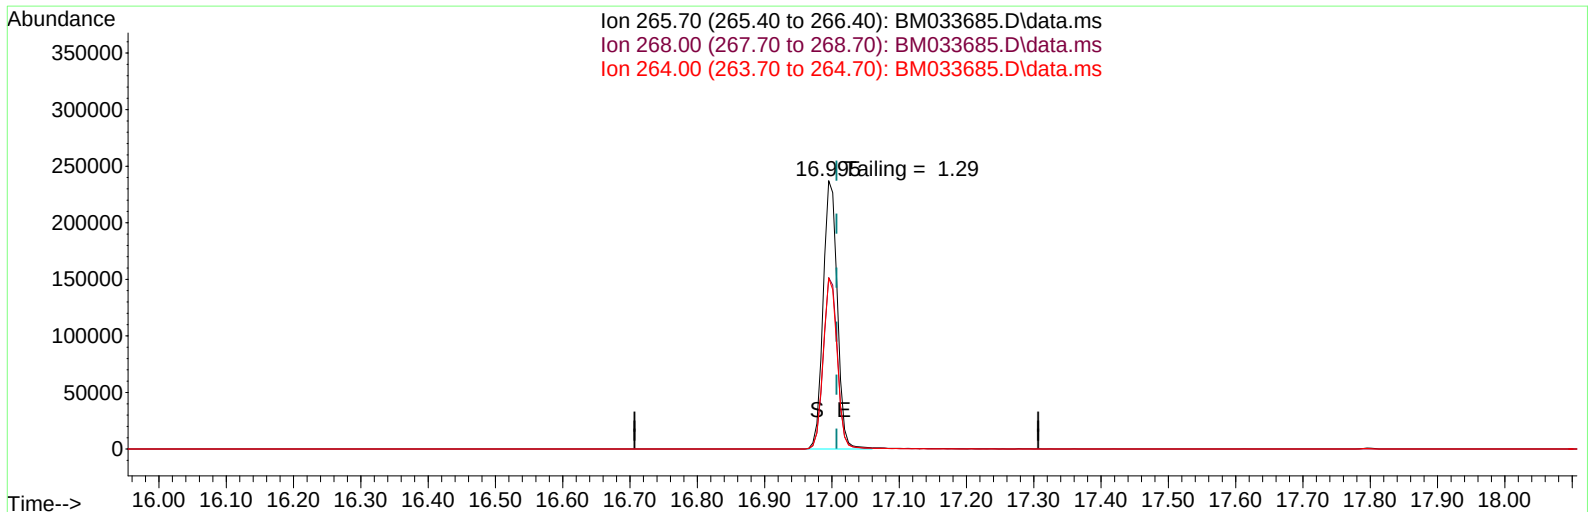

TIC: BM033685.D\data.ms

(70) Pentachlorophenol (C)

16.995min (-0.011) 0.00 ng

response 349684

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.88
264.00	61.40	63.74
0.00	0.00	0.00