

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011023\
 Data File : BM038417.D
 Acq On : 10 Jan 2023 09:55
 Operator : CG/JU
 Sample : PB150090BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	26	30	38	rVB	31315	40350	2.28%	0.223%
2	3.793	99	103	125	rBV	346870	545873	30.88%	3.014%
3	4.116	156	158	163	rVB2	6389	8776	0.50%	0.048%
4	6.592	577	579	582	rBV3	1961	2042	0.12%	0.011%
5	7.151	668	674	686	rBV	399076	621812	35.18%	3.433%
6	7.322	697	703	716	rBV	319123	481428	27.24%	2.658%
7	7.522	730	737	752	rVB	391241	608102	34.41%	3.358%
8	7.992	811	817	828	rVB	299950	465466	26.34%	2.570%
9	8.704	932	938	952	rVB	417132	661967	37.45%	3.655%
10	9.163	1010	1016	1026	rBV	340363	567029	32.08%	3.131%
11	9.886	1132	1139	1149	rBV	285702	465997	26.37%	2.573%
12	10.427	1223	1231	1244	rBV	390885	655856	37.11%	3.621%
13	10.804	1288	1295	1302	rBV	355123	576492	32.62%	3.183%
14	10.951	1313	1320	1333	rBV	361454	629583	35.62%	3.476%
15	12.398	1560	1566	1569	rBV5	3218	5887	0.33%	0.033%
16	14.033	1838	1844	1852	rBV	622362	848088	47.98%	4.683%
17	14.321	1884	1893	1903	rBV	690749	939487	53.15%	5.188%
18	14.627	1937	1945	1955	rVB	482962	679719	38.46%	3.753%
19	14.827	1974	1979	1998	rBV	244725	406347	22.99%	2.244%
20	15.615	2107	2113	2121	rBV	875514	1165001	65.91%	6.433%
21	15.739	2129	2134	2146	rBV	324626	452105	25.58%	2.496%
22	15.857	2149	2154	2159	rVV6	2712	4770	0.27%	0.026%
23	17.168	2373	2377	2380	rVB4	1526	2322	0.13%	0.013%
24	17.368	2404	2411	2419	rBV	581571	780324	44.15%	4.309%
25	17.468	2421	2428	2441	rVV	915625	1259836	71.28%	6.956%
26	17.886	2493	2499	2501	rBV5	1960	2977	0.17%	0.016%
27	18.209	2550	2554	2556	rBV4	1949	2061	0.12%	0.011%
28	18.250	2556	2561	2562	rVV4	1712	2113	0.12%	0.012%
29	18.315	2570	2572	2577	rBV3	1956	2718	0.15%	0.015%
30	18.815	2655	2657	2660	rVB4	1819	1847	0.10%	0.010%
31	19.321	2739	2743	2746	rVB5	9753	11482	0.65%	0.063%
32	19.392	2751	2755	2758	rBV	8616	10736	0.61%	0.059%
33	19.503	2772	2774	2776	rBV4	2347	2006	0.11%	0.011%
34	19.662	2798	2801	2805	rBV4	4898	5916	0.33%	0.033%
35	19.750	2811	2816	2823	rBV	1139812	1514830	85.71%	8.364%
36	20.727	2979	2982	2987	rVB3	57250	66209	3.75%	0.366%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011023\
Data File : BM038417.D
Acq On : 10 Jan 2023 09:55
Operator : CG/JU
Sample : PB150090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK090

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Title : SVOA CALIBRATION

37	21.539	3115	3120	3127	rBV	667498	860929	48.71%	4.754%
38	23.815	3500	3507	3519	rBV	941379	1767467	100.00%	9.759%
39	23.968	3527	3533	3545	rVB2	499146	984301	55.69%	5.435%




Sum of corrected areas: 18110251

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011023\
Data File : BM038417.D
Acq On : 10 Jan 2023 09:55
Operator : CG/JU
Sample : PB150090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

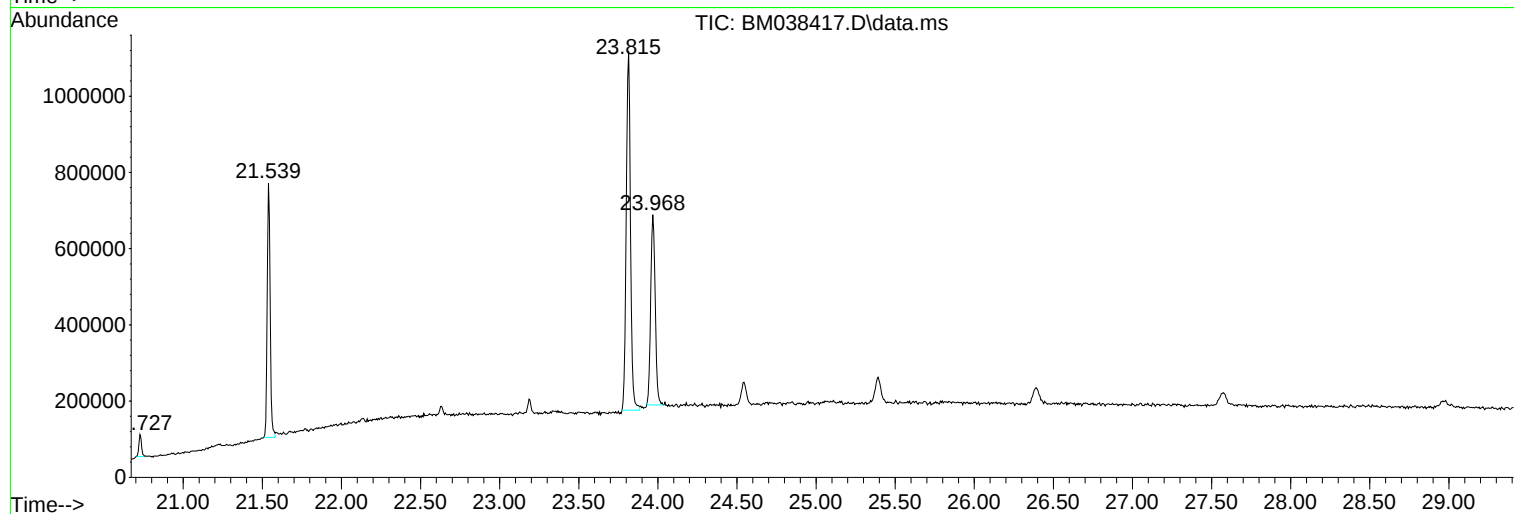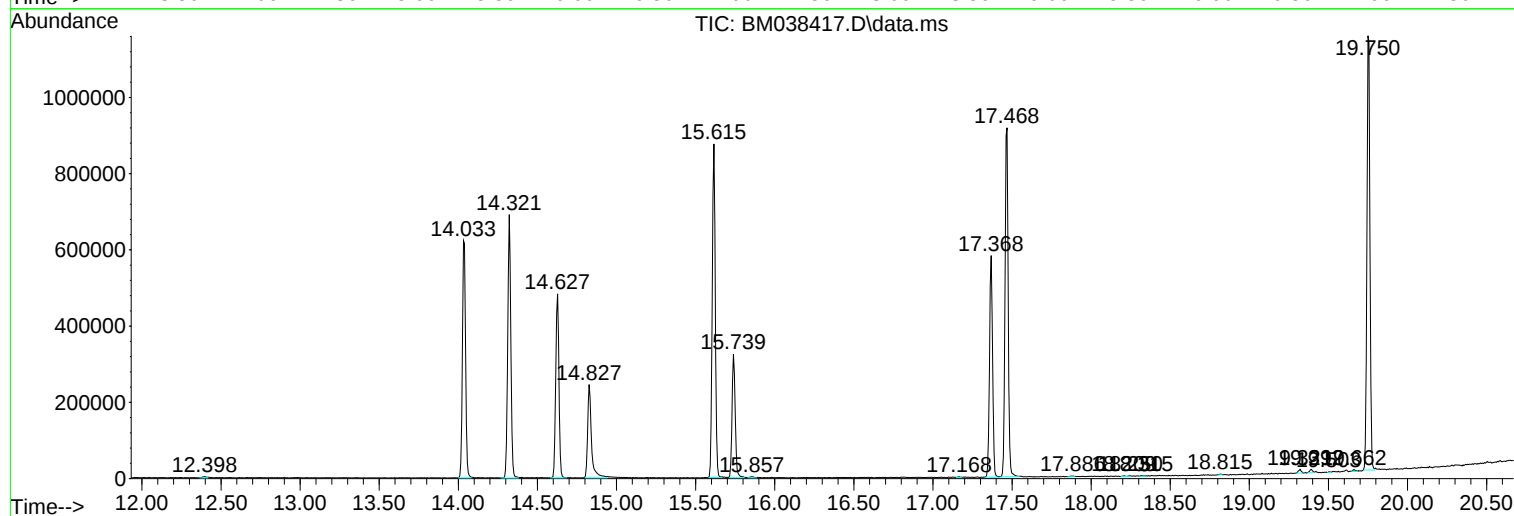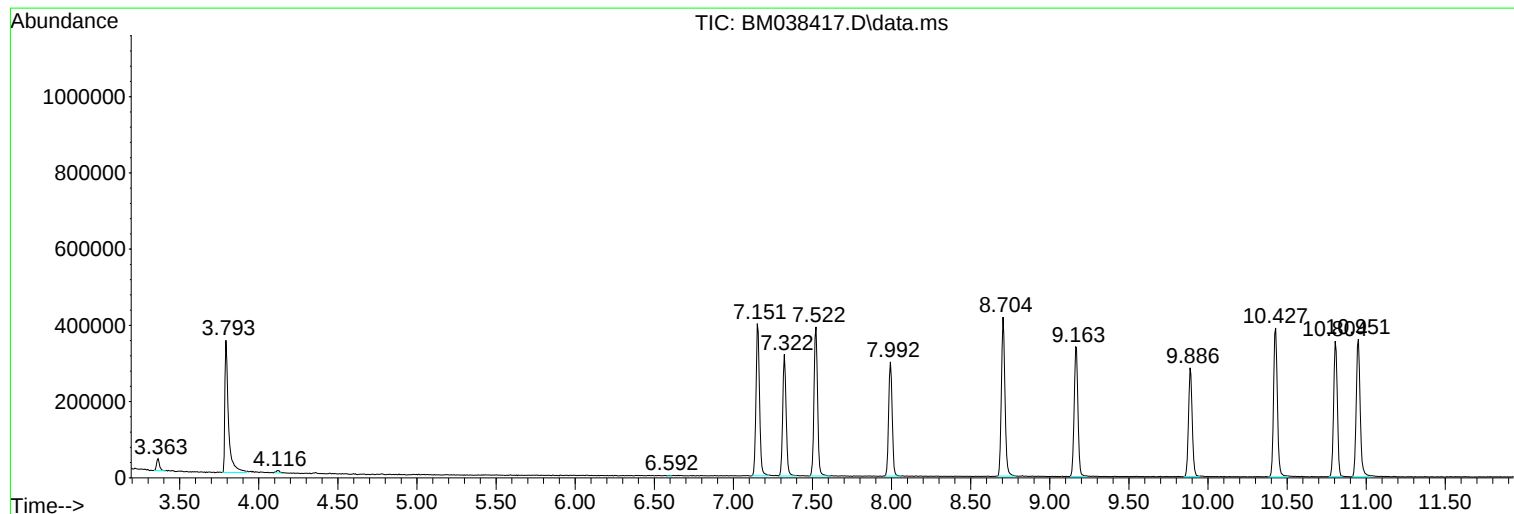

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011023\
Data File : BM038417.D
Acq On : 10 Jan 2023 09:55
Operator : CG/JU
Sample : PB150090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011023\
Data File : BM038417.D
Acq On : 10 Jan 2023 09:55
Operator : CG/JU
Sample : PB150090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc