


Data Path : Z:\HPCHEM1\BNA M\DATA\BM011116\
Data File : BM003934.D
Acq On : 11 Jan 2016 09:07
Operator : SJ/UM
Sample : DFTPP67
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP67

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION
Last Update : Tue Jan 12 00:35:37 2016

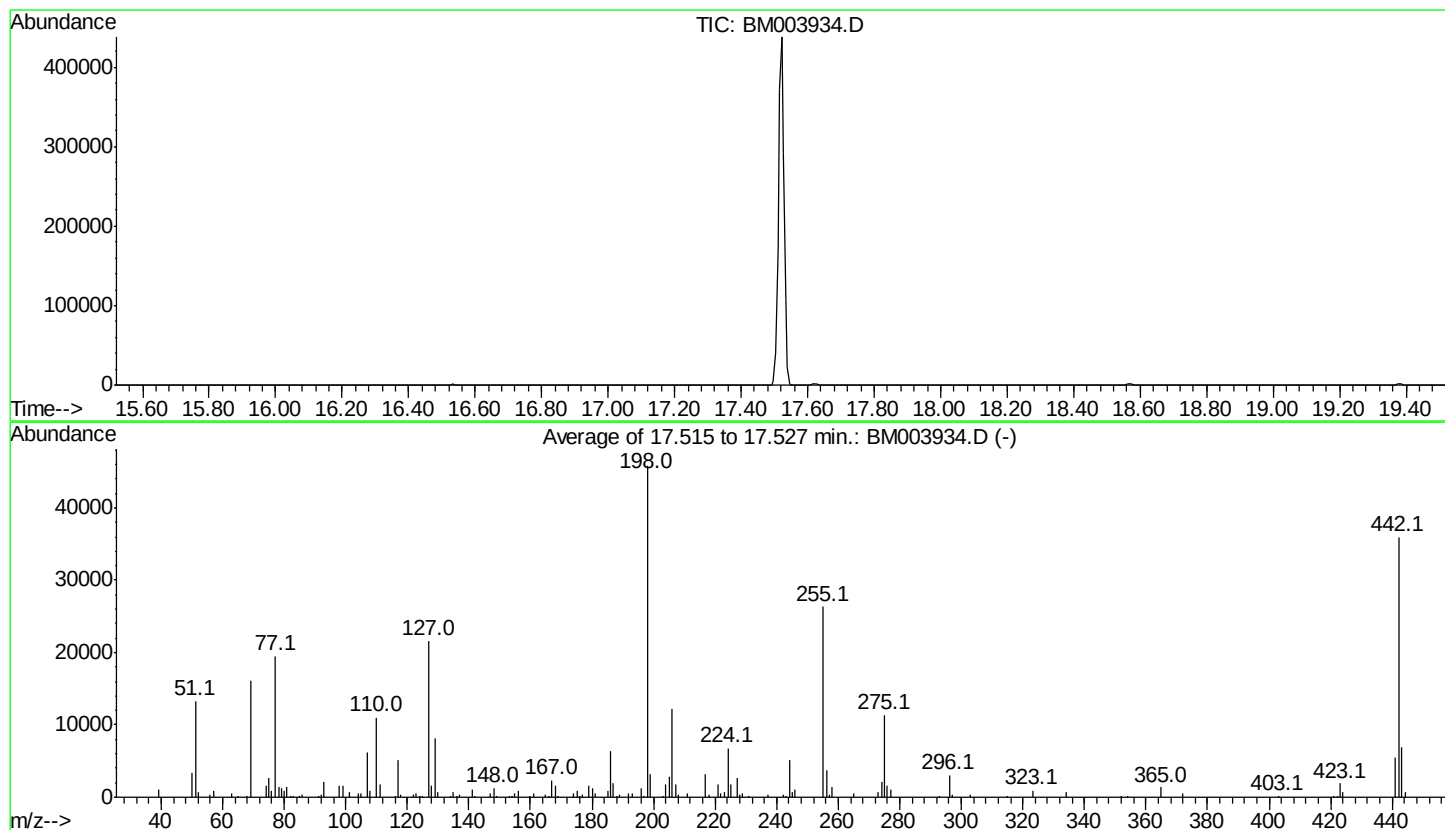

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	13343	PASS
68	69	0.00	2	1.3	211	PASS
69	198	0.00	100	35.1	16103	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	21664	PASS
197	198	0.00	2	0.2	112	PASS
198	198	100	100	100.0	45824	PASS
199	198	5	9	6.8	3115	PASS
275	198	10	60	24.8	11387	PASS
365	198	1	100	2.9	1336	PASS
441	443	0.01	100	78.4	5468	PASS
442	198	50	100	78.4	35936	PASS
443	442	15	24	19.4	6975	PASS

m/z	Abundance
39.10	1088.0
50.10	3860.0
51.10	15515.0
52.00	816.0
56.00	487.0
57.00	1125.0
63.00	727.0
65.10	374.0
68.00	308.0
69.00	18384.0
74.00	1847.0
75.00	2959.0
76.00	960.0
77.10	21856.0
78.10	1523.0
79.00	1372.0
80.00	1011.0
81.00	1544.0
82.00	370.0
83.00	446.0
85.00	335.0
85.90	408.0
91.00	342.0
92.00	412.0
93.00	2389.0
98.00	1715.0
99.00	1916.0
101.00	847.0
104.00	565.0
105.00	556.0
107.00	6738.0
108.00	941.0
110.00	12097.0
111.00	1881.0
116.00	363.0
117.00	5525.0
118.00	467.0
122.00	459.0
123.00	673.0
124.00	340.0
127.00	23312.0
128.00	1756.0
129.00	8763.0
130.00	767.0
135.00	726.0
136.00	311.0
137.10	478.0
141.00	1135.0
142.00	359.0
147.00	677.0
148.00	1331.0
149.00	388.0
153.00	369.0
155.00	710.0
156.00	982.0
159.90	378.0
161.00	552.0
165.00	402.0
166.00	319.0
167.00	2456.0
168.00	2002.0
169.00	343.0
174.10	491.0
175.10	919.0
176.10	324.0
177.00	397.0
179.00	1621.0
180.00	1466.0
181.00	579.0
185.00	842.0
186.10	6371.0
187.00	1883.0
189.00	392.0
192.00	527.0
193.00	635.0
196.10	1267.0
198.00	45752.0
199.00	3328.0
203.00	378.0
204.10	1781.0
205.10	2674.0
206.10	12204.0
207.00	1682.0
208.00	390.0
211.00	483.0
217.00	3091.0
218.00	467.0
221.00	1790.0
221.80	493.0
223.10	701.0
224.10	6674.0

Instrument :

BNA_M

ClientSampleId :

DFTPP67

225.10	1699.0
227.00	2601.0
228.00	452.0
229.00	584.0
237.00	394.0
242.00	331.0
243.00	329.0
244.10	4952.0
245.10	708.0
246.00	961.0
255.10	25032.0
256.10	3718.0
257.00	423.0
258.10	1422.0
265.00	569.0
273.00	740.0
274.10	1887.0
275.10	10879.0
276.10	1573.0
277.00	1007.0
296.00	2820.0
297.00	410.0
303.00	309.0
315.00	322.0
323.10	802.0
334.10	604.0
365.00	1202.0
372.10	443.0
423.10	1509.0
424.10	664.0
441.10	4325.0
442.10	28488.0
443.10	5630.0
444.10	530.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67

m/z	Abundance
39.00	1228.0
50.10	3962.0
51.10	15523.0
52.10	785.0
56.00	454.0
57.00	1085.0
63.00	682.0
65.00	359.0
68.10	325.0
69.00	18496.0
74.00	1913.0
75.00	3049.0
76.00	1080.0
77.10	22672.0
78.10	1591.0
79.00	1432.0
80.00	1139.0
81.00	1542.0
82.00	369.0
83.00	367.0
85.00	343.0
86.00	402.0
91.00	332.0
92.00	430.0
93.00	2392.0
98.00	1899.0
99.00	1685.0
101.00	872.0
104.00	594.0
105.00	528.0
107.00	7284.0
108.00	1125.0
110.00	13059.0
111.00	2034.0
116.00	367.0
117.00	5934.0
118.00	456.0
122.00	411.0
123.00	720.0
124.00	360.0
125.00	312.0
127.00	25568.0
128.00	1926.0
129.00	9547.0
130.00	844.0
134.00	301.0
135.00	861.0
135.90	306.0
137.00	469.0
141.00	1286.0
142.00	393.0
147.00	689.0
148.00	1471.0
149.00	340.0
153.00	382.0
153.90	349.0
155.00	718.0
156.00	1088.0
160.00	383.0
161.00	597.0
165.00	449.0
166.00	390.0
167.00	2815.0
168.00	1669.0
174.10	593.0
175.00	1059.0
177.00	437.0
179.00	2016.0
180.00	1453.0
181.00	734.0
185.10	1009.0
186.10	7628.0
187.00	2249.0
188.00	317.0
189.00	459.0
192.00	629.0
193.00	694.0
196.00	1491.0
197.00	336.0
198.00	54824.0
199.00	3610.0
203.00	340.0
204.00	2008.0
205.10	3432.0
206.10	14444.0
207.10	2034.0
208.00	557.0
211.00	547.0
217.00	3870.0
217.90	433.0
221.10	1949.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67

221.80	540.0
223.00	858.0
224.10	8026.0
225.00	2068.0
227.00	3303.0
228.00	455.0
229.00	751.0
231.00	303.0
237.00	454.0
242.00	410.0
243.00	448.0
244.10	5981.0
245.00	858.0
246.00	1232.0
255.10	31728.0
256.10	4467.0
257.00	419.0
258.00	1653.0
265.00	776.0
273.00	866.0
274.10	2509.0
275.10	13524.0
276.00	1852.0
277.10	1199.0
293.00	327.0
296.10	3766.0
297.00	489.0
303.10	450.0
315.00	409.0
323.10	1254.0
334.10	800.0
352.00	306.0
354.10	400.0
365.00	1519.0
372.10	634.0
403.00	420.0
421.10	317.0
422.10	336.0
423.10	2227.0
424.10	709.0
441.10	6279.0
442.10	42096.0
443.20	8369.0
444.10	802.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67

m/z	Abundance
39.00	702.0
50.10	2278.0
51.10	8993.0
52.00	440.0
57.00	632.0
63.00	410.0
69.00	11429.0
74.00	1167.0
75.00	1798.0
76.10	604.0
77.10	13856.0
78.10	912.0
79.00	913.0
80.00	649.0
81.00	1001.0
86.00	320.0
93.00	1462.0
98.00	1214.0
99.00	1073.0
101.00	500.0
103.90	331.0
105.00	337.0
107.00	4447.0
108.00	688.0
110.00	7839.0
111.00	1220.0
117.00	3839.0
122.90	478.0
127.00	16113.0
128.00	1096.0
129.00	6080.0
129.90	498.0
135.00	565.0
137.10	306.0
141.00	756.0
147.00	479.0
148.00	1000.0
155.00	419.0
156.00	736.0
161.00	398.0
165.00	324.0
167.00	1886.0
168.00	1162.0
174.00	378.0
175.00	771.0
177.00	345.0
179.00	1320.0
180.00	987.0
181.00	400.0
185.00	578.0
186.00	4957.0
187.00	1505.0
189.00	338.0
192.00	424.0
193.00	512.0
196.00	1077.0
198.00	36896.0
199.00	2408.0
204.10	1352.0
205.00	2381.0
206.10	9963.0
207.00	1477.0
208.00	330.0
211.10	371.0
217.00	2578.0
217.90	334.0
221.00	1534.0
221.80	344.0
223.00	649.0
224.10	5734.0
225.00	1431.0
227.00	2273.0
228.00	326.0
229.00	505.0
242.00	312.0
244.10	4302.0
245.10	528.0
246.00	864.0
255.10	22296.0
256.10	3174.0
258.00	1251.0
265.10	521.0
273.10	639.0
274.00	1791.0
275.10	9760.0
276.00	1305.0
277.00	918.0
296.00	2659.0
297.00	344.0
303.00	331.0
323.10	880.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67

334.10	583.0
352.10	337.0
365.00	1288.0
372.10	514.0
403.10	300.0
423.10	1971.0
424.10	586.0
441.10	5800.0
442.10	37224.0
443.10	6928.0
444.10	637.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67