


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011121\
 Data File : BM028362.D
 Acq On : 11 Jan 2021 09:08
 Operator : CG/JU
 Sample : DFTPP14
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP014

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM011121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 11 13:19:00 2021

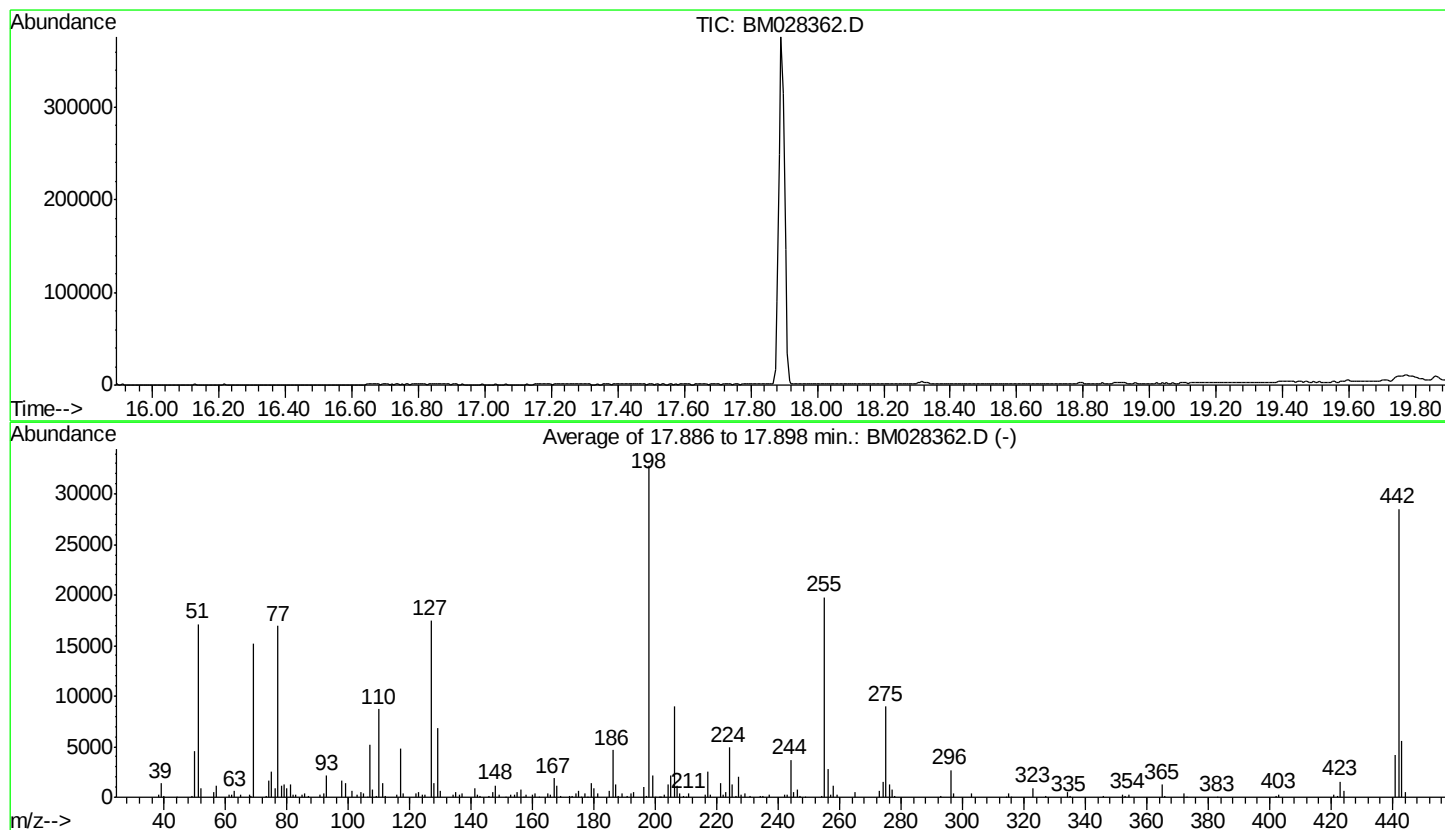

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	17156	PASS
68	69	0.00	2	1.4	218	PASS
69	198	0.00	100	46.4	15210	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.2	17468	PASS
197	198	0.00	2	0.5	168	PASS
198	198	100	100	100.0	32805	PASS
199	198	5	9	6.4	2111	PASS
275	198	10	60	27.4	8974	PASS
365	198	1	100	3.7	1225	PASS
441	198	0.01	100	12.9	4220	PASS
442	198	50	100	87.0	28539	PASS
443	442	15	24	19.3	5520	PASS

m/z	Abundance
38.00	239.0
39.00	1205.0
40.00	183.0
44.00	517.0
50.10	4155.0
51.10	15926.0
52.00	918.0
56.00	476.0
57.00	996.0
61.00	183.0
62.00	267.0
63.00	550.0
65.00	253.0
68.00	274.0
69.00	14167.0
73.10	245.0
74.00	1501.0
75.00	2378.0
76.00	752.0
77.10	15306.0
78.10	1054.0
79.00	1129.0
79.90	814.0
81.00	1222.0
82.00	221.0
83.00	244.0
85.00	174.0
85.90	359.0
86.90	155.0
90.90	283.0
92.00	410.0
93.00	1879.0
98.00	1531.0
99.00	1175.0
101.00	571.0
103.00	178.0
104.00	366.0
105.00	405.0
107.00	4460.0
108.00	750.0
109.00	157.0
110.00	7600.0
111.00	1218.0
116.00	283.0
117.00	4335.0
117.90	385.0
122.00	302.0
123.00	460.0
124.00	257.0
125.00	241.0
127.00	14966.0
128.00	1114.0
129.00	6030.0
130.00	551.0
133.90	160.0
135.00	442.0
136.00	222.0
137.00	254.0
141.00	785.0
142.00	252.0
147.00	361.0
148.00	1021.0
149.00	207.0
153.00	208.0
154.00	152.0
155.00	445.0
156.00	531.0
157.80	158.0
159.90	225.0
160.90	380.0
164.90	278.0
166.00	163.0
167.00	1602.0
168.00	1114.0
172.90	183.0
174.00	274.0
175.00	528.0
177.00	294.0
178.90	1150.0
180.00	872.0
181.00	373.0
185.00	496.0
186.00	3913.0
187.00	1036.0
188.00	167.0
188.90	305.0
190.90	168.0
192.00	328.0
193.00	459.0
196.00	836.0
197.10	189.0
198.00	25776.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

199.00	1711.0
199.90	163.0
201.20	165.0
202.90	180.0
204.00	1137.0
205.00	1858.0
206.10	7151.0
207.00	1275.0
208.00	332.0
209.00	158.0
210.90	264.0
216.00	201.0
217.00	1877.0
218.00	241.0
221.00	983.0
221.80	237.0
223.00	466.0
224.00	3722.0
225.00	863.0
226.10	160.0
227.00	1663.0
227.90	253.0
229.00	333.0
237.00	220.0
242.00	185.0
242.90	219.0
244.10	2781.0
245.00	427.0
246.00	593.0
255.00	14588.0
256.00	2062.0
257.00	247.0
258.00	847.0
258.90	152.0
265.00	308.0
273.00	416.0
274.00	1152.0
275.00	6189.0
276.00	947.0
277.00	628.0
292.90	155.0
296.00	1940.0
296.90	231.0
303.00	205.0
314.90	178.0
323.00	584.0
333.90	332.0
352.00	183.0
354.00	192.0
365.00	742.0
372.00	260.0
403.00	256.0
420.90	170.0
423.00	957.0
423.90	420.0
441.00	2561.0
442.00	15827.0
443.00	3408.0
444.00	341.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

Scan 2493 (17.851 min): BM028362.D
DFTPP14

m/z	Abundance
44.00	491.0
73.10	167.0
207.10	301.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

m/z	Abundance
38.00	171.0
39.00	1232.0
39.90	200.0
44.00	493.0
49.00	156.0
50.00	3925.0
51.10	14800.0
52.00	828.0
56.00	459.0
57.00	1040.0
61.00	169.0
62.00	180.0
63.00	544.0
65.00	298.0
68.20	274.0
69.00	13384.0
73.00	318.0
74.00	1485.0
75.00	2251.0
76.10	728.0
77.10	15062.0
78.00	1002.0
79.00	1148.0
80.00	851.0
81.00	1090.0
81.90	296.0
83.00	254.0
85.00	210.0
85.90	402.0
90.90	208.0
92.00	316.0
93.00	1968.0
98.00	1599.0
99.00	1309.0
101.00	611.0
103.00	175.0
103.90	445.0
104.90	353.0
107.00	4628.0
108.00	731.0
110.00	7716.0
111.00	1282.0
112.10	159.0
115.90	253.0
117.00	4467.0
117.90	385.0
121.90	400.0
123.00	528.0
124.00	266.0
125.00	158.0
127.00	16262.0
128.00	1172.0
129.00	6363.0
130.00	578.0
134.00	246.0
135.00	577.0
136.00	205.0
137.00	302.0
141.00	873.0
141.90	245.0
142.80	174.0
145.90	225.0
147.00	444.0
148.00	1111.0
149.00	252.0
152.90	341.0
153.90	196.0
154.90	408.0
156.00	753.0
157.90	218.0
160.00	289.0
161.00	381.0
165.00	352.0
165.90	258.0
167.00	1819.0
168.00	1124.0
169.00	197.0
173.00	217.0
174.00	361.0
175.00	578.0
176.90	388.0
179.00	1332.0
180.00	942.0
181.00	329.0
185.00	619.0
186.00	4443.0
187.00	1305.0
188.00	164.0
188.90	372.0
190.90	177.0
192.00	395.0
193.00	473.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

196.00	1027.0
198.00	33008.0
199.00	2101.0
201.60	167.0
202.90	266.0
204.00	1179.0
205.00	2046.0
206.00	9108.0
207.10	1499.0
208.00	368.0
209.00	153.0
210.10	167.0
211.00	366.0
216.00	230.0
217.00	2556.0
217.90	252.0
221.00	1582.0
222.00	251.0
223.00	531.0
224.00	4970.0
225.00	1409.0
227.00	2155.0
227.90	211.0
229.00	410.0
230.90	184.0
234.00	156.0
234.90	152.0
237.00	240.0
241.90	186.0
243.00	300.0
244.00	3937.0
245.00	546.0
246.00	717.0
246.90	206.0
255.00	21128.0
256.00	2987.0
257.00	265.0
258.00	1301.0
258.90	209.0
265.00	544.0
273.00	710.0
274.00	1719.0
275.00	10083.0
276.00	1247.0
277.00	783.0
277.90	164.0
292.90	165.0
296.00	2936.0
297.00	370.0
303.00	344.0
315.00	428.0
323.00	1050.0
326.90	222.0
334.00	602.0
335.00	164.0
345.90	246.0
351.90	291.0
353.00	156.0
354.00	350.0
365.00	1459.0
365.90	182.0
372.10	518.0
401.90	266.0
403.00	338.0
420.90	242.0
422.00	271.0
423.00	2052.0
424.00	656.0
441.00	5241.0
442.00	36720.0
443.00	6950.0
444.00	625.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

m/z	Abundance
38.10	323.0
39.10	1650.0
40.00	194.0
44.00	584.0
49.20	168.0
50.10	5431.0
51.10	20744.0
52.00	1024.0
56.00	597.0
57.00	1248.0
61.00	285.0
62.00	327.0
63.00	695.0
64.90	325.0
68.00	380.0
69.00	18080.0
73.10	343.0
74.00	1977.0
75.00	3043.0
76.10	1031.0
77.10	20512.0
78.00	1422.0
79.00	1437.0
80.00	1067.0
81.00	1531.0
82.00	376.0
82.90	290.0
85.00	201.0
86.00	418.0
86.90	177.0
91.00	336.0
92.00	428.0
93.00	2552.0
98.00	1996.0
99.00	1632.0
101.00	819.0
102.90	334.0
104.00	642.0
105.00	511.0
106.00	166.0
107.00	6382.0
108.00	931.0
109.00	207.0
110.00	10743.0
111.00	1611.0
112.00	274.0
116.00	416.0
117.00	5641.0
117.90	438.0
122.00	571.0
123.00	688.0
124.00	262.0
125.00	326.0
127.00	21176.0
128.00	1735.0
129.00	8025.0
130.00	742.0
134.00	277.0
135.00	631.0
136.00	249.0
137.00	453.0
141.00	1161.0
141.90	415.0
142.90	235.0
146.00	202.0
147.00	612.0
148.00	1400.0
149.00	260.0
151.00	168.0
153.00	342.0
154.00	253.0
155.00	657.0
156.00	888.0
157.00	201.0
157.90	226.0
159.90	332.0
161.00	436.0
161.90	152.0
164.90	427.0
166.00	296.0
167.00	2212.0
168.00	1276.0
169.00	277.0
171.90	244.0
173.00	175.0
174.00	444.0
175.00	775.0
175.90	192.0
176.90	377.0
177.90	179.0
178.90	1568.0
180.00	1008.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014

181.00	560.0
185.00	804.0
186.00	5692.0
187.00	1634.0
187.90	204.0
189.00	389.0
191.00	211.0
191.90	517.0
193.00	528.0
196.00	1128.0
197.10	315.0
198.00	39632.0
199.00	2522.0
201.40	196.0
203.00	296.0
204.00	1532.0
205.00	2727.0
206.00	10664.0
207.10	1732.0
208.00	495.0
210.90	427.0
216.00	290.0
217.00	3142.0
218.00	375.0
221.00	1658.0
221.90	318.0
223.00	669.0
224.10	5953.0
225.00	1453.0
226.00	196.0
227.00	2454.0
228.00	361.0
229.00	532.0
230.90	177.0
233.90	164.0
234.90	163.0
237.00	258.0
242.00	263.0
243.00	375.0
244.00	4428.0
245.00	637.0
246.00	1015.0
247.00	176.0
248.90	182.0
254.20	235.0
255.00	23696.0
256.00	3396.0
257.00	340.0
258.00	1286.0
259.00	248.0
265.00	527.0
273.00	744.0
274.00	1816.0
275.00	10650.0
276.00	1534.0
277.00	877.0
278.00	162.0
293.00	246.0
296.00	3162.0
297.00	456.0
303.00	439.0
314.00	176.0
314.90	366.0
315.90	178.0
323.00	1057.0
327.00	223.0
334.00	552.0
334.90	163.0
352.00	304.0
353.00	218.0
354.00	366.0
365.00	1474.0
366.00	197.0
372.00	543.0
372.90	158.0
383.00	159.0
401.90	194.0
402.90	302.0
420.90	235.0
421.90	185.0
423.00	1642.0
424.00	666.0
441.00	4858.0
442.00	33072.0
443.00	6204.0
444.00	571.0

Instrument :
BNA_M
ClientSampleId :
DFTPP014