

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011216\
 Data File : BM003949.D
 Acq On : 12 Jan 2016 11:38
 Operator : SJ/UM
 Sample : H1057-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9EK8

Quant Time: Jan 12 13:48:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 12 00:35:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	34358	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	164315	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	100202	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.07	188	231907	20.00	ng/ul	0.00
78) Chrysene-d12	21.28	240	258070	20.00	ng/ul	0.00
86) Perylene-d12	23.52	264	235907	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	3847	5.01	ng/uL	0.00
5) Phenol-d5	6.85	99	19892	6.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	61403	38.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	66267	28.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	42046	18.19	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	41202	33.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	44555	32.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	73972	30.69	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	0.00
44) Dimethylphthalate-d6	13.73	166	301284	38.30	ng/ul	0.00
47) Acenaphthylene-d8	14.02	160	356502	37.20	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	5691	4.03	ng/ul	0.00
58) Fluorene-d10	15.32	176	267533	40.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	36553	27.95	ng/ul	0.00
71) Anthracene-d10	17.17	188	421661	39.31	ng/ul	0.00
79) Pyrene-d10	19.48	212	475568	35.58	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.38	264	465682	39.53	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.16	88	18612	20.88	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011216\
Data File : BM003949.D
Acq On : 12 Jan 2016 11:38
Operator : SJ/UM
Sample : H1057-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9EK8

Quant Time: Jan 12 13:48:47 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 12 00:35:37 2016
Response via : Initial Calibration

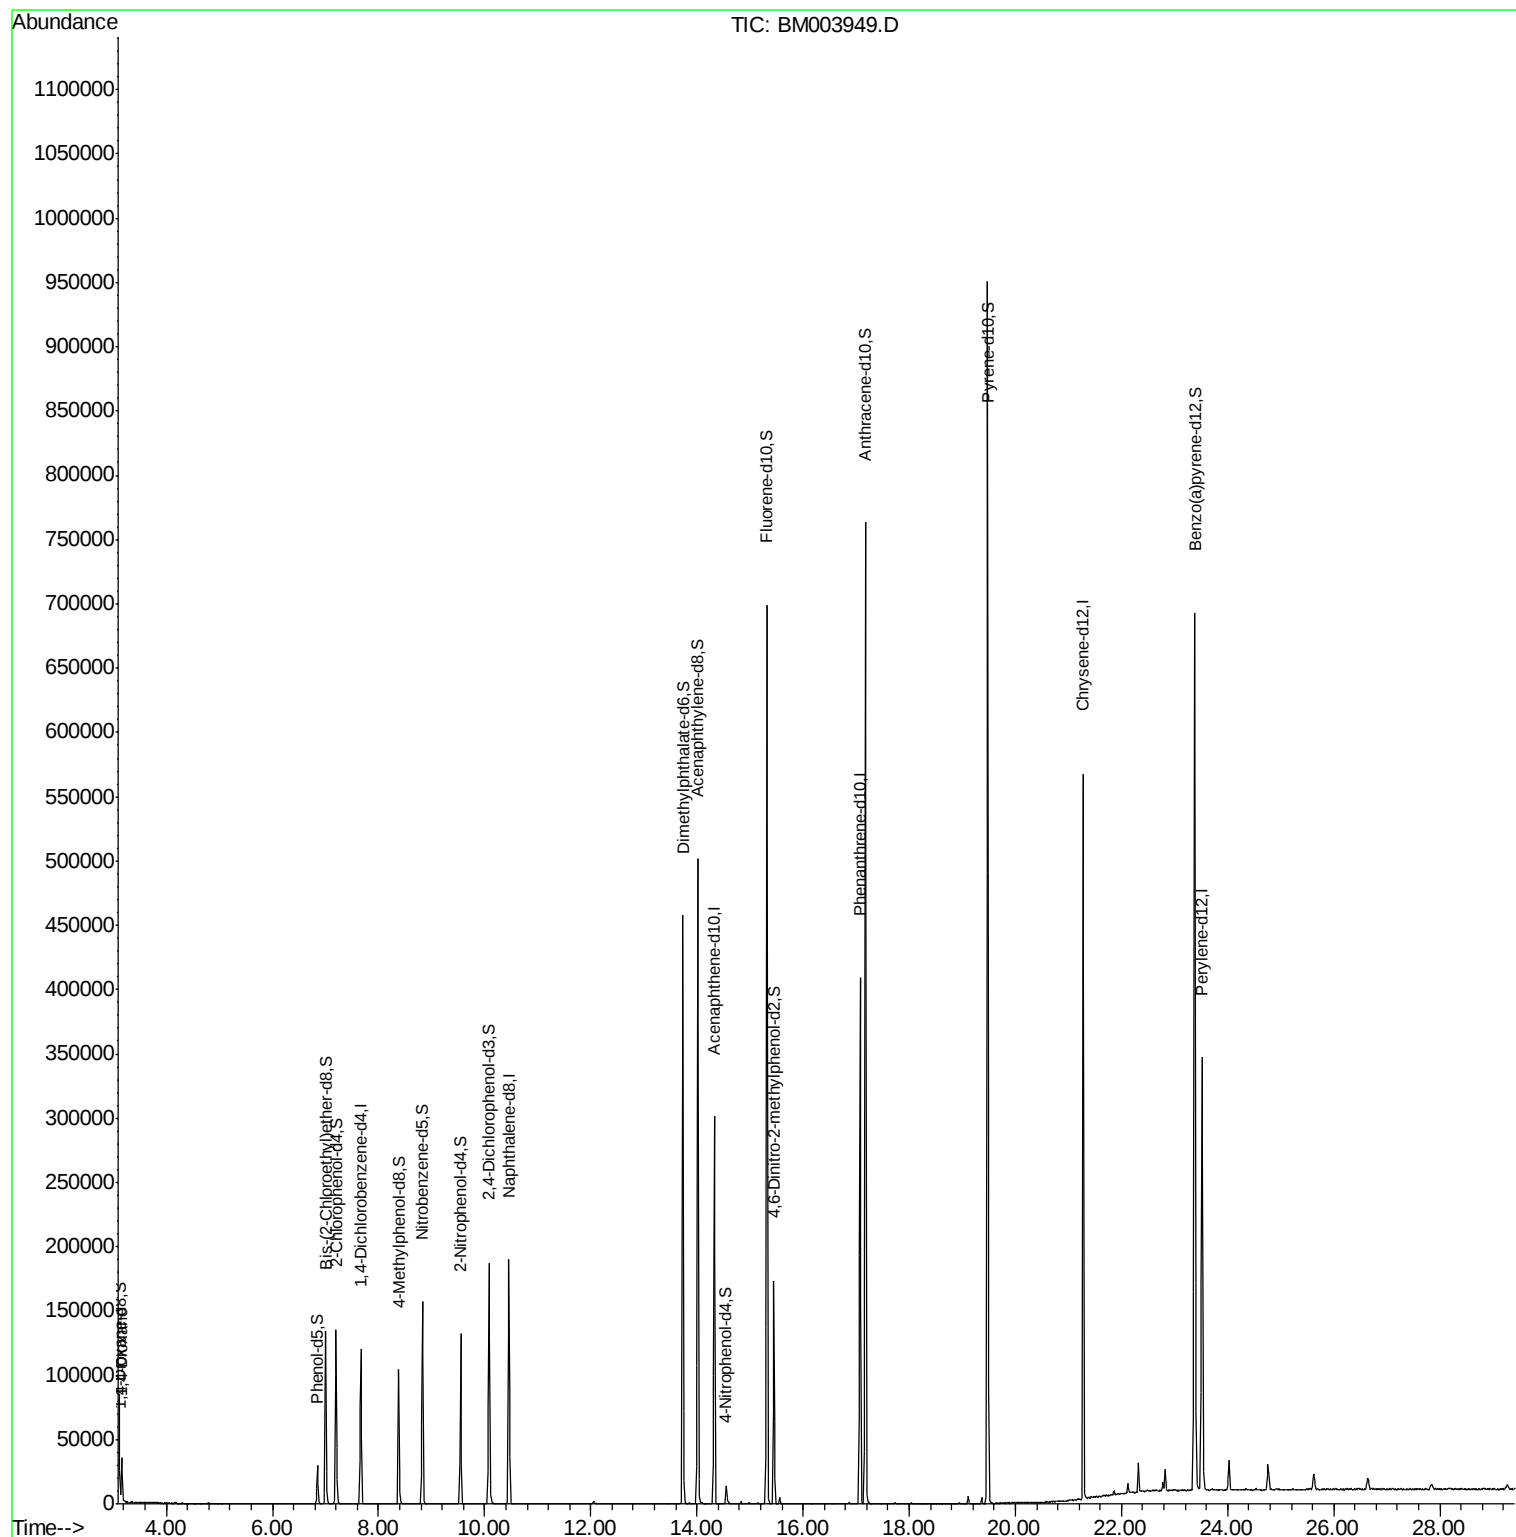

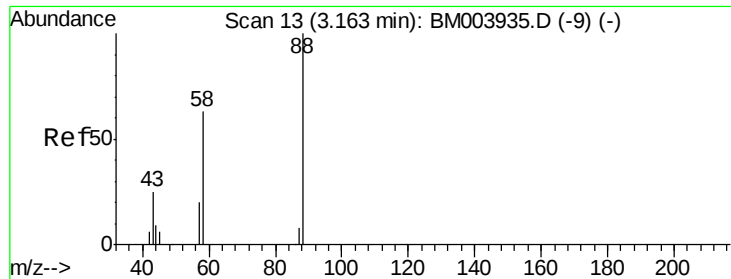

#2
 1,4-Dioxane
 Concen: 20.88 ng/uL
 RT: 3.16 min Scan# 13
 Delta R.T. 0.00 min
 Lab File: BM003949.D
 Acq: 12 Jan 2016 11:38

Instrument :
 BNA_M
 ClientSampleId :
 G9EK8

Tgt Ion: 88 Resp: 18612
 Ion Ratio Lower Upper
 88 100
 43 21.8 21.0 31.6
 58 62.4 47.8 71.8

