


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011216\
Data File : BM003946.D
Acq On : 12 Jan 2016 09:43
Operator : SJ/UM
Sample : DFTPP35
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP35

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION
Last Update : Tue Jan 12 00:35:37 2016

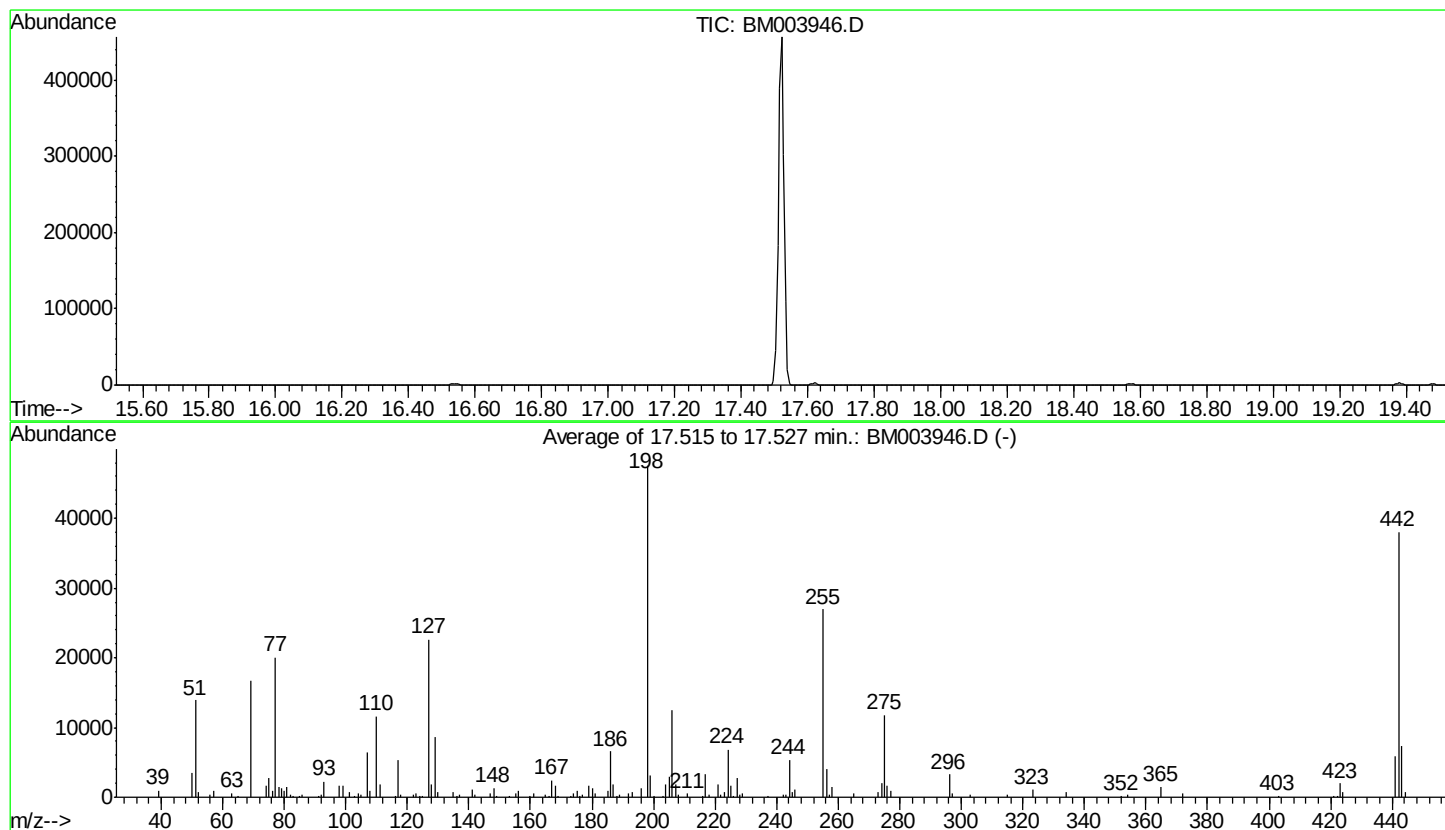

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	13911	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.2	16739	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	22669	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47560	PASS
199	198	5	9	6.6	3151	PASS
275	198	10	60	24.8	11794	PASS
365	198	1	100	3.1	1480	PASS
441	443	0.01	100	81.2	5914	PASS
442	198	50	100	80.0	38056	PASS
443	442	15	24	19.1	7279	PASS

m/z	Abundance
39.00	1192.0
50.10	4203.0
51.10	16059.0
52.10	855.0
56.00	416.0
57.00	1099.0
63.00	663.0
65.00	391.0
69.00	19384.0
74.00	2019.0
75.00	3174.0
76.10	1052.0
77.10	22736.0
78.10	1621.0
79.00	1486.0
80.00	1135.0
81.00	1543.0
82.00	409.0
83.00	435.0
85.00	314.0
86.00	411.0
91.00	408.0
92.00	458.0
93.00	2481.0
98.00	1828.0
99.00	1869.0
101.00	911.0
103.00	312.0
104.00	563.0
105.00	489.0
107.00	7194.0
108.00	1056.0
110.00	12812.0
111.00	1929.0
116.00	400.0
117.00	5663.0
118.00	444.0
122.00	412.0
122.90	670.0
123.90	300.0
125.00	302.0
127.10	24664.0
128.00	1926.0
129.00	9479.0
130.00	808.0
135.00	793.0
136.00	392.0
137.10	524.0
141.00	1125.0
142.00	381.0
147.00	729.0
148.00	1415.0
149.00	406.0
153.00	402.0
155.00	671.0
156.00	972.0
160.00	358.0
161.00	601.0
164.90	364.0
166.00	355.0
167.00	2492.0
168.00	2014.0
174.00	508.0
175.00	965.0
176.90	458.0
179.00	1800.0
180.00	1505.0
181.10	563.0
185.00	889.0
186.10	6960.0
187.00	1983.0
189.00	391.0
192.00	592.0
193.00	677.0
196.00	1241.0
198.00	48744.0
199.00	3373.0
203.00	336.0
204.00	1799.0
205.10	2900.0
206.10	12810.0
207.10	1963.0
208.00	442.0
211.00	503.0
217.00	3258.0
218.00	447.0
221.00	1763.0
221.80	531.0
223.00	685.0
224.10	6660.0
225.10	1776.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

227.00	2783.0
227.90	417.0
229.00	629.0
237.00	414.0
242.00	372.0
243.10	419.0
244.10	5102.0
245.00	629.0
246.00	975.0
255.10	25424.0
256.10	4056.0
257.00	415.0
258.00	1504.0
265.00	617.0
273.00	731.0
274.10	1974.0
275.10	11263.0
276.00	1593.0
277.00	947.0
296.10	3090.0
297.00	489.0
303.00	328.0
315.10	322.0
323.10	960.0
334.00	565.0
354.10	327.0
365.00	1246.0
372.10	456.0
423.10	1599.0
424.10	678.0
441.10	4605.0
442.10	30016.0
443.10	5956.0
444.10	546.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

m/z	Abundance
39.10	1226.0
50.10	4024.0
51.10	16217.0
52.00	759.0
56.00	546.0
57.00	1149.0
63.00	774.0
65.10	396.0
69.00	19352.0
74.00	1966.0
75.00	3213.0
76.10	975.0
77.10	23664.0
78.10	1533.0
79.00	1489.0
80.00	1130.0
81.00	1636.0
82.00	439.0
83.10	394.0
85.00	423.0
85.90	444.0
91.00	311.0
92.00	468.0
93.00	2626.0
98.00	2002.0
99.00	1918.0
101.00	927.0
103.00	316.0
104.00	562.0
105.00	536.0
107.00	7319.0
108.00	1189.0
110.00	13560.0
111.00	2087.0
116.00	415.0
117.00	6236.0
118.00	455.0
122.00	442.0
123.00	730.0
124.00	368.0
125.00	313.0
127.00	26648.0
128.00	1991.0
129.00	9938.0
130.00	922.0
135.00	901.0
137.10	479.0
141.00	1337.0
142.00	494.0
147.00	697.0
148.00	1675.0
149.00	323.0
153.00	406.0
155.10	739.0
156.00	1073.0
160.00	476.0
161.00	672.0
165.00	480.0
166.00	377.0
167.00	2788.0
168.00	1837.0
169.00	340.0
173.00	323.0
174.10	586.0
175.10	1052.0
176.00	326.0
177.00	507.0
179.00	1917.0
180.00	1597.0
181.00	687.0
185.00	979.0
186.10	7795.0
187.10	2312.0
188.00	322.0
189.00	506.0
192.00	688.0
193.00	803.0
196.00	1418.0
198.00	56504.0
199.00	3734.0
200.00	309.0
203.10	363.0
204.10	2063.0
205.10	3523.0
206.10	14964.0
207.10	2139.0
208.00	573.0
211.00	690.0
216.00	374.0
217.00	3871.0
218.00	485.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

221.10	2156.0
221.80	491.0
223.00	830.0
224.10	8264.0
225.10	2001.0
226.00	306.0
227.00	3360.0
228.00	490.0
229.00	716.0
237.00	396.0
242.10	438.0
243.00	499.0
244.10	6442.0
245.00	827.0
246.00	1248.0
255.10	32336.0
256.10	4738.0
257.00	514.0
258.00	1843.0
265.00	731.0
273.10	937.0
274.10	2477.0
275.10	14149.0
276.10	1905.0
277.00	1126.0
296.00	3870.0
297.00	548.0
303.00	461.0
315.00	397.0
323.10	1202.0
334.10	820.0
352.10	336.0
354.10	379.0
365.10	1745.0
372.10	666.0
403.10	392.0
421.10	356.0
422.10	333.0
423.10	2390.0
424.10	861.0
441.10	7268.0
442.10	45472.0
443.10	8466.0
444.10	806.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

m/z	Abundance
39.00	619.0
50.10	2303.0
51.10	9459.0
52.00	439.0
57.00	636.0
63.00	437.0
69.00	11481.0
74.00	1200.0
75.00	1875.0
76.00	653.0
77.10	13835.0
78.10	1005.0
79.00	923.0
80.00	649.0
81.00	1022.0
93.00	1546.0
98.00	1189.0
99.00	1098.0
101.00	612.0
104.00	316.0
105.00	324.0
107.00	4526.0
108.00	711.0
110.00	8359.0
111.00	1349.0
117.00	3856.0
123.00	441.0
127.00	16696.0
128.00	1364.0
129.00	6347.0
130.00	496.0
135.00	497.0
137.00	323.0
141.00	771.0
147.00	437.0
148.00	938.0
155.00	461.0
156.00	781.0
161.00	402.0
165.00	358.0
167.00	1904.0
168.00	1126.0
174.00	416.0
175.10	676.0
176.90	324.0
179.00	1327.0
180.00	975.0
181.00	420.0
185.00	690.0
186.10	5034.0
187.00	1464.0
188.90	317.0
192.00	386.0
193.00	506.0
196.00	1068.0
198.00	37432.0
199.00	2346.0
204.10	1414.0
205.10	2386.0
206.10	9961.0
207.10	1548.0
208.00	337.0
211.00	361.0
217.00	2736.0
218.00	305.0
221.10	1586.0
221.90	343.0
223.00	584.0
224.10	5680.0
225.10	1464.0
227.00	2411.0
229.00	470.0
242.00	318.0
244.10	4506.0
245.10	534.0
246.00	902.0
255.10	23032.0
256.10	3318.0
258.00	1272.0
265.00	493.0
273.00	668.0
274.10	1788.0
275.10	9972.0
276.10	1421.0
277.00	811.0
296.00	2796.0
297.10	386.0
303.00	303.0
315.10	326.0
323.10	980.0
334.10	675.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

352.10	316.0
354.10	308.0
365.10	1451.0
372.00	551.0
403.10	330.0
423.10	1972.0
424.10	613.0
441.10	5871.0
442.10	38680.0
443.10	7416.0
444.10	646.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35