
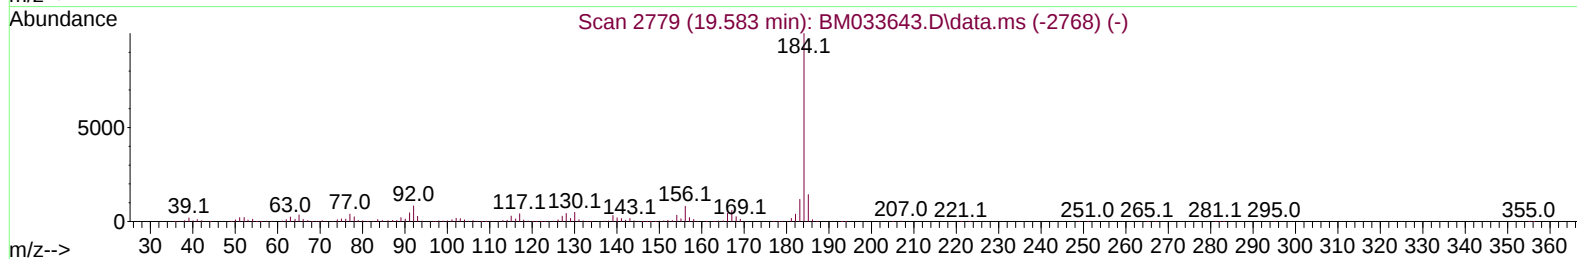
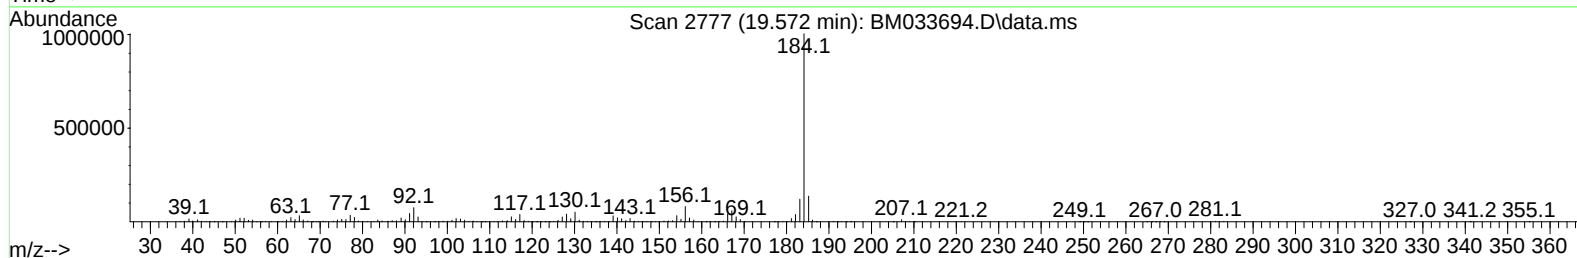


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033694.D
 Acq On : 12 Jan 2022 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 08:57:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 13 07:49:01 2022
 Response via : Initial Calibration

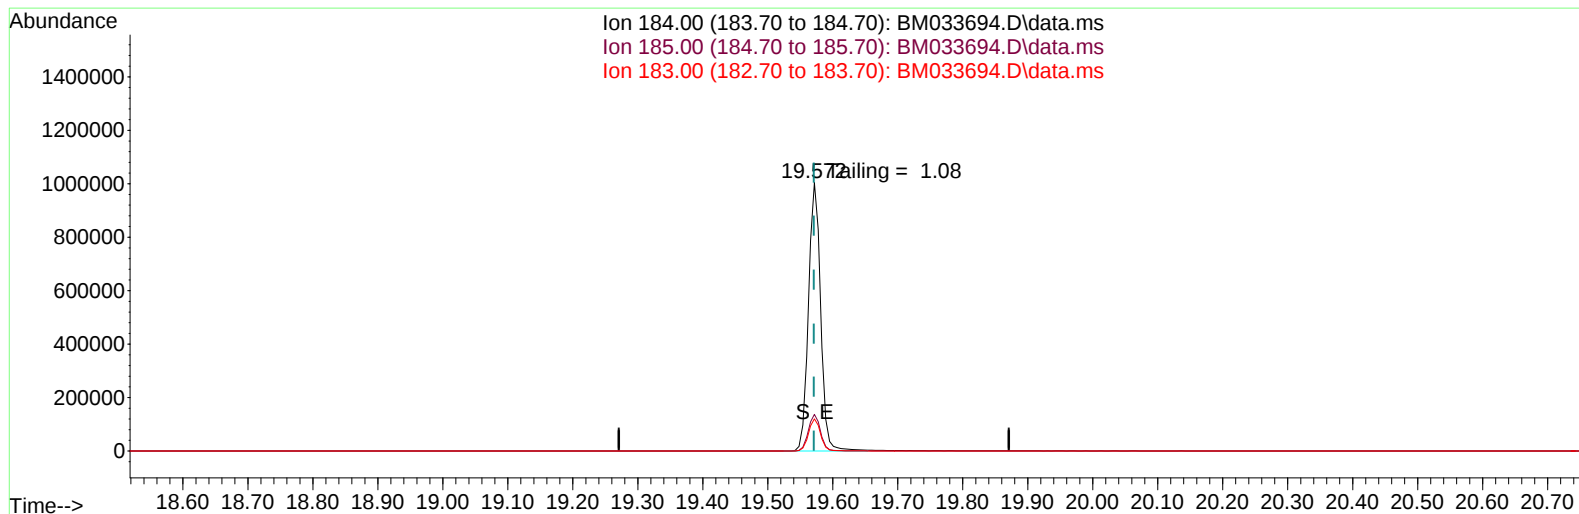




TIC: BM033694.D\data.ms

(77) Benzidine**19.572min (+ 0.000) 51782.18 ng****response 1319460**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.66
183.00	12.10	12.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033694.D
Acq On : 12 Jan 2022 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 08:57:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 13 07:49:01 2022
Response via : Initial Calibration

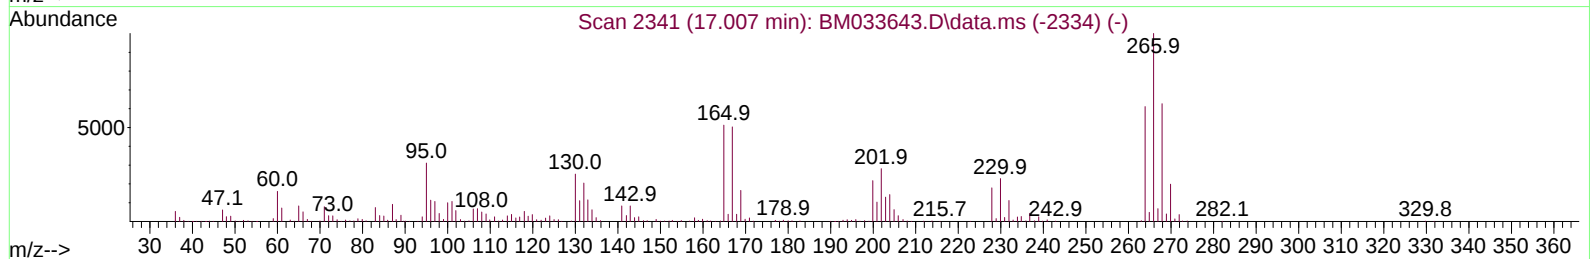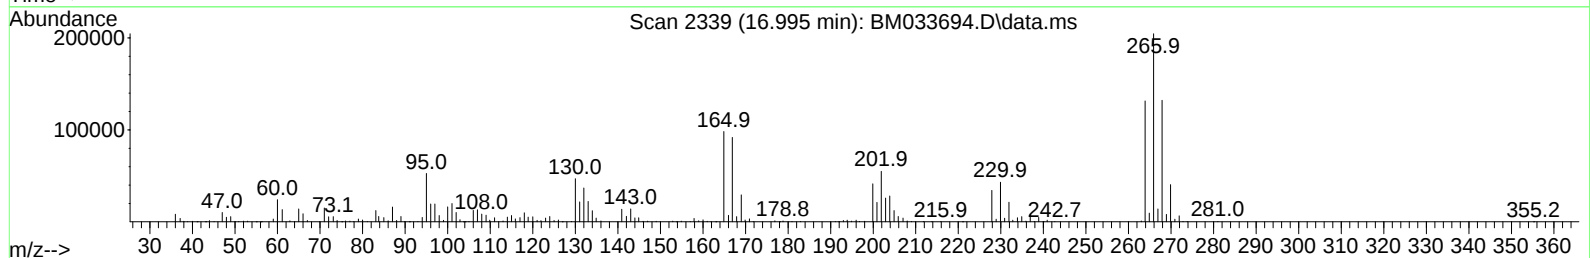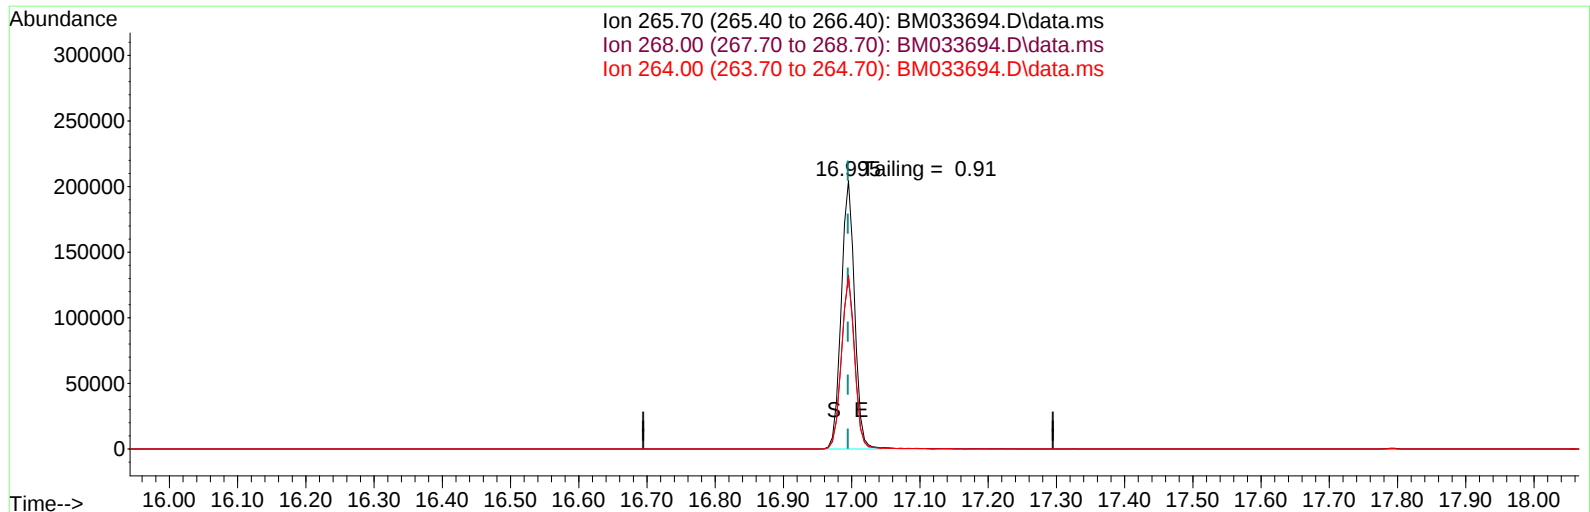

TIC: BM033694.D\data.ms

(70) Pentachlorophenol (C)

16.995min (+ 0.000) 0.00 ng

response 279047

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.61
264.00	61.40	64.30
0.00	0.00	0.00