

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033696.D
 Acq On : 12 Jan 2022 13:21
 Operator : CG/JU
 Sample : PB141980BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB141980BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.513	380	387	402	rBV	3497762	5147896	66.53%	11.773%
2	7.131	653	662	674	rBV	3171004	5221731	67.48%	11.942%
3	7.972	796	805	812	rBV	643194	1033838	13.36%	2.364%
4	9.131	994	1002	1011	rBV	2061401	3515295	45.43%	8.040%
5	10.783	1275	1283	1291	rBV	830244	1395372	18.03%	3.191%
6	13.236	1693	1700	1713	rBV	4897051	7384365	95.43%	16.888%
7	14.607	1925	1933	1947	rBV	1180544	1728023	22.33%	3.952%
8	16.089	2178	2185	2203	rBV	3491116	4963821	64.15%	11.352%
9	17.342	2391	2398	2407	rBV	1275217	1774964	22.94%	4.059%
10	19.659	2788	2792	2795	rBV2	86306	99221	1.28%	0.227%
11	19.953	2836	2842	2850	rBV	6567165	7737870	100.00%	17.697%
12	21.500	3101	3105	3112	rBV	1252218	1654974	21.39%	3.785%
13	23.924	3510	3517	3528	rVB2	1032099	2067180	26.72%	4.728%




Sum of corrected areas: 43724550

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033696.D
Acq On : 12 Jan 2022 13:21
Operator : CG/JU
Sample : PB141980BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141980BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

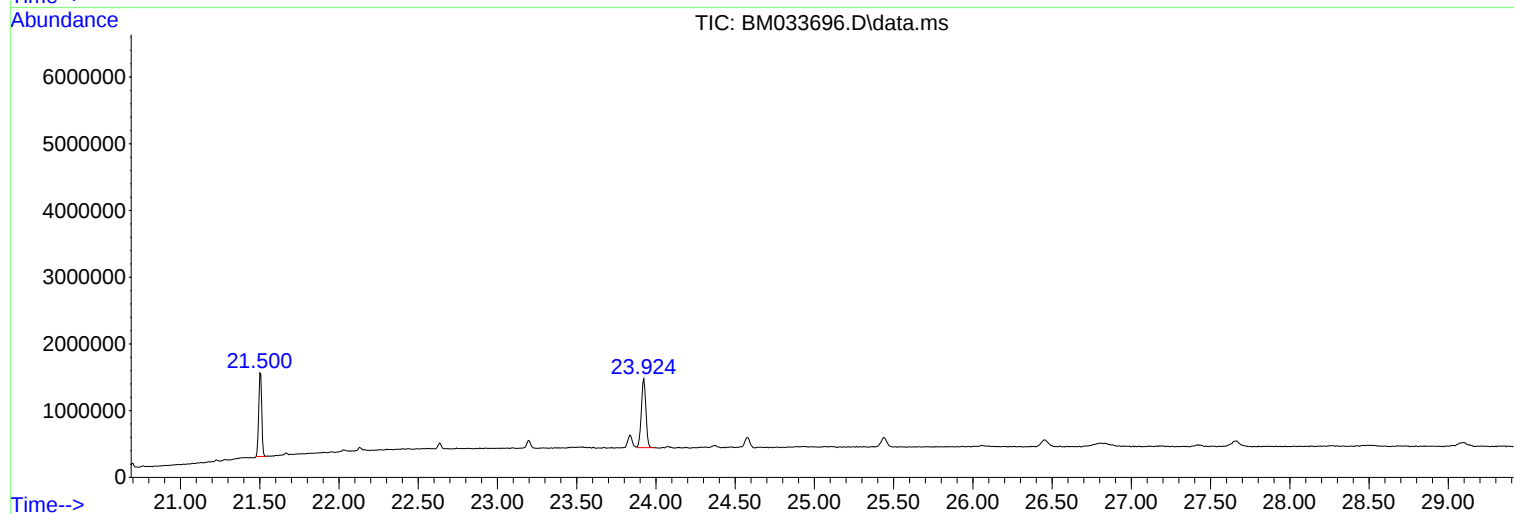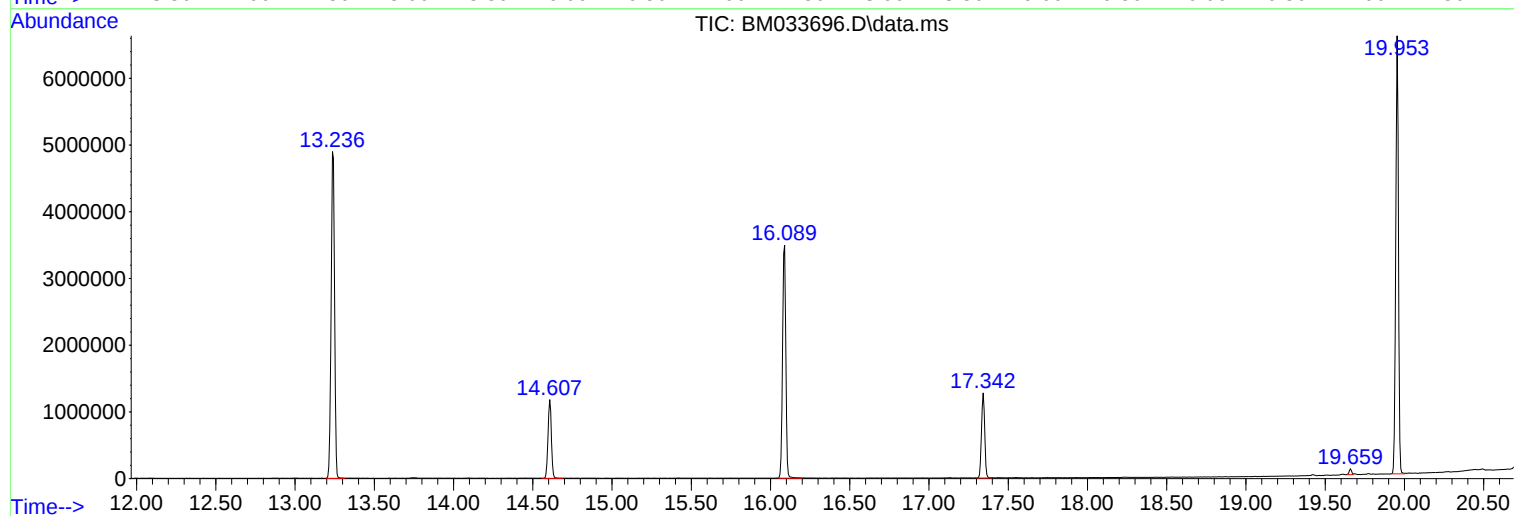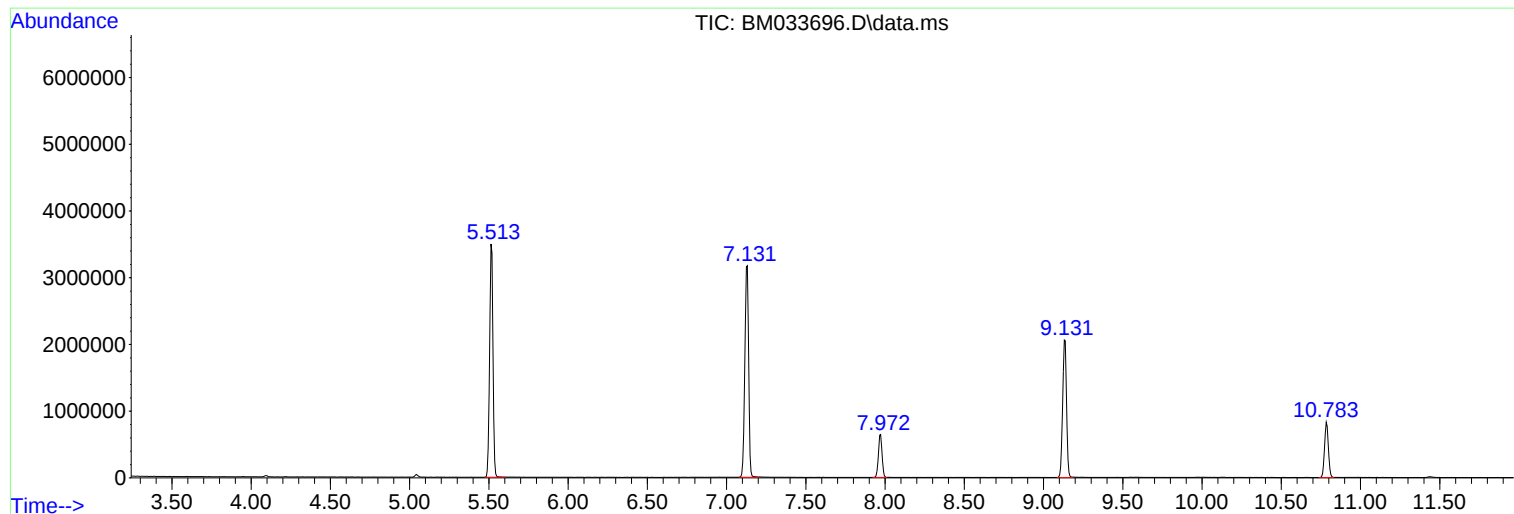

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033696.D
Acq On : 12 Jan 2022 13:21
Operator : CG/JU
Sample : PB141980BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141980BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033696.D
Acq On : 12 Jan 2022 13:21
Operator : CG/JU
Sample : PB141980BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141980BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------