

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033700.D
 Acq On : 12 Jan 2022 15:50
 Operator : CG/JU
 Sample : N1099-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-09

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.507	379	386	400	rBV	1392991	2168272	35.70%	7.439%
2	7.119	653	660	670	rBV	1495525	2431719	40.03%	8.343%
3	7.966	797	804	812	rBV	325222	517864	8.53%	1.777%
4	9.131	991	1002	1013	rBV	920827	1535379	25.28%	5.268%
5	10.560	1238	1245	1255	rBV	302737	483791	7.96%	1.660%
6	10.783	1276	1283	1290	rBV	467015	771431	12.70%	2.647%
7	13.236	1692	1700	1710	rBV	2441883	3516257	57.89%	12.064%
8	14.607	1927	1933	1943	rBV	740185	1102149	18.14%	3.782%
9	16.083	2178	2184	2200	rVB	2210665	3229687	53.17%	11.081%
10	17.342	2389	2398	2408	rBV	1005791	1438363	23.68%	4.935%
11	18.018	2508	2513	2519	rBV	66403	80821	1.33%	0.277%
12	18.236	2545	2550	2559	rBV	200105	310239	5.11%	1.064%
13	19.183	2707	2711	2716	rVB2	84646	93637	1.54%	0.321%
14	19.506	2762	2766	2774	rBV2	93901	152777	2.52%	0.524%
15	19.953	2836	2842	2848	rBV	5082760	6074155	100.00%	20.841%
16	21.212	3053	3056	3062	rBV	365707	476655	7.85%	1.635%
17	21.500	3101	3105	3111	rBV	1538933	1958279	32.24%	6.719%
18	23.924	3510	3517	3530	rVB2	1300700	2804051	46.16%	9.621%




Sum of corrected areas: 29145526

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033700.D
Acq On : 12 Jan 2022 15:50
Operator : CG/JU
Sample : N1099-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

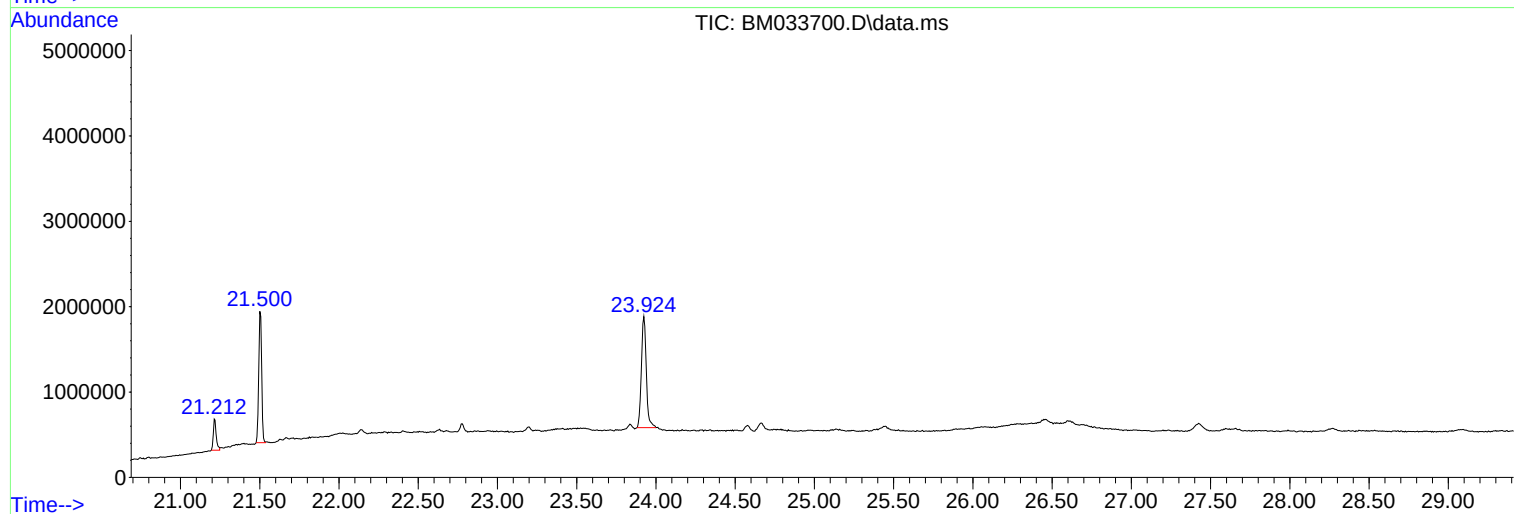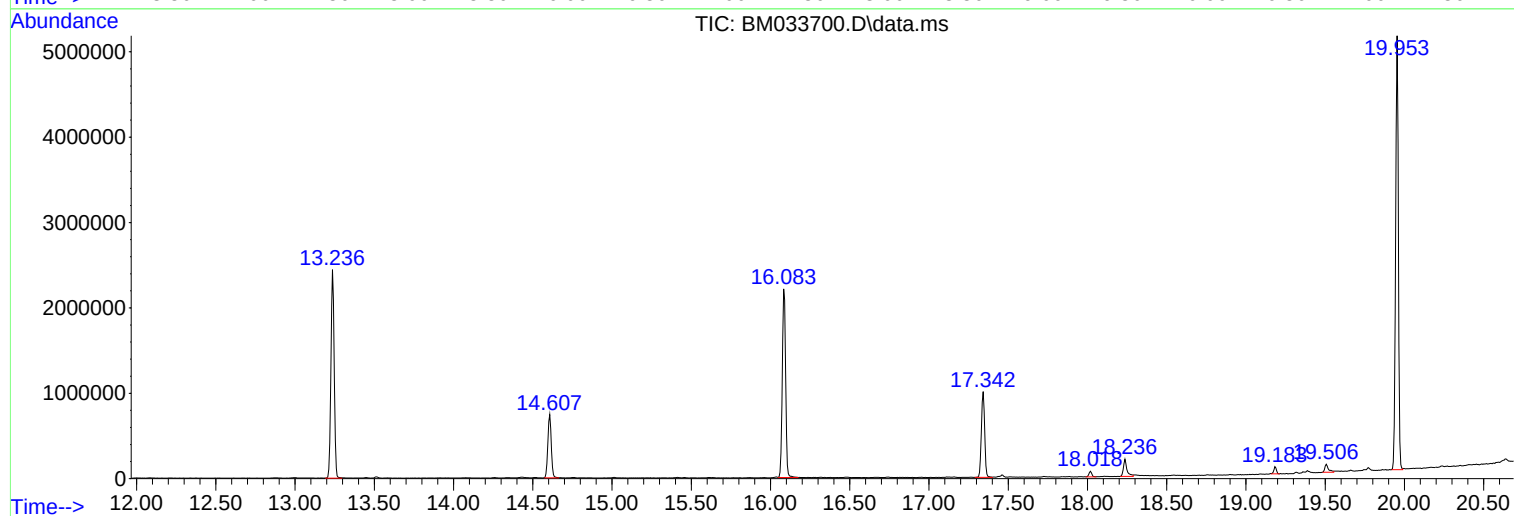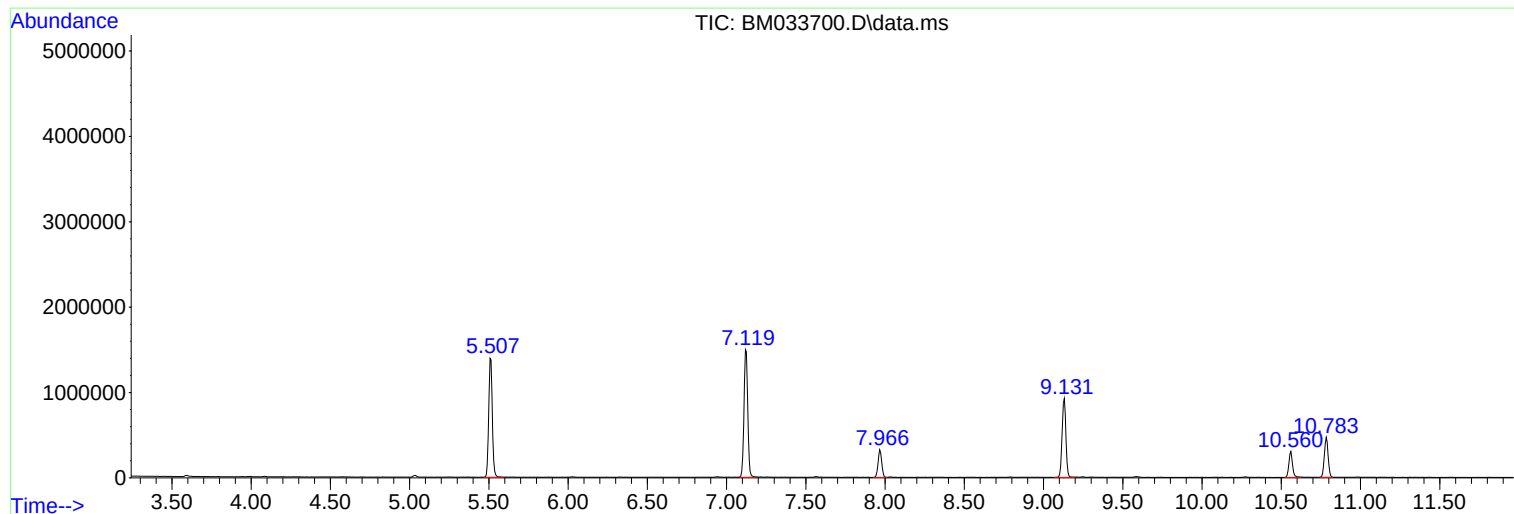

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033700.D
Acq On : 12 Jan 2022 15:50
Operator : CG/JU
Sample : N1099-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033700.D
Acq On : 12 Jan 2022 15:50
Operator : CG/JU
Sample : N1099-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------