

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033701.D
 Acq On : 12 Jan 2022 16:35
 Operator : CG/JU
 Sample : N1099-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-04

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033701.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.043	302	307	312	rVB2	58574	86658	1.45%	0.162%
2	5.513	380	387	402	rBV	2768910	4003282	67.15%	7.493%
3	7.125	653	661	675	rBV	2556072	4123457	69.17%	7.718%
4	7.972	795	805	813	rBV	572699	909460	15.26%	1.702%
5	9.136	994	1003	1014	rBV	1641826	2772826	46.51%	5.190%
6	10.278	1191	1197	1208	rVB	42812	80182	1.35%	0.150%
7	10.560	1238	1245	1257	rBV	166419	283007	4.75%	0.530%
8	10.789	1276	1284	1291	rBV	744963	1269238	21.29%	2.376%
9	13.242	1693	1701	1711	rBV	3697751	5594060	93.84%	10.470%
10	14.607	1926	1933	1945	rBV	1030363	1495880	25.09%	2.800%
11	15.683	2098	2116	2117	rBV7	33330	116447	1.95%	0.218%
12	16.089	2178	2185	2202	rVB	2234171	3343758	56.09%	6.258%
13	17.342	2391	2398	2412	rBV	1019137	1477407	24.78%	2.765%
14	17.777	2452	2472	2487	rBV	256185	1299040	21.79%	2.431%
15	17.971	2491	2505	2513	rVV	347655	1548771	25.98%	2.899%
16	18.118	2515	2530	2543	rVV2	750519	3280197	55.02%	6.139%
17	18.236	2545	2550	2564	rVV	337674	533287	8.95%	0.998%
18	18.383	2567	2575	2588	rVB3	65856	235901	3.96%	0.442%
19	18.665	2611	2623	2635	rVB2	359068	1140689	19.13%	2.135%
20	19.389	2738	2746	2756	rBV	474753	1210911	20.31%	2.266%
21	19.506	2762	2766	2775	rBV	190323	286508	4.81%	0.536%
22	19.771	2809	2811	2821	rVB4	39304	63695	1.07%	0.119%
23	19.953	2836	2842	2848	rBV	5005494	5961482	100.00%	11.158%
24	20.348	2902	2909	2916	rVB	771202	1472941	24.71%	2.757%
25	21.118	3034	3040	3046	rBV	928783	1457986	24.46%	2.729%
26	21.218	3053	3057	3063	rBV	284742	376029	6.31%	0.704%
27	21.500	3101	3105	3110	rBV	1368341	1803002	30.24%	3.375%
28	21.794	3150	3155	3168	rVB	915962	1573012	26.39%	2.944%
29	22.518	3273	3278	3292	rVB	633236	1361427	22.84%	2.548%
30	23.341	3413	3418	3424	rVB	483309	964253	16.17%	1.805%
31	23.418	3426	3431	3444	rVB2	561793	1291761	21.67%	2.418%
32	23.924	3511	3517	3526	rVB2	997938	2012961	33.77%	3.768%




Sum of corrected areas: 53429515

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033701.D
Acq On : 12 Jan 2022 16:35
Operator : CG/JU
Sample : N1099-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

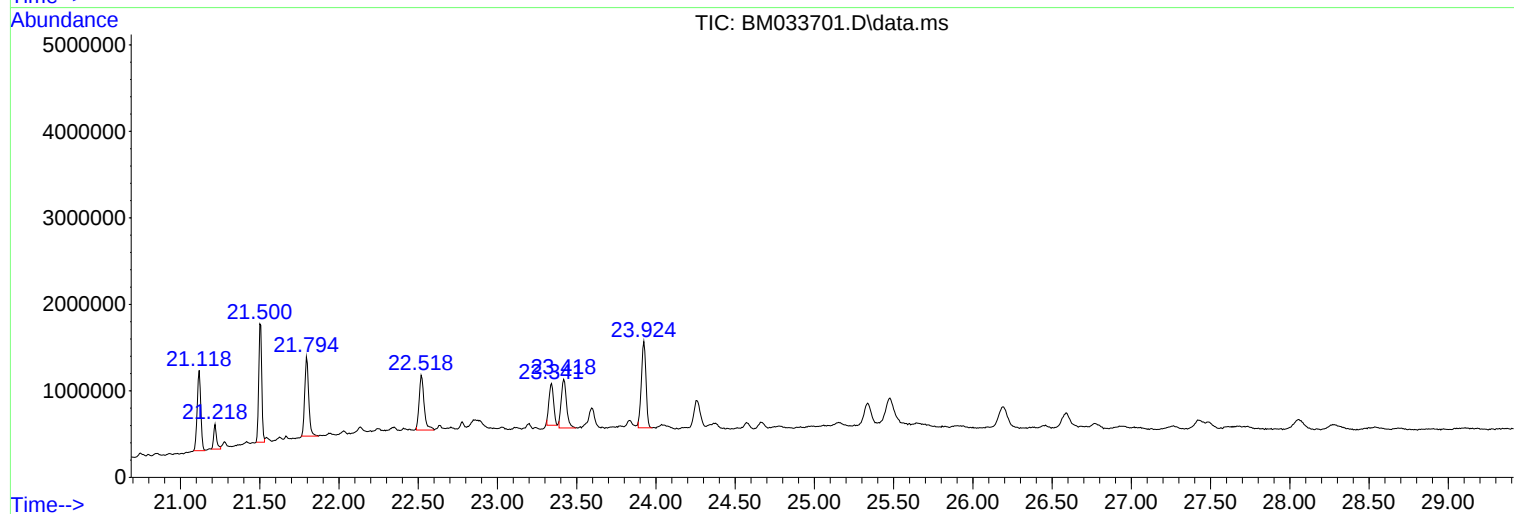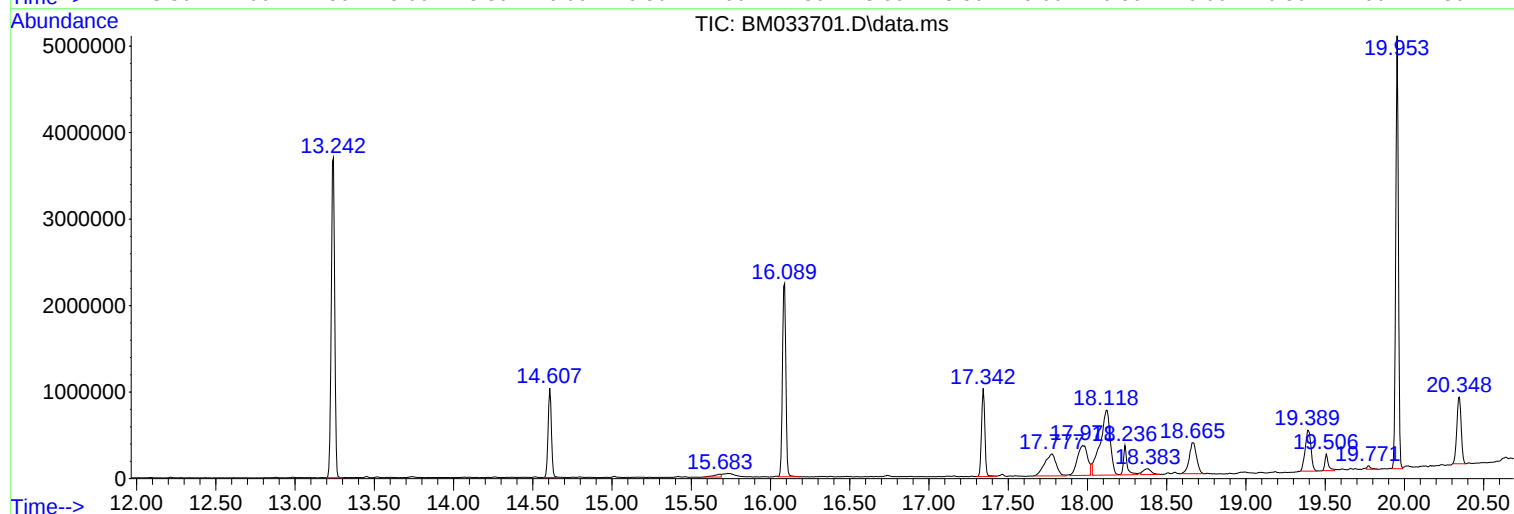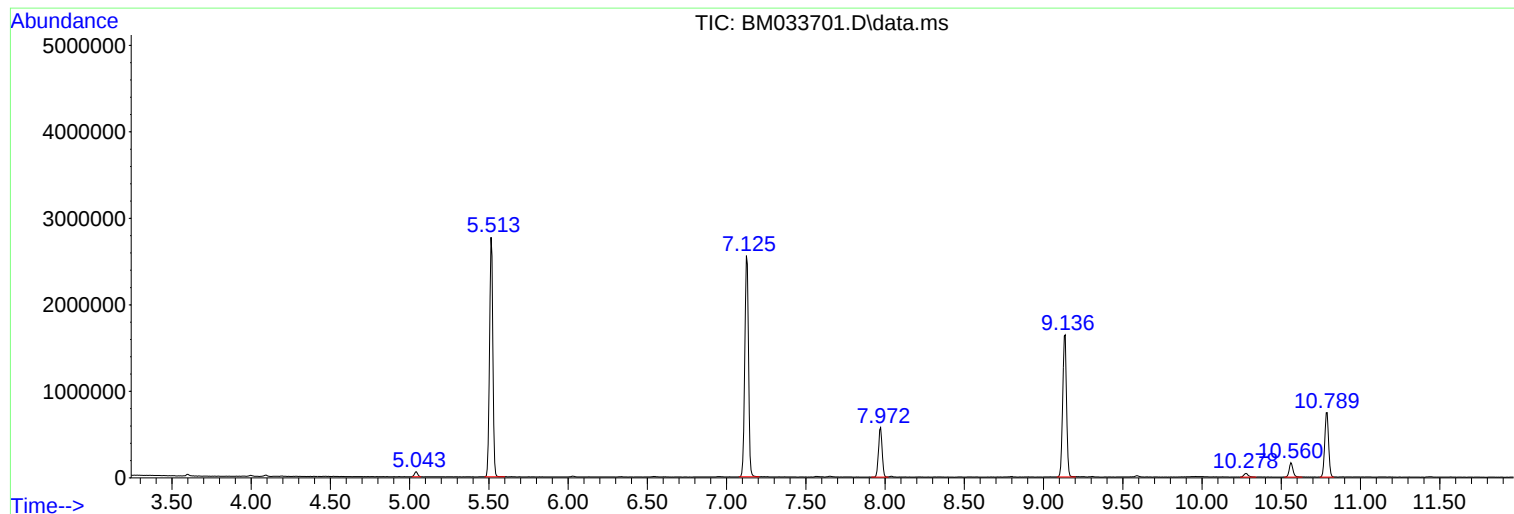

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033701.D
Acq On : 12 Jan 2022 16:35
Operator : CG/JU
Sample : N1099-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033701.D
Acq On : 12 Jan 2022 16:35
Operator : CG/JU
Sample : N1099-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------