

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033702.D
 Acq On : 12 Jan 2022 17:11
 Operator : CG/JU
 Sample : N1099-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-07

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.043	302	307	312	rVB2	86830	125801	1.97%	0.321%
2	5.513	380	387	401	rVB	3180967	4553402	71.24%	11.623%
3	7.125	653	661	674	rBV	2928831	4741069	74.18%	12.102%
4	7.972	797	805	811	rBV	569776	920990	14.41%	2.351%
5	9.131	994	1002	1012	rBV	1881305	3162119	49.47%	8.072%
6	10.278	1189	1197	1206	rBV2	39805	80872	1.27%	0.206%
7	10.560	1239	1245	1258	rBV	260006	415361	6.50%	1.060%
8	10.784	1275	1283	1291	rBV	763806	1315781	20.59%	3.359%
9	13.236	1692	1700	1713	rBV	4296316	6391628	100.00%	16.315%
10	14.607	1926	1933	1945	rBV	1054495	1554750	24.32%	3.969%
11	16.083	2178	2184	2201	rVB	2646317	3842771	60.12%	9.809%
12	17.342	2391	2398	2404	rBV	1028431	1438330	22.50%	3.671%
13	18.236	2544	2550	2561	rBV2	162869	267831	4.19%	0.684%
14	19.507	2762	2766	2770	rBV	84887	121323	1.90%	0.310%
15	19.760	2805	2809	2815	rVB3	58943	106272	1.66%	0.271%
16	19.954	2836	2842	2848	rBV	5002725	6205413	97.09%	15.840%
17	21.218	3054	3057	3062	rVB4	171828	204393	3.20%	0.522%
18	21.501	3101	3105	3111	rBV	1289483	1750334	27.38%	4.468%
19	23.924	3511	3517	3530	rVB2	921722	1977537	30.94%	5.048%




Sum of corrected areas: 39175977

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033702.D
Acq On : 12 Jan 2022 17:11
Operator : CG/JU
Sample : N1099-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

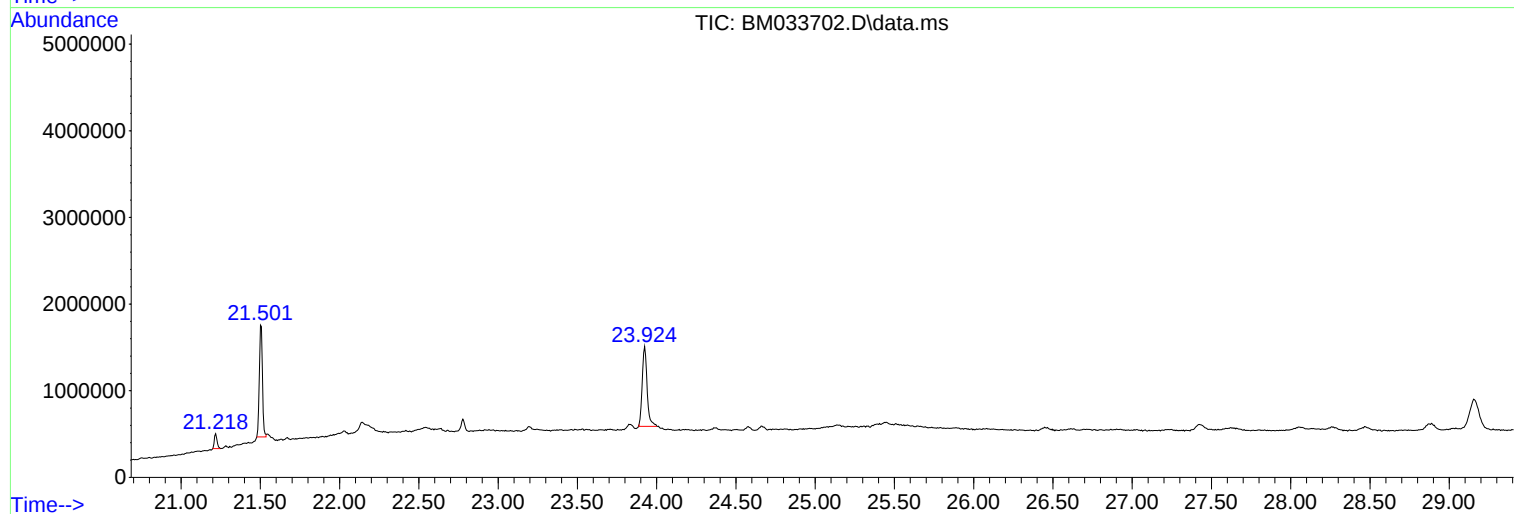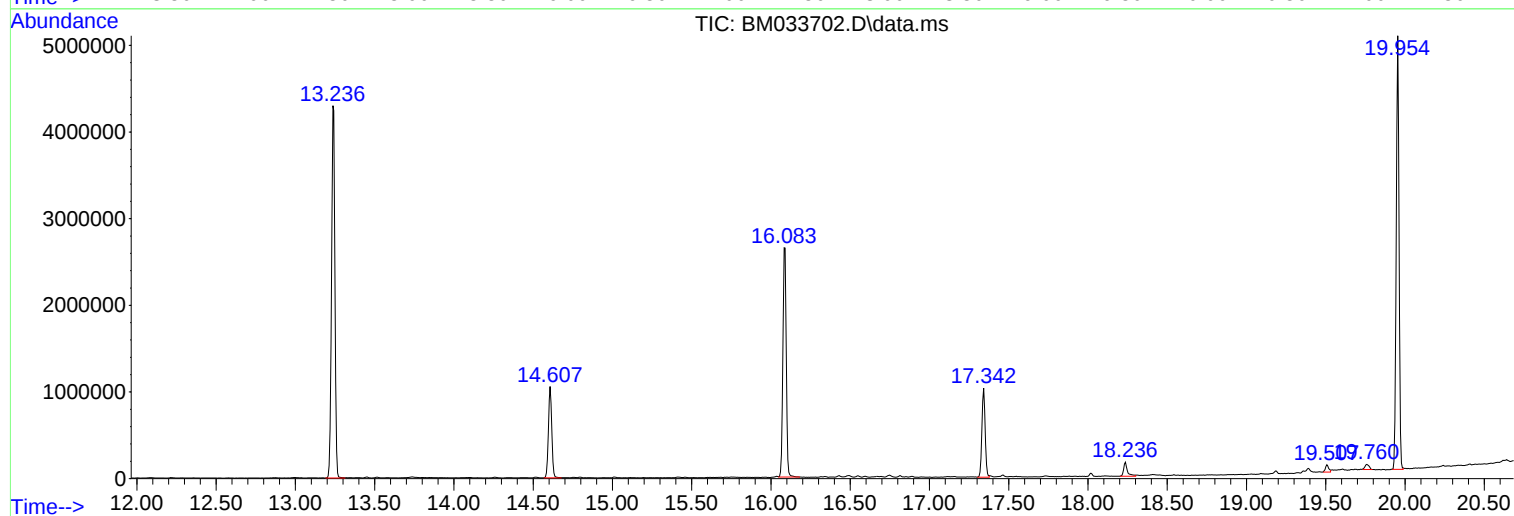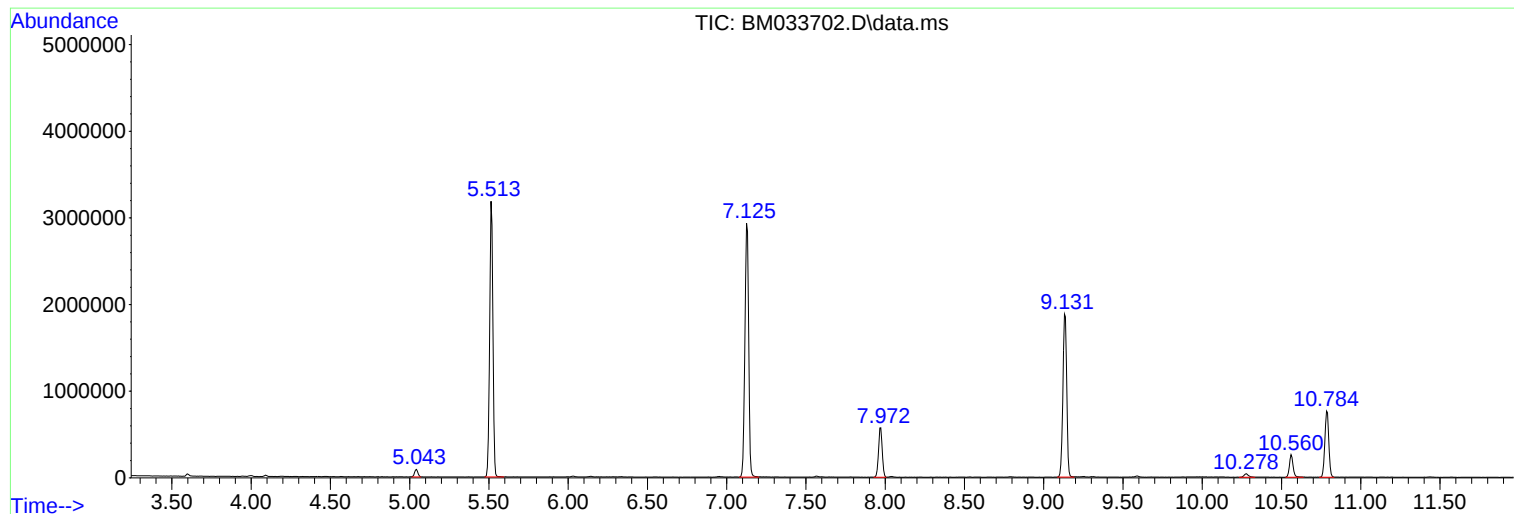

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033702.D
Acq On : 12 Jan 2022 17:11
Operator : CG/JU
Sample : N1099-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033702.D
Acq On : 12 Jan 2022 17:11
Operator : CG/JU
Sample : N1099-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------