

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033703.D
 Acq On : 12 Jan 2022 17:47
 Operator : CG/JU
 Sample : N1099-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-06

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033703.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.043	300	307	313	rBV2	46584	73458	1.15%	0.187%
2	5.513	380	387	396	rBV	3290113	4724746	73.93%	12.027%
3	7.125	653	661	673	rBV	3016810	4921588	77.01%	12.528%
4	7.972	796	805	813	rBV	630209	999473	15.64%	2.544%
5	9.131	994	1002	1010	rBV	1948265	3258836	50.99%	8.295%
6	10.560	1239	1245	1255	rBV	183088	299542	4.69%	0.762%
7	10.783	1275	1283	1293	rBV	821046	1411494	22.09%	3.593%
8	13.236	1693	1700	1711	rBV	4295276	6390712	100.00%	16.267%
9	14.607	1926	1933	1945	rVB	1094172	1627032	25.46%	4.142%
10	16.089	2178	2185	2203	rVB	2458618	3700424	57.90%	9.419%
11	17.342	2391	2398	2409	rBV	1029587	1458068	22.82%	3.711%
12	18.236	2545	2550	2560	rBV	180766	265620	4.16%	0.676%
13	19.506	2762	2766	2775	rBV5	62977	113691	1.78%	0.289%
14	19.953	2836	2842	2848	rBV	5014568	5894010	92.23%	15.003%
15	21.218	3053	3057	3063	rBV	323419	409988	6.42%	1.044%
16	21.500	3101	3105	3113	rBV	1255996	1689280	26.43%	4.300%
17	23.924	3511	3517	3531	rVB2	986972	2047748	32.04%	5.212%




Sum of corrected areas: 39285710

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033703.D
Acq On : 12 Jan 2022 17:47
Operator : CG/JU
Sample : N1099-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

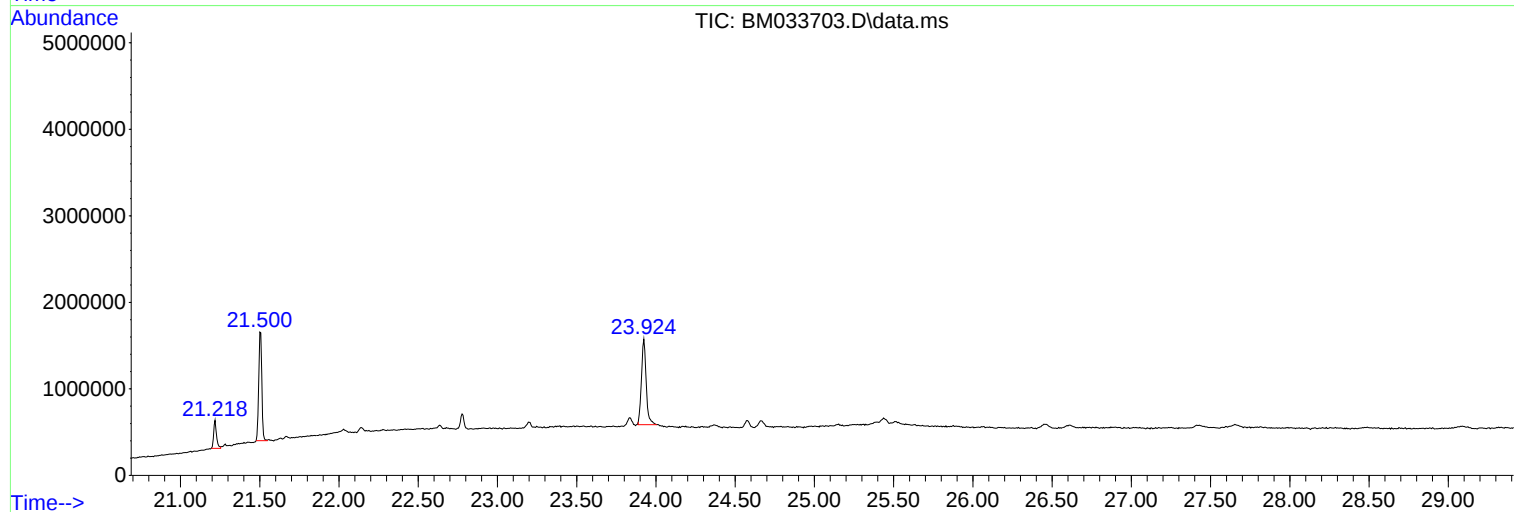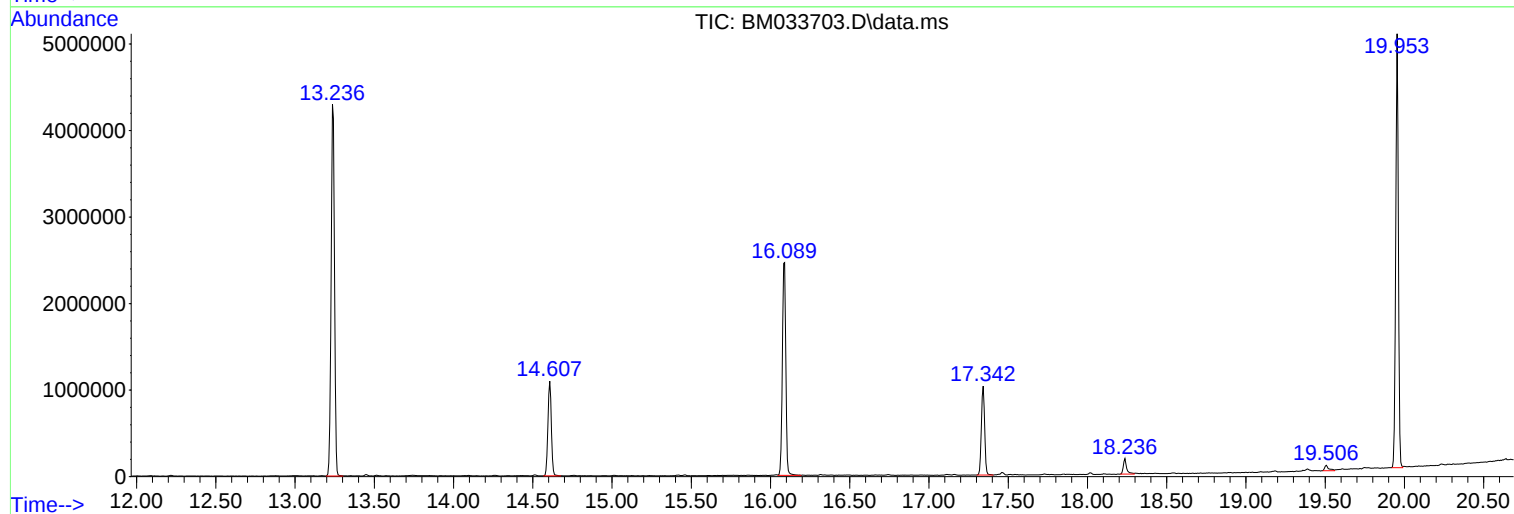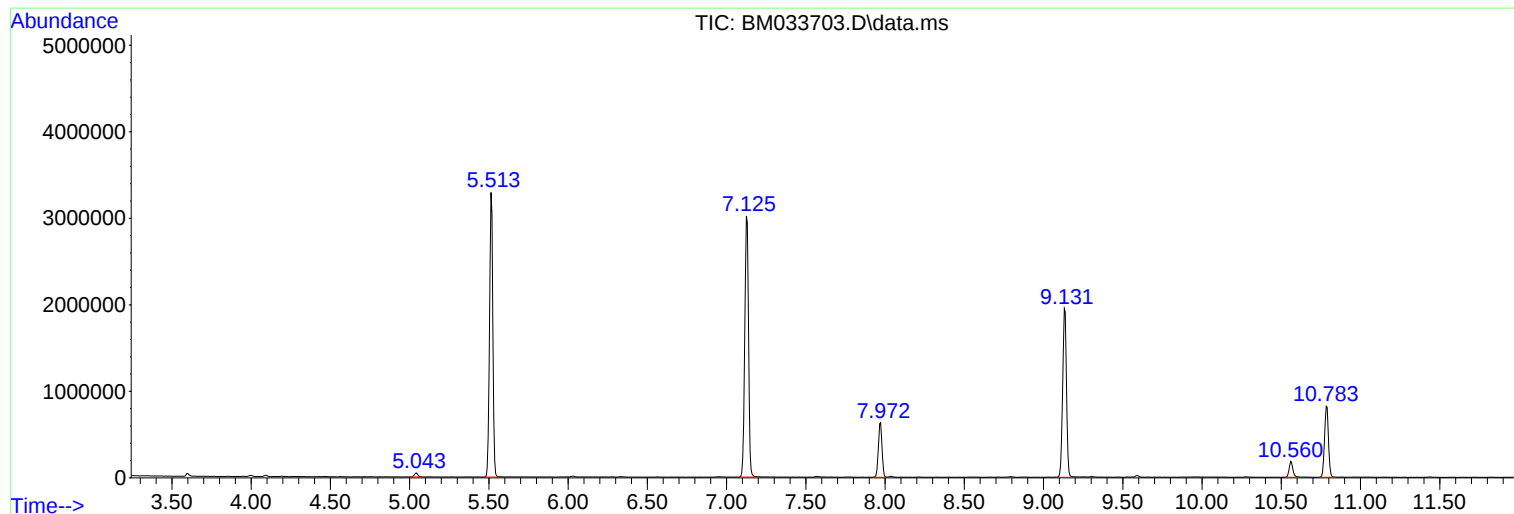

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033703.D
Acq On : 12 Jan 2022 17:47
Operator : CG/JU
Sample : N1099-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033703.D
Acq On : 12 Jan 2022 17:47
Operator : CG/JU
Sample : N1099-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------