

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033704.D
 Acq On : 12 Jan 2022 18:23
 Operator : CG/JU
 Sample : N1099-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.037	301	306	313	rBV2	44394	69806	1.07%	0.175%
2	5.513	380	387	395	rBV	3160437	4514576	69.21%	11.291%
3	7.125	653	661	672	rBV	2957977	4736206	72.61%	11.845%
4	7.966	797	804	812	rBV	713743	1138353	17.45%	2.847%
5	9.131	993	1002	1013	rBV	1920541	3163721	48.50%	7.912%
6	10.560	1238	1245	1256	rBV	254874	421483	6.46%	1.054%
7	10.784	1275	1283	1294	rBV	934610	1587466	24.34%	3.970%
8	13.236	1693	1700	1715	rBV	4417928	6522962	100.00%	16.313%
9	14.607	1926	1933	1947	rBV	1283186	1876143	28.76%	4.692%
10	16.083	2178	2184	2201	rVB	2700931	3798788	58.24%	9.500%
11	17.342	2392	2398	2404	rBV	1209817	1688269	25.88%	4.222%
12	18.236	2544	2550	2559	rBV	158492	253231	3.88%	0.633%
13	19.507	2762	2766	2771	rBV3	51495	84933	1.30%	0.212%
14	19.954	2836	2842	2848	rBV	4898940	5898444	90.43%	14.752%
15	21.218	3053	3057	3064	rBV	313055	411290	6.31%	1.029%
16	21.501	3101	3105	3112	rBV	1344465	1803416	27.65%	4.510%
17	23.924	3511	3517	3528	rVB	989968	2016269	30.91%	5.043%




Sum of corrected areas: 39985356

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033704.D
Acq On : 12 Jan 2022 18:23
Operator : CG/JU
Sample : N1099-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

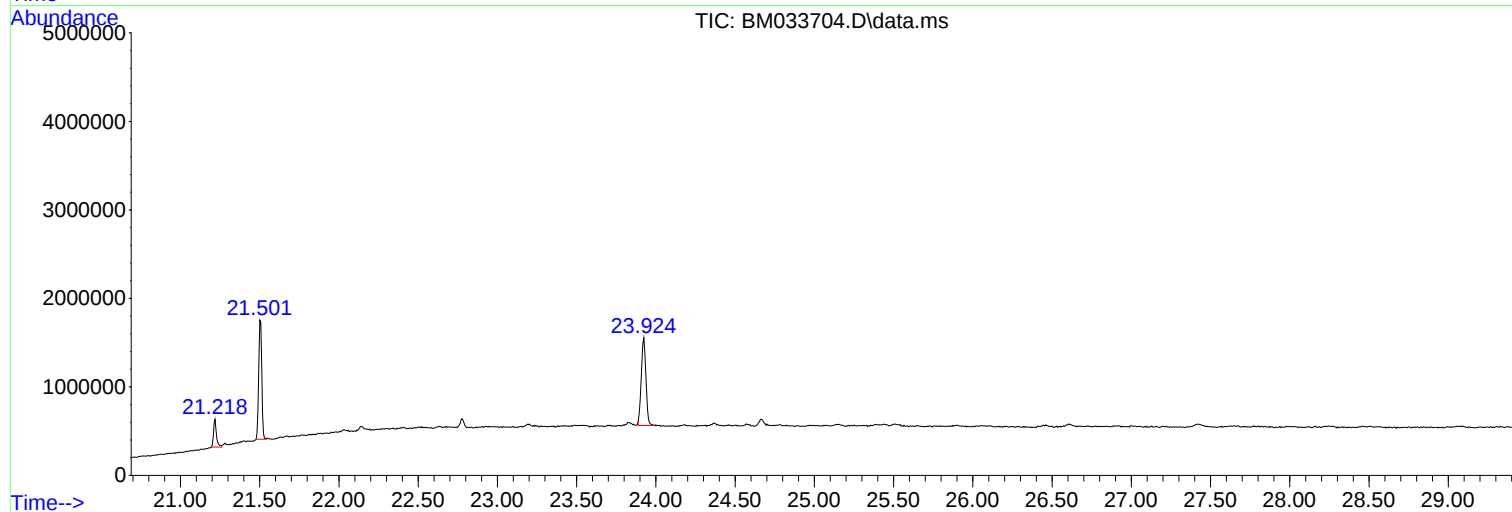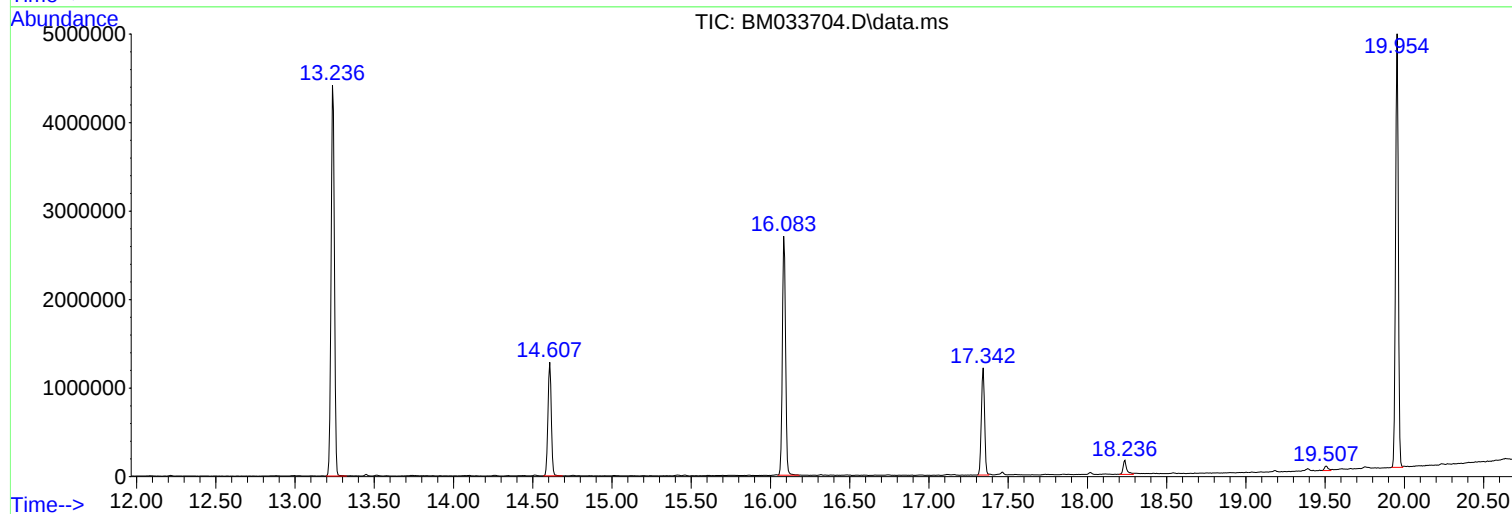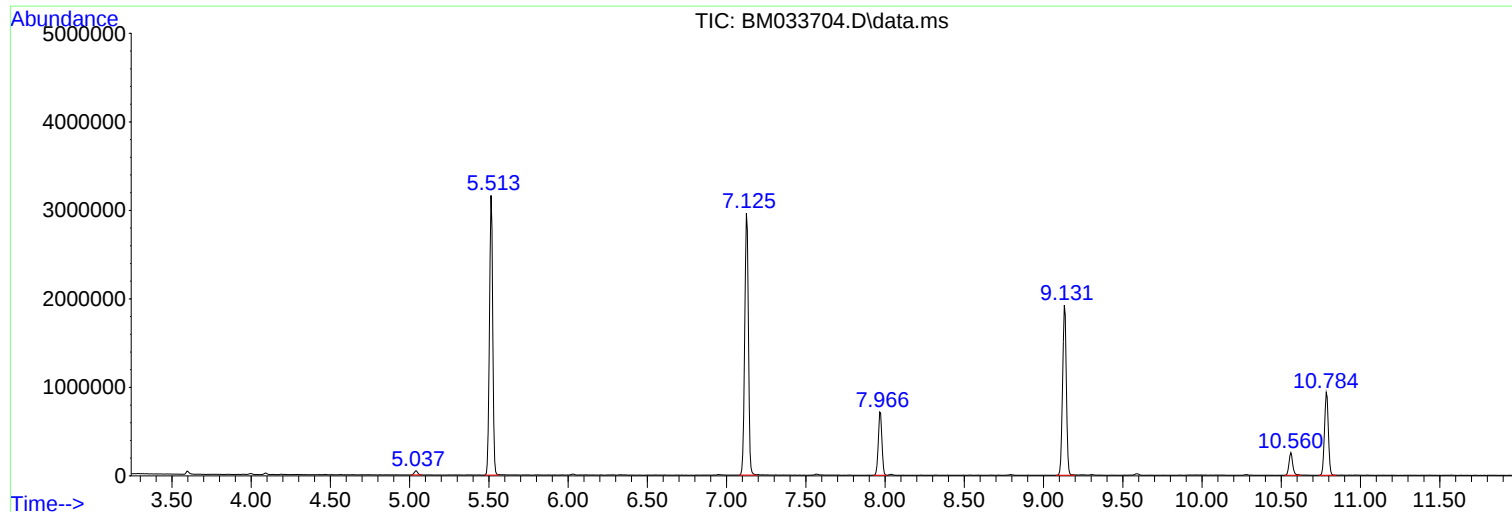

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033704.D
Acq On : 12 Jan 2022 18:23
Operator : CG/JU
Sample : N1099-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033704.D
Acq On : 12 Jan 2022 18:23
Operator : CG/JU
Sample : N1099-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------