

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033705.D
 Acq On : 12 Jan 2022 18:58
 Operator : CG/JU
 Sample : N1099-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-08

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.043	300	307	313	rBV2	51703	80767	1.34%	0.217%
2	5.513	379	387	398	rBV	3075238	4369480	72.68%	11.740%
3	7.125	653	661	672	rBV	2781075	4437585	73.81%	11.923%
4	7.966	796	804	812	rBV	699244	1117517	18.59%	3.003%
5	9.131	994	1002	1012	rBV	1818401	2957302	49.19%	7.946%
6	10.560	1238	1245	1252	rBV	253766	411240	6.84%	1.105%
7	10.783	1275	1283	1296	rBV	886358	1468867	24.43%	3.947%
8	13.236	1693	1700	1710	rBV	3933305	5669016	94.29%	15.232%
9	14.607	1926	1933	1944	rVB	1051559	1549176	25.77%	4.162%
10	16.083	2178	2184	2199	rBV	2243776	3238152	53.86%	8.700%
11	17.342	2391	2398	2407	rBV	1043472	1484957	24.70%	3.990%
12	18.230	2545	2549	2555	rBV	89400	137099	2.28%	0.368%
13	19.506	2762	2766	2769	rBV2	44047	64261	1.07%	0.173%
14	19.953	2836	2842	2849	rBV	4961448	6012338	100.00%	16.154%
15	21.218	3053	3057	3063	rBV	201529	269784	4.49%	0.725%
16	21.500	3101	3105	3111	rBV	1473651	1877968	31.24%	5.046%
17	23.924	3511	3517	3528	rVB2	1015018	2072680	34.47%	5.569%




Sum of corrected areas: 37218189

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033705.D
Acq On : 12 Jan 2022 18:58
Operator : CG/JU
Sample : N1099-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

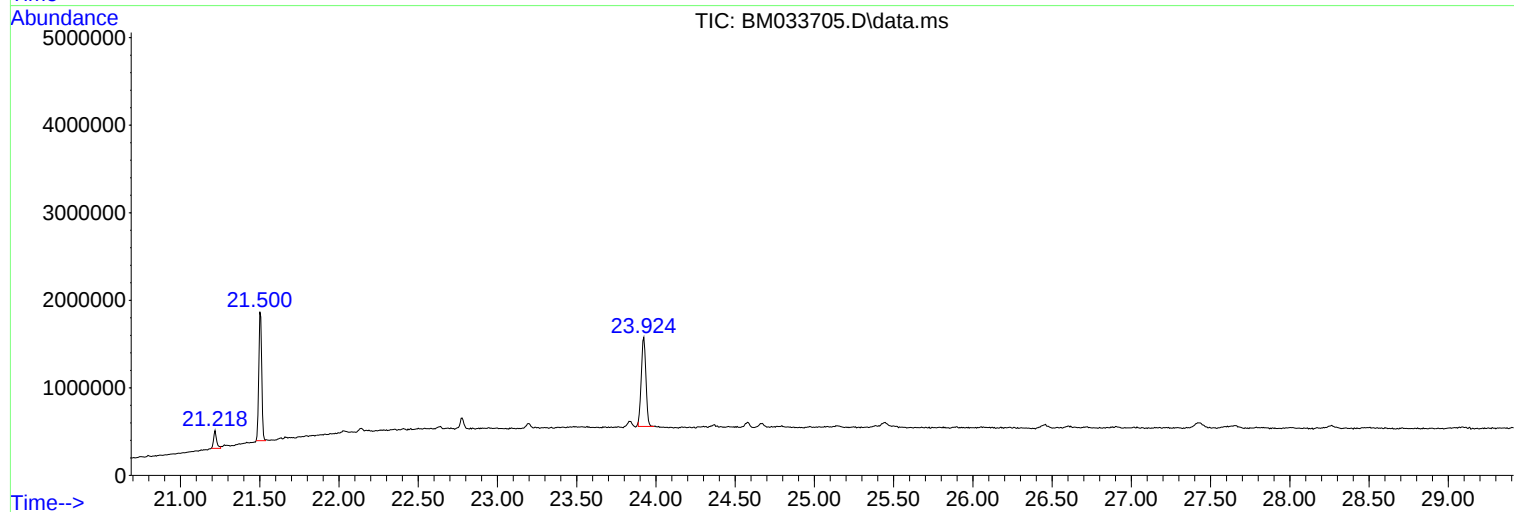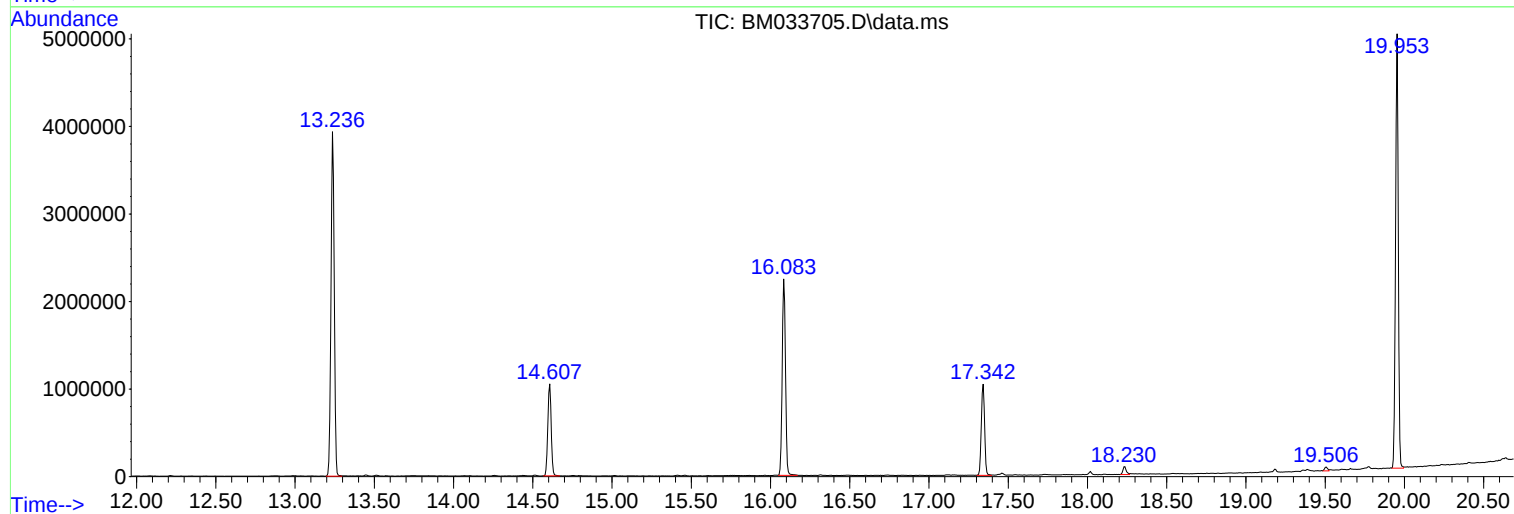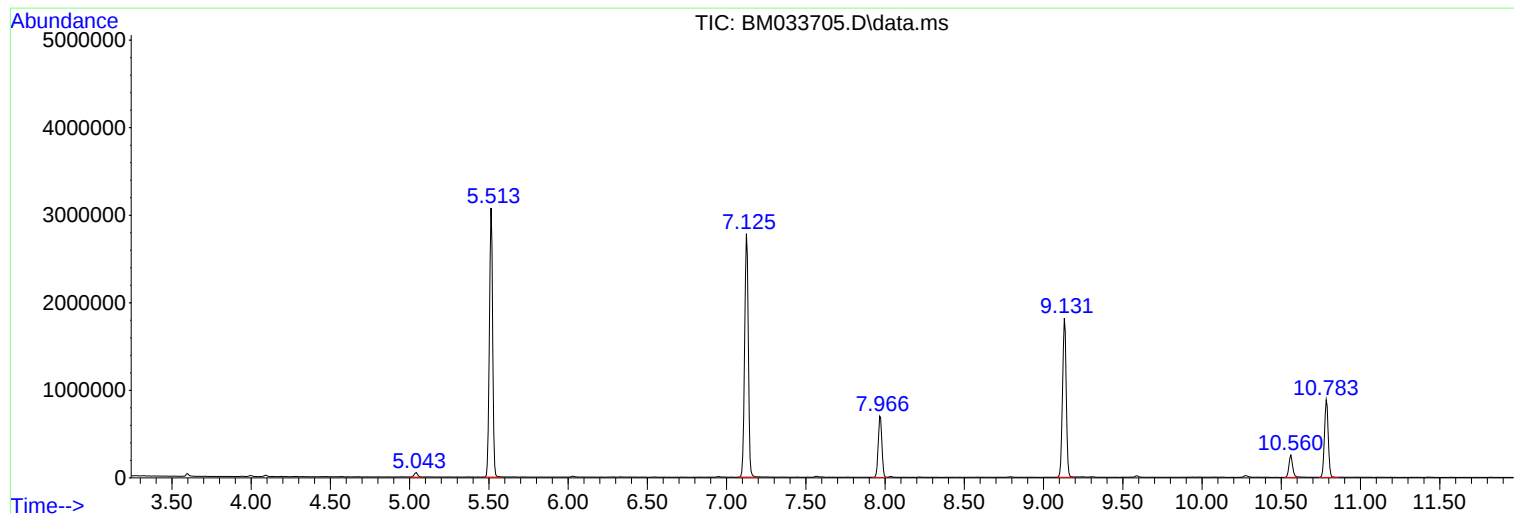

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033705.D
Acq On : 12 Jan 2022 18:58
Operator : CG/JU
Sample : N1099-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033705.D
Acq On : 12 Jan 2022 18:58
Operator : CG/JU
Sample : N1099-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------