

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033706.D
 Acq On : 12 Jan 2022 19:34
 Operator : CG/JU
 Sample : N1099-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.037	301	306	312	rVB2	50081	78871	1.27%	0.206%
2	5.513	380	387	398	rBV	3087911	4412863	71.13%	11.506%
3	7.125	652	661	672	rBV	2862868	4583377	73.88%	11.951%
4	7.966	798	804	811	rBV	712623	1108973	17.87%	2.892%
5	9.131	994	1002	1014	rBV	1870923	3074310	49.55%	8.016%
6	9.742	1099	1106	1117	rBV	50518	87199	1.41%	0.227%
7	10.560	1237	1245	1258	rBV	433797	701083	11.30%	1.828%
8	10.783	1275	1283	1291	rBV	909720	1512698	24.38%	3.944%
9	13.236	1693	1700	1707	rBV	4278264	6204073	100.00%	16.177%
10	14.607	1925	1933	1950	rBV	1112857	1671901	26.95%	4.359%
11	16.083	2178	2184	2198	rVB	2417742	3339454	53.83%	8.707%
12	17.342	2391	2398	2404	rBV	1010576	1456082	23.47%	3.797%
13	18.236	2544	2550	2557	rBV	123436	190066	3.06%	0.496%
14	19.500	2762	2765	2772	rBV3	43566	65752	1.06%	0.171%
15	19.953	2836	2842	2847	rBV	4594309	5722970	92.25%	14.922%
16	21.212	3053	3056	3064	rBV	313176	440409	7.10%	1.148%
17	21.500	3100	3105	3110	rBV	1336553	1753036	28.26%	4.571%
18	23.918	3511	3516	3529	rVB2	949480	1949252	31.42%	5.082%




Sum of corrected areas: 38352369

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033706.D
Acq On : 12 Jan 2022 19:34
Operator : CG/JU
Sample : N1099-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

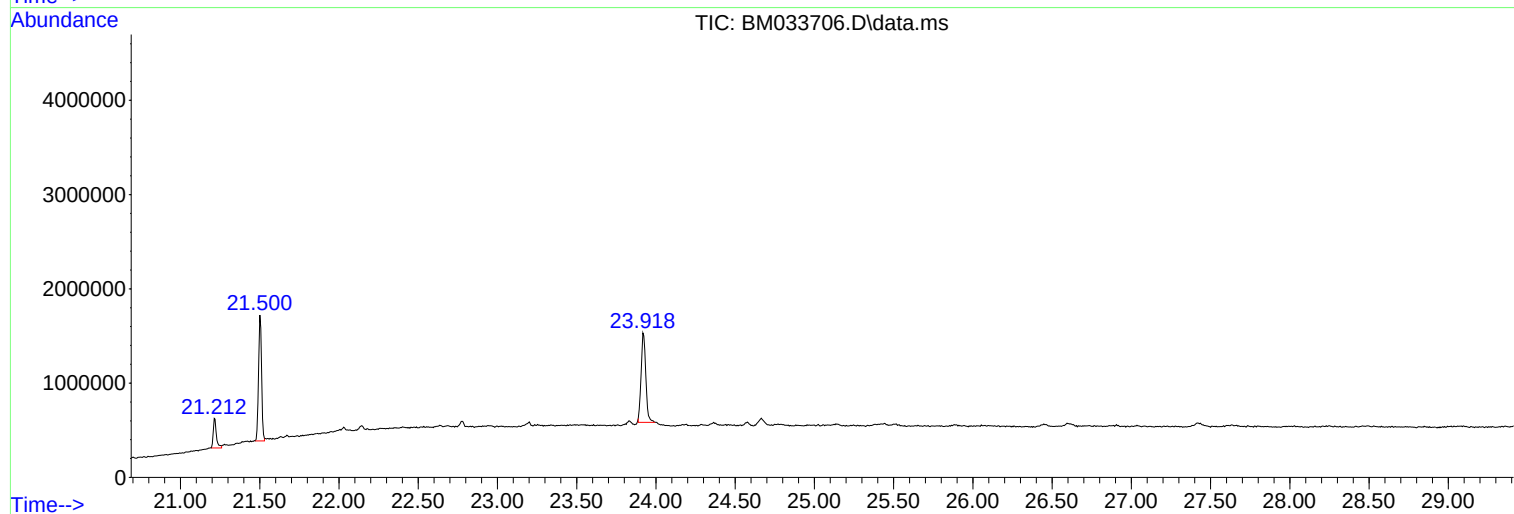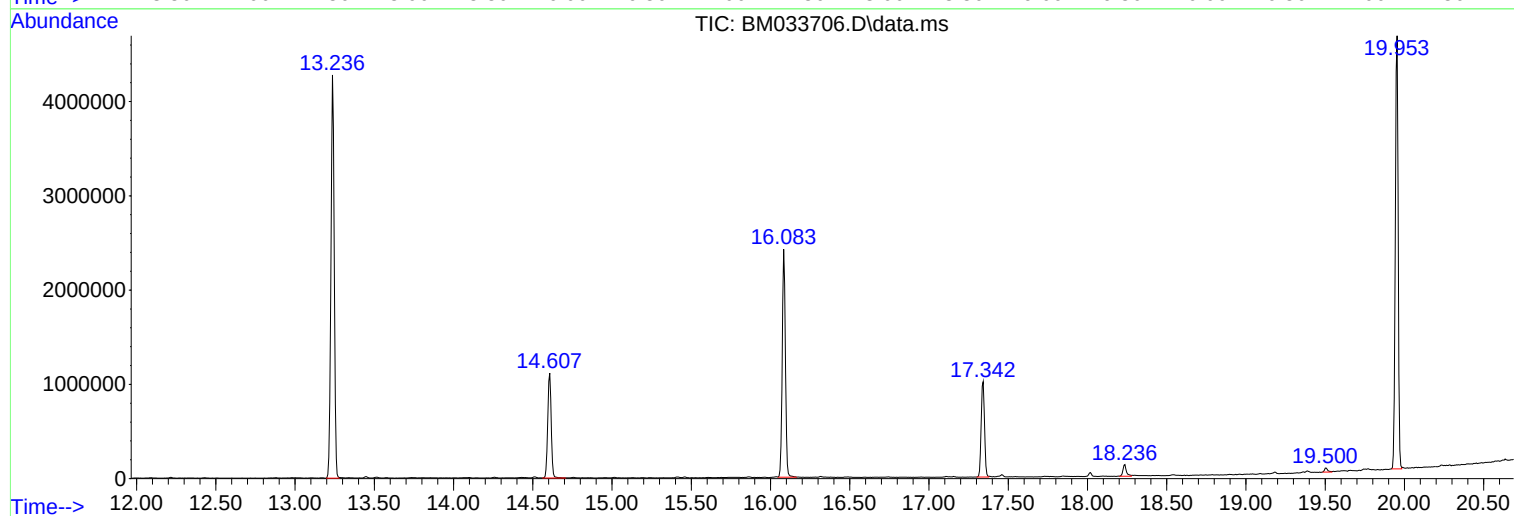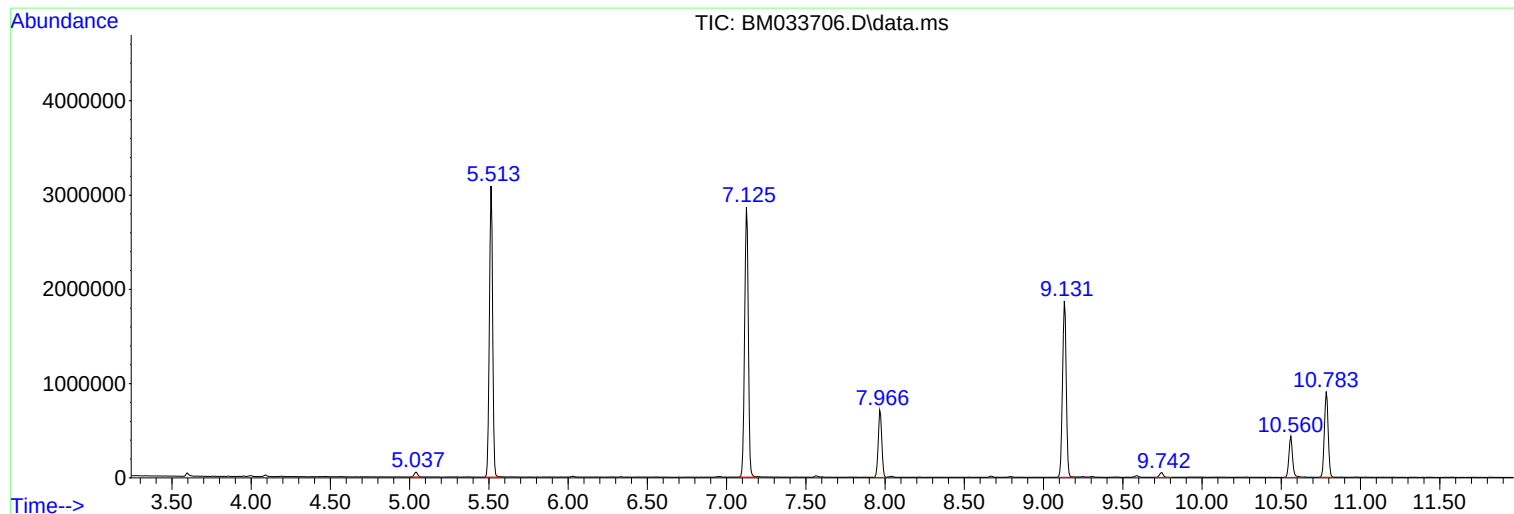

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033706.D
Acq On : 12 Jan 2022 19:34
Operator : CG/JU
Sample : N1099-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033706.D
Acq On : 12 Jan 2022 19:34
Operator : CG/JU
Sample : N1099-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------