

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033707.D
 Acq On : 12 Jan 2022 20:10
 Operator : CG/JU
 Sample : N1099-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.037	300	306	313	rVB2	52206	82702	1.34%	0.235%
2	5.513	379	387	396	rBV	2860219	4052981	65.84%	11.510%
3	7.125	653	661	671	rBV	2570074	4086045	66.37%	11.604%
4	7.966	797	804	812	rBV	632720	984361	15.99%	2.796%
5	9.131	994	1002	1012	rBV	1683043	2741314	44.53%	7.785%
6	10.560	1239	1245	1256	rBV	181929	291851	4.74%	0.829%
7	10.784	1275	1283	1290	rBV	767487	1281683	20.82%	3.640%
8	13.236	1693	1700	1714	rBV	3766292	5375175	87.31%	15.265%
9	14.607	1926	1933	1942	rBV	912845	1386019	22.51%	3.936%
10	16.083	2177	2184	2201	rVB	2239550	3222004	52.34%	9.150%
11	17.342	2390	2398	2404	rBV	944667	1386135	22.52%	3.937%
12	18.230	2544	2549	2556	rBV	90222	135627	2.20%	0.385%
13	19.953	2836	2842	2849	rBV	5280160	6156235	100.00%	17.483%
14	21.218	3053	3057	3063	rBV	270680	359689	5.84%	1.021%
15	21.506	3101	3106	3111	rBV	1311220	1709423	27.77%	4.855%
16	23.924	3511	3517	3528	rVB	934682	1960731	31.85%	5.568%




Sum of corrected areas: 35211975

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033707.D
Acq On : 12 Jan 2022 20:10
Operator : CG/JU
Sample : N1099-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

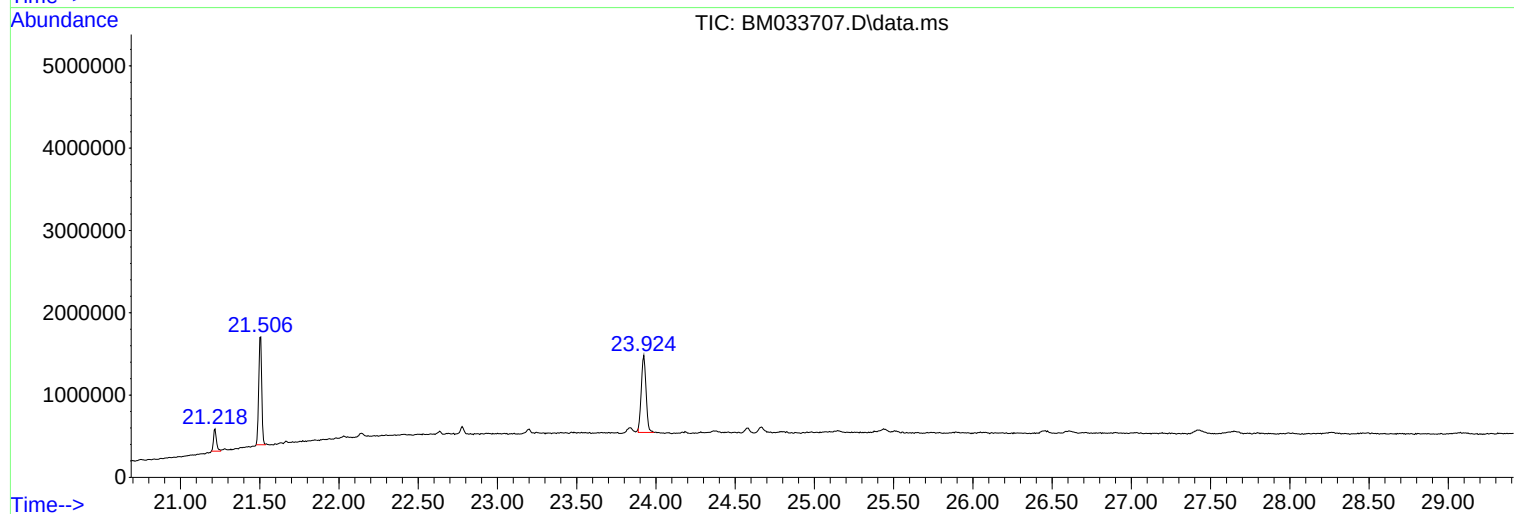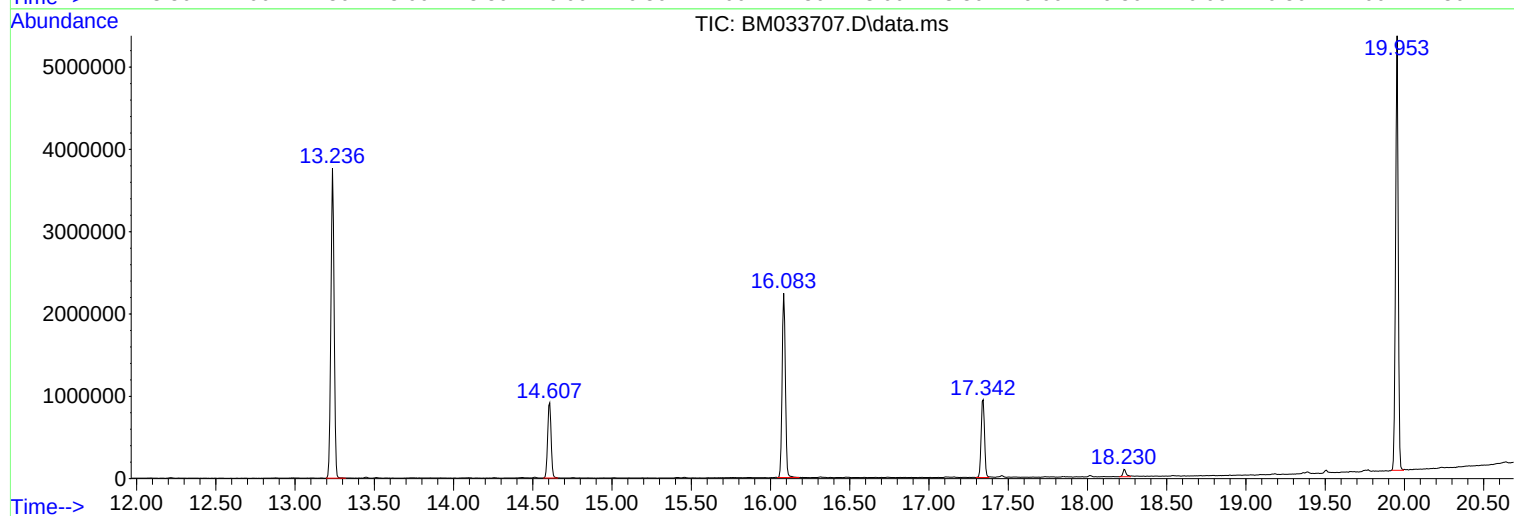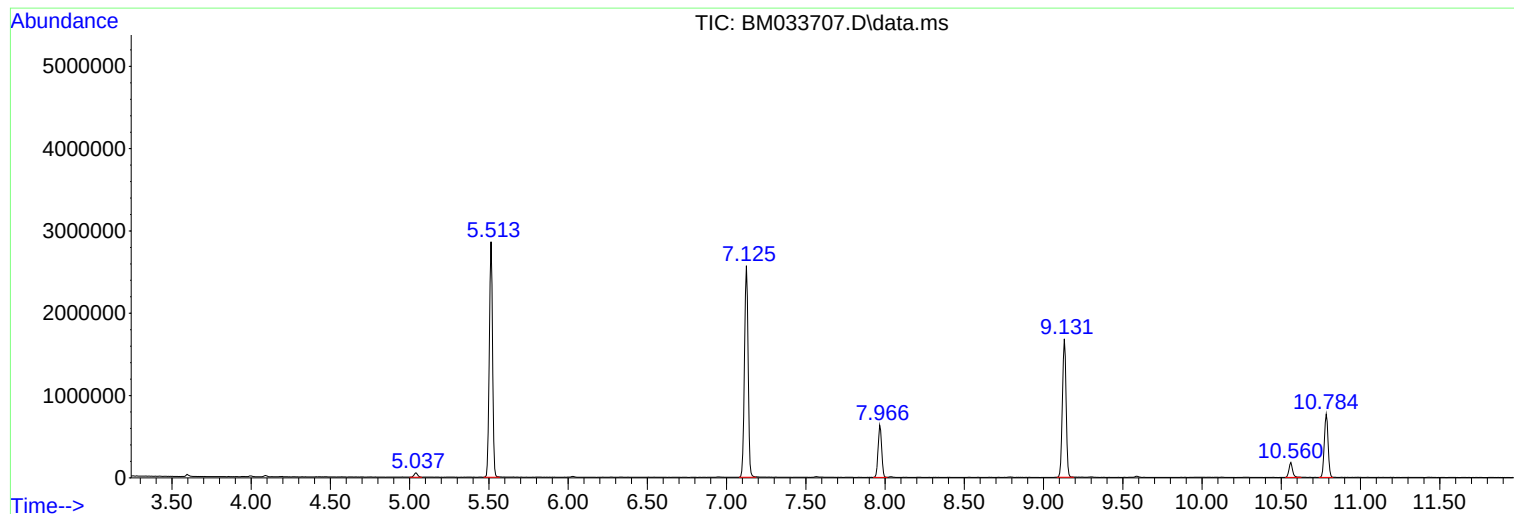

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033707.D
Acq On : 12 Jan 2022 20:10
Operator : CG/JU
Sample : N1099-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
Data File : BM033707.D
Acq On : 12 Jan 2022 20:10
Operator : CG/JU
Sample : N1099-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VACLOT-BACKFILL-TILCON-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------