
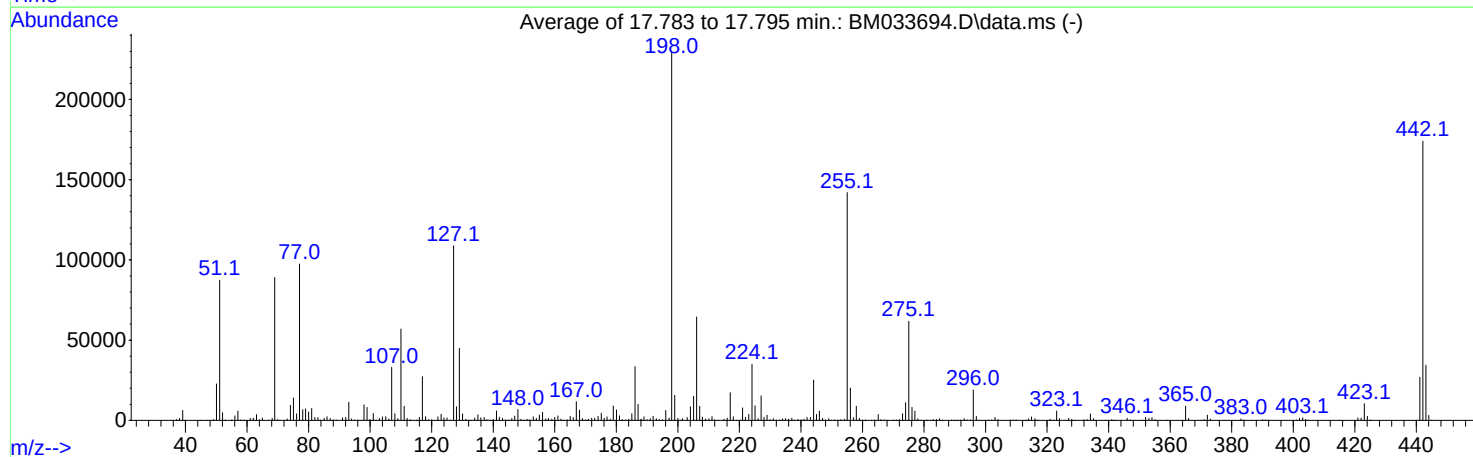


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033694.D
 Acq On : 12 Jan 2022 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 13 07:49:01 2022

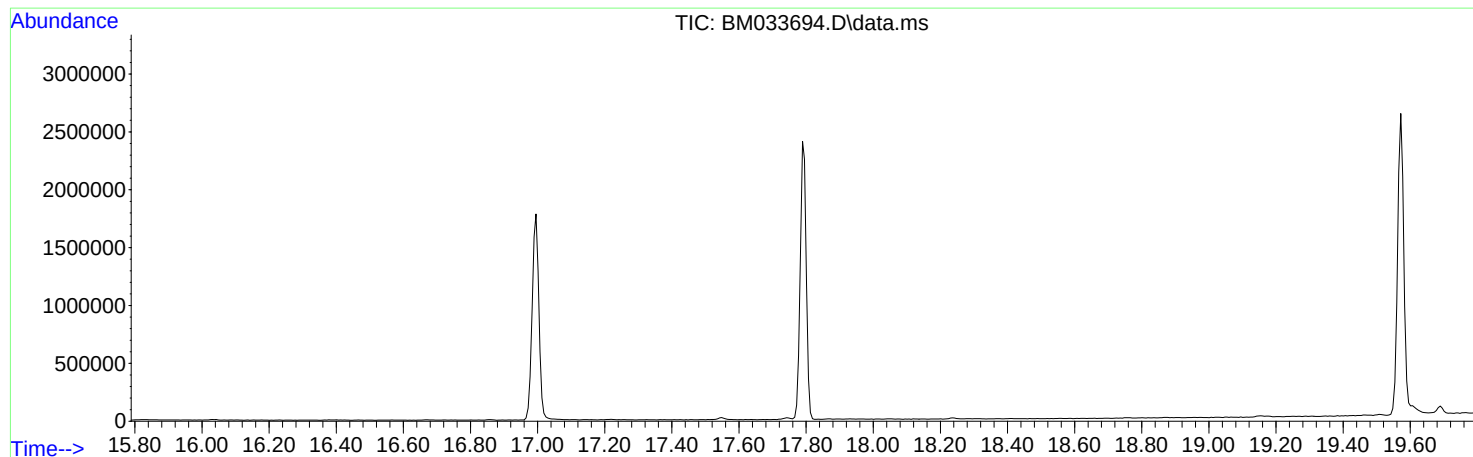




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	87400	PASS
68	69	0.00	2	1.4	1259	PASS
69	198	0.00	100	38.8	89043	PASS
70	69	0.00	2	0.5	488	PASS
127	198	10	80	47.5	108848	PASS
197	198	0.00	2	0.7	1500	PASS
198	198	100	100	100.0	229269	PASS
199	198	5	9	6.8	15650	PASS
275	198	10	60	26.9	61768	PASS
365	198	1	100	3.8	8784	PASS
441	198	0.01	100	11.7	26801	PASS
442	442	50	100	100.0	173987	PASS
443	442	15	24	19.8	34429	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033694.D
 Acq On : 12 Jan 2022 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 13 08:57:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 13 07:49:01 2022
 Response via : Initial Calibration

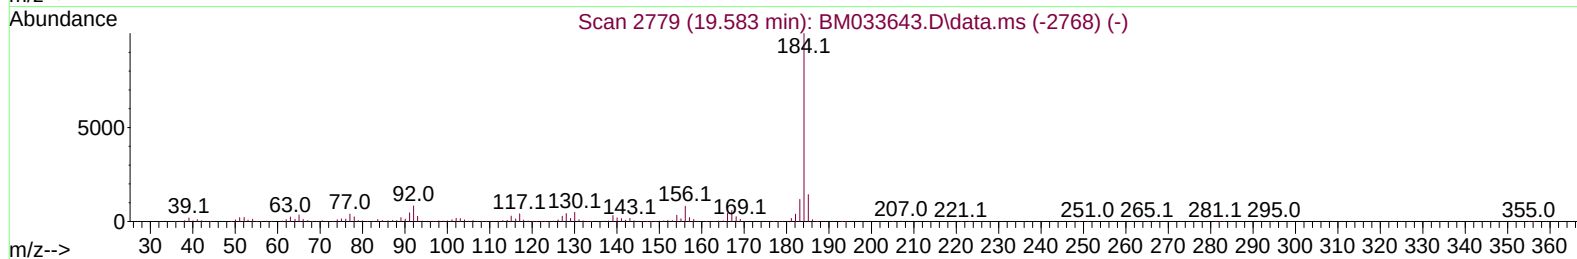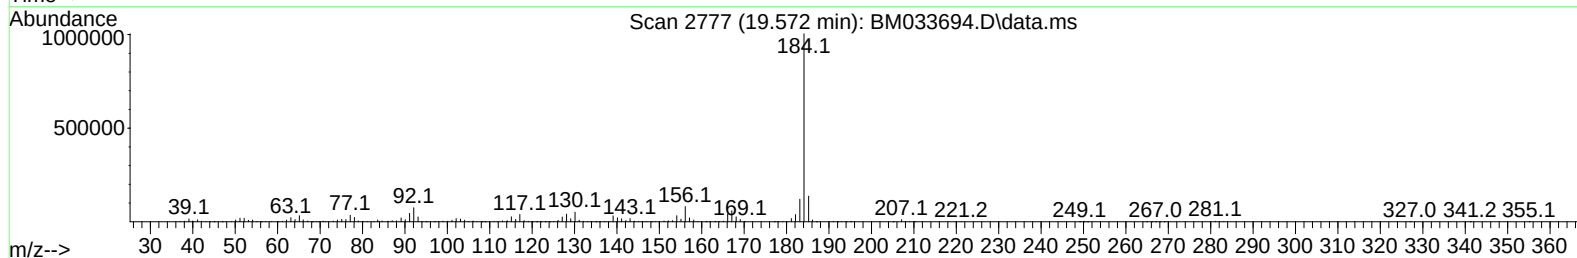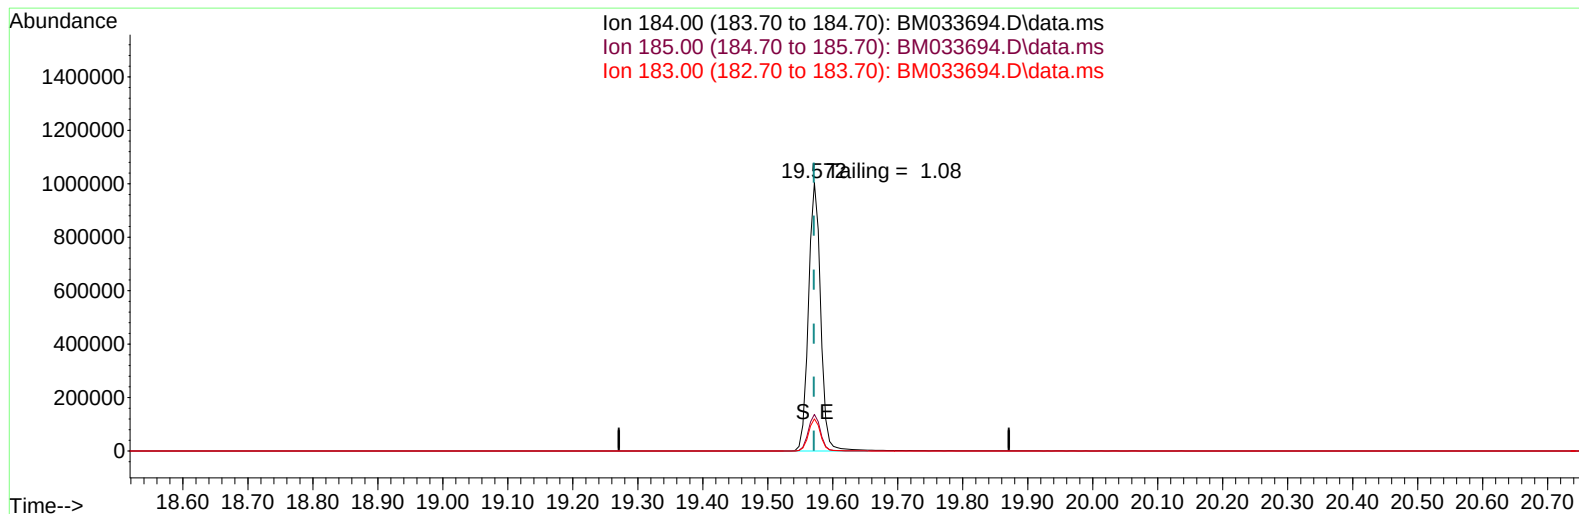

TIC: BM033694.D\data.ms

(77) Benzidine

19.572min (+ 0.000) 51782.18 ng




response 1319460

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.66
183.00	12.10	12.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011222\
 Data File : BM033694.D
 Acq On : 12 Jan 2022 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 13 08:57:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 13 07:49:01 2022
 Response via : Initial Calibration

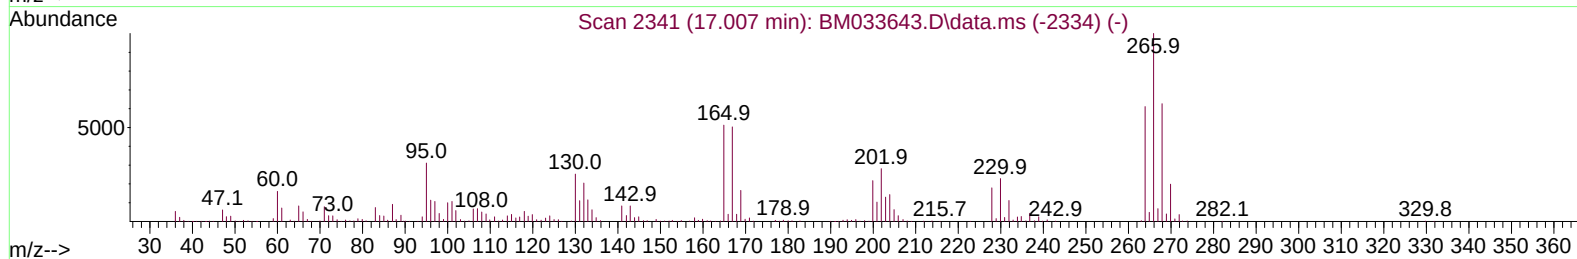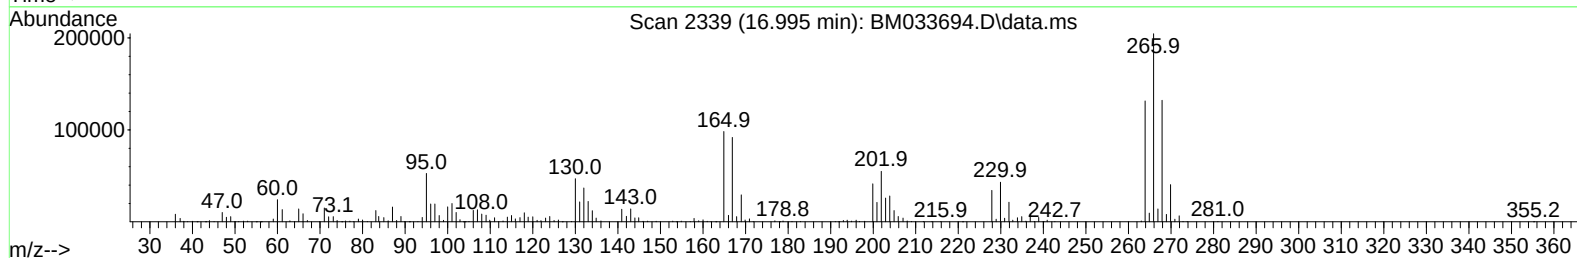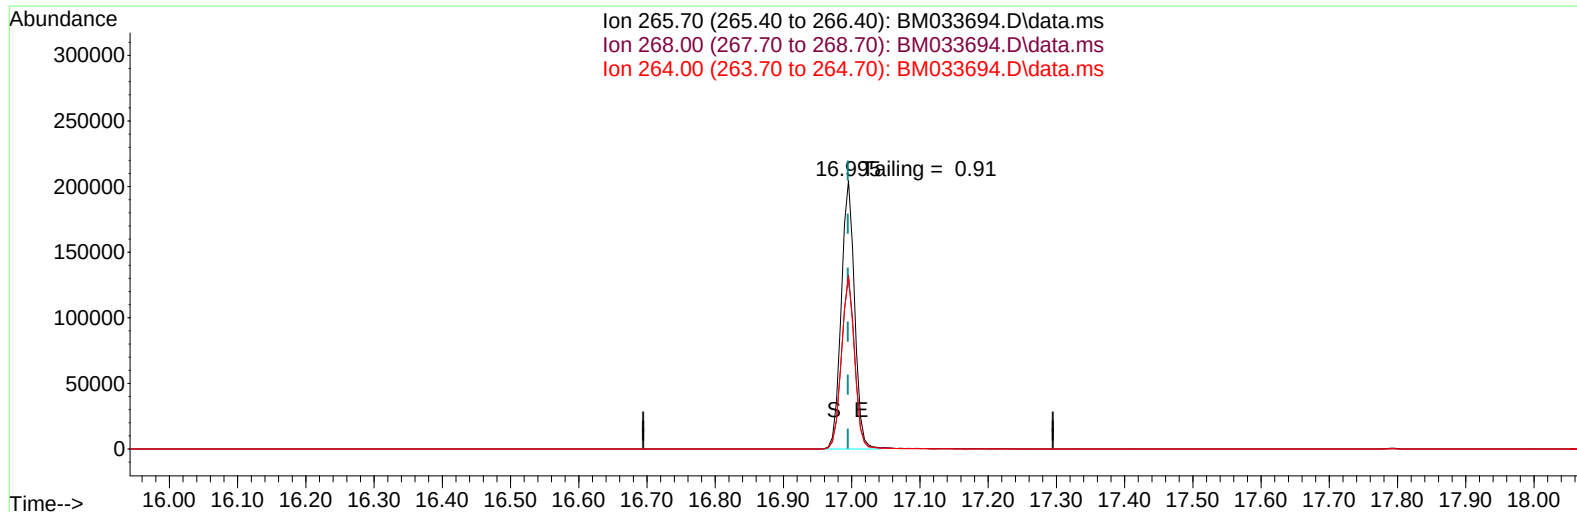

TIC: BM033694.D\data.ms

(70) Pentachlorophenol (C)

16.995min (+ 0.000) 0.00 ng

response 279047

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.61
264.00	61.40	64.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/12/2022	BNA_M	<u>BM033694.D</u>
Compound Name	Response	Retention Time
DDT	664512	20.807
DDD	17554	20.371
DDE	213	19.866
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17767	682279	2.60

Instrument :
BNA_M
ClientSampleId :
DFTPP